

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP102521\
 Data File : BP007706.D
 Acq On : 27 Oct 2021 07:29
 Operator : CG/JU
 Sample : M4303-11
 Misc :
 ALS Vial : 64 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 P014-TW001-02

Integration Parameters: LSCINT.P

Integrator: RTE

Smoother: OFF

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 0.1 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SFAM-EPA-BP102521.M
 Title : SVOA CALIBRATION

Signal : TIC: BP007706.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.370	10	14	23	rVB	50382	66323	0.95%	0.118%
2	3.787	83	85	100	rBV	133960	225409	3.24%	0.401%
3	4.028	121	126	130	rVB	34974	53355	0.77%	0.095%
4	4.117	137	141	147	rVB2	15275	24253	0.35%	0.043%
5	4.211	154	157	162	rVB3	12454	18469	0.27%	0.033%
6	5.046	294	299	304	rVV4	11239	19182	0.28%	0.034%
7	5.111	307	310	316	rVB7	4579	8643	0.12%	0.015%
8	6.317	510	515	520	rBV3	13507	20348	0.29%	0.036%
9	7.093	641	647	656	rVB	211545	337983	4.86%	0.601%
10	7.264	669	676	689	rVB	632372	1032168	14.85%	1.836%
11	7.464	701	710	720	rBV	680812	1074062	15.46%	1.910%
12	7.564	723	727	734	rVB9	5780	12073	0.17%	0.021%
13	7.934	783	790	798	rVV	800882	1279351	18.41%	2.275%
14	7.999	798	801	807	rVB8	4568	7988	0.11%	0.014%
15	8.175	826	831	837	rBV9	4982	11189	0.16%	0.020%
16	8.640	902	910	920	rBV	575113	904833	13.02%	1.609%
17	9.087	979	986	994	rBV	739150	1229038	17.69%	2.186%
18	9.546	1062	1064	1071	rVB8	4623	7920	0.11%	0.014%
19	9.816	1101	1110	1119	rBV	557261	933061	13.43%	1.659%
20	10.358	1193	1202	1212	rBV	900379	1525490	21.95%	2.713%
21	10.516	1224	1229	1238	rBV	60192	111186	1.60%	0.198%
22	10.734	1259	1266	1274	rBV	1085379	1826200	26.28%	3.248%
23	10.869	1281	1289	1302	rBV	715261	1224943	17.63%	2.179%
24	12.328	1531	1537	1545	rVB2	19695	35832	0.52%	0.064%
25	13.193	1678	1684	1687	rBV7	7024	11298	0.16%	0.020%
26	13.981	1811	1818	1830	rBV	1833698	2603372	37.46%	4.630%
27	14.263	1855	1866	1875	rBV	2031283	2960547	42.60%	5.265%
28	14.569	1910	1918	1930	rBV	1785721	2575758	37.06%	4.581%
29	14.757	1945	1950	1963	rBV	204512	322360	4.64%	0.573%
30	14.993	1985	1990	1994	rBV6	12861	19755	0.28%	0.035%
31	15.387	2052	2057	2062	rBV7	7834	13281	0.19%	0.024%
32	15.428	2062	2064	2071	rVB8	3719	7324	0.11%	0.013%
33	15.563	2080	2087	2097	rBV	2754427	3968647	57.11%	7.058%
34	15.681	2100	2107	2115	rBV	856648	1180112	16.98%	2.099%
35	15.804	2124	2128	2132	rVB2	20287	29953	0.43%	0.053%
36	16.010	2160	2163	2169	rVB8	3685	7195	0.10%	0.013%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP102521\
 Data File : BP007706.D
 Acq On : 27 Oct 2021 07:29
 Operator : CG/JU
 Sample : M4303-11
 Misc :
 ALS Vial : 64 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 P014-TW001-02

Integration Parameters: LSCINT.P
 Integrator: RTE
 Smoothing : OFF Filtering: 5
 Sampling : 1 Min Area: 0.1 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SFAM-EPA-BP102521.M
 Title : SVOA CALIBRATION

37	16.257	2198	2205	2209	rBV8	10612	24754	0.36%	0.044%
38	16.998	2326	2331	2334	rBV7	4884	7874	0.11%	0.014%
39	17.104	2346	2349	2356	rVB3	10962	17848	0.26%	0.032%
40	17.328	2379	2387	2396	rBV	2144543	3188424	45.88%	5.671%
41	17.428	2396	2404	2415	rBV	3578585	5292327	76.16%	9.413%
42	17.698	2446	2450	2454	rBV5	4449	7907	0.11%	0.014%
43	18.010	2498	2503	2508	rVB	48374	59258	0.85%	0.105%
44	18.216	2534	2538	2547	rBV	101525	159102	2.29%	0.283%
45	18.522	2585	2590	2598	rBV3	20937	46374	0.67%	0.082%
46	19.239	2707	2712	2716	rBV	57061	83719	1.20%	0.149%
47	19.304	2719	2723	2726	rBV2	55848	73499	1.06%	0.131%
48	19.451	2744	2748	2755	rBV3	65116	107734	1.55%	0.192%
49	19.598	2770	2773	2777	rBV5	18868	25734	0.37%	0.046%
50	19.657	2777	2783	2793	rBV	4716621	6584188	94.74%	11.710%
51	21.133	3031	3034	3040	rBV4	54896	89666	1.29%	0.159%
52	21.416	3077	3082	3087	rBV	2926962	3823817	55.02%	6.801%
53	23.704	3463	3471	3480	rBV2	3392535	6949382	100.00%	12.360%
54	23.863	3491	3498	3507	rVB2	1930580	3995971	57.50%	7.107%




Sum of corrected areas: 56226479

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP102521\
Data File : BP007706.D
Acq On : 27 Oct 2021 07:29
Operator : CG/JU
Sample : M4303-11
Misc :
ALS Vial : 64 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
P014-TW001-02

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SFAM-EPA-BP102521.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

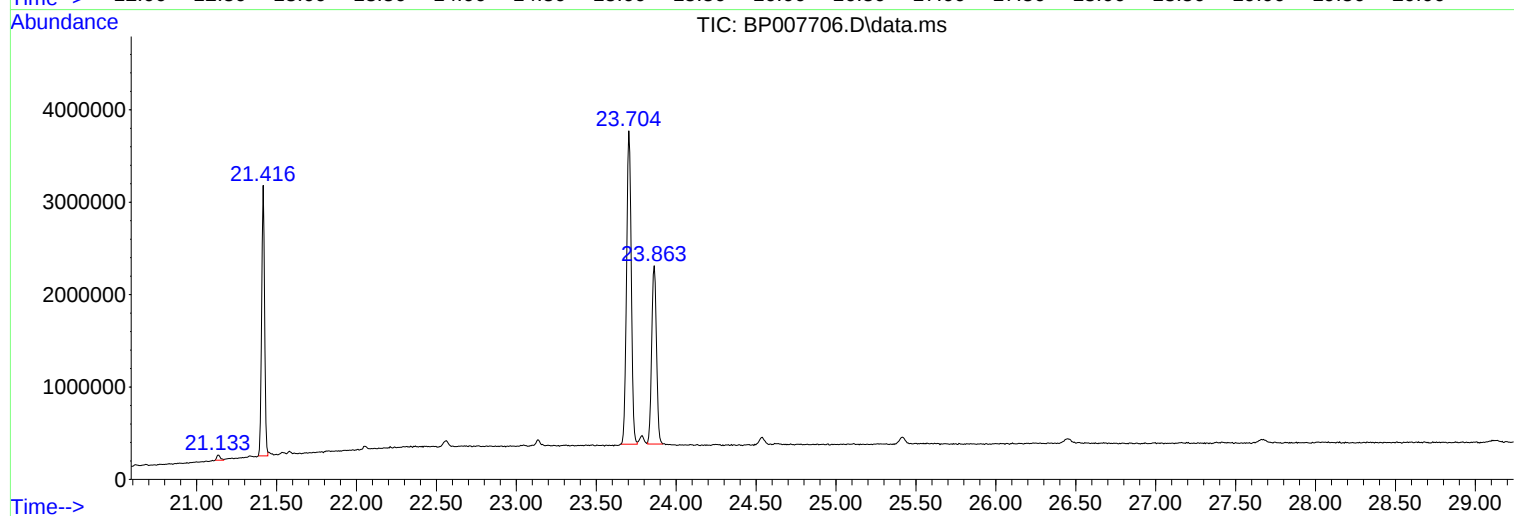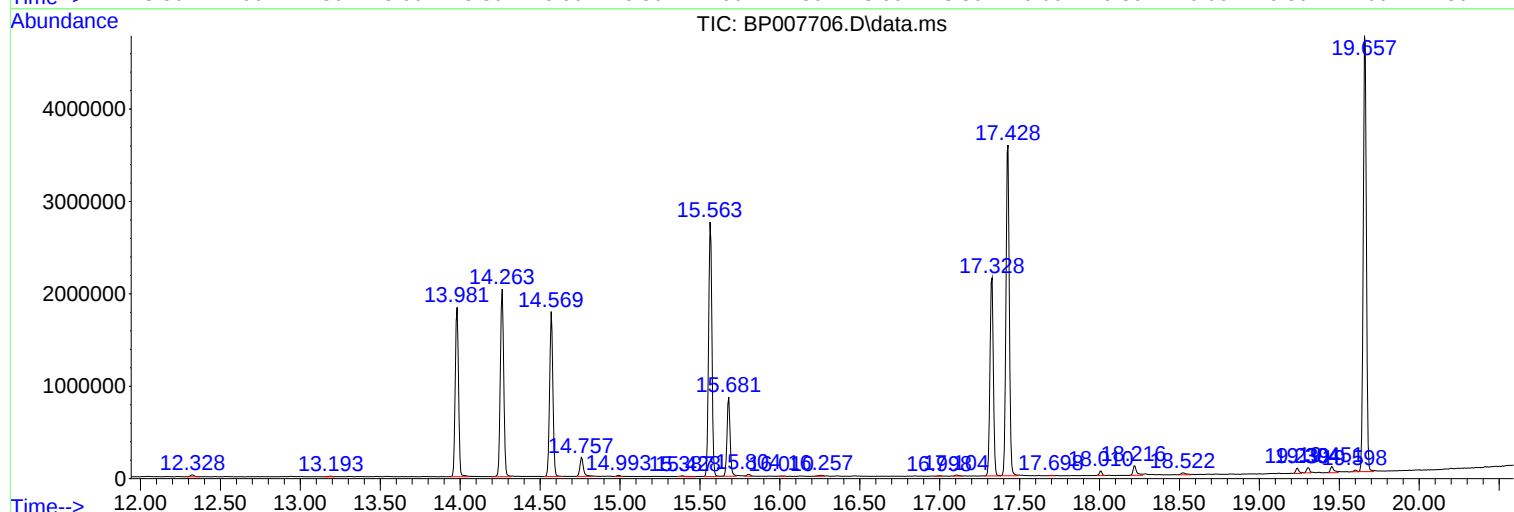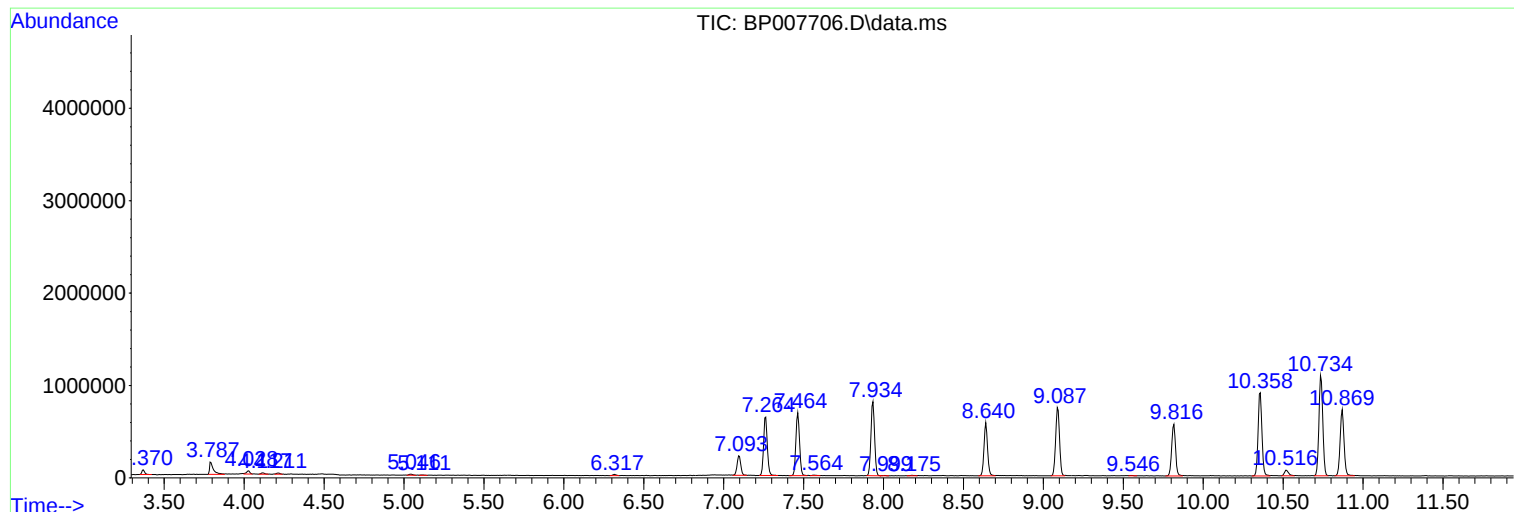

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP102521\
Data File : BP007706.D
Acq On : 27 Oct 2021 07:29
Operator : CG/JU
Sample : M4303-11
Misc :
ALS Vial : 64 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
P014-TW001-02

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SFAM-EPA-BP102521.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP102521\
Data File : BP007706.D
Acq On : 27 Oct 2021 07:29
Operator : CG/JU
Sample : M4303-11
Misc :
ALS Vial : 64 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
P014-TW001-02

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SFAM-EPA-BP102521.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
