

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP102521\
 Data File : BP007707.D
 Acq On : 27 Oct 2021 08:03
 Operator : CG/JU
 Sample : M4303-12
 Misc :
 ALS Vial : 65 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 P015-TW001-02

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SFAM-EPA-BP102521.M
 Title : SVOA CALIBRATION

Signal : TIC: BP007707.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.370	10	14	20	rVB	47867	62583	1.03%	0.118%
2	3.787	83	85	96	rBV	201510	315475	5.17%	0.596%
3	4.023	121	125	133	rVB	29465	46299	0.76%	0.087%
4	4.117	138	141	148	rVB	15757	25005	0.41%	0.047%
5	4.217	153	158	163	rBV5	13177	20726	0.34%	0.039%
6	5.034	295	297	304	rVB7	6963	9086	0.15%	0.017%
7	6.317	509	515	521	rBV3	9425	16298	0.27%	0.031%
8	7.093	642	647	654	rBV	180597	280031	4.59%	0.529%
9	7.258	669	675	686	rBV	584394	957056	15.70%	1.809%
10	7.464	703	710	722	rBV	618707	975422	16.00%	1.843%
11	7.569	722	728	733	rVB7	5872	11558	0.19%	0.022%
12	7.934	782	790	797	rBV	837909	1308228	21.46%	2.472%
13	8.640	902	910	922	rBV	514797	828581	13.59%	1.566%
14	9.087	979	986	1000	rBV	697965	1153482	18.92%	2.180%
15	9.546	1062	1064	1069	rVB6	5056	7389	0.12%	0.014%
16	9.816	1101	1110	1125	rBV	524590	872622	14.31%	1.649%
17	10.358	1192	1202	1217	rBV	827714	1421492	23.32%	2.686%
18	10.734	1259	1266	1277	rVB	1101823	1875849	30.77%	3.545%
19	10.869	1280	1289	1300	rBV	822732	1402344	23.00%	2.650%
20	12.046	1483	1489	1493	rBV9	4722	8840	0.14%	0.017%
21	12.322	1531	1536	1544	rVB2	17436	33805	0.55%	0.064%
22	12.940	1637	1641	1648	rBV8	7912	16504	0.27%	0.031%
23	13.193	1674	1684	1689	rVB8	8635	17024	0.28%	0.032%
24	13.540	1739	1743	1750	rVB7	5605	10551	0.17%	0.020%
25	13.981	1809	1818	1834	rBV	1810878	2552940	41.87%	4.824%
26	14.263	1856	1866	1880	rBV	1945932	2864507	46.98%	5.413%
27	14.569	1911	1918	1926	rBV	1727333	2601729	42.67%	4.916%
28	14.757	1942	1950	1958	rBV	155134	257539	4.22%	0.487%
29	14.987	1985	1989	1993	rBV6	10594	13749	0.23%	0.026%
30	15.387	2052	2057	2061	rBV7	5372	11228	0.18%	0.021%
31	15.563	2080	2087	2100	rBV	2676073	3899494	63.96%	7.369%
32	15.681	2100	2107	2122	rVV	743405	1031686	16.92%	1.950%
33	15.804	2123	2128	2133	rVB4	20462	35761	0.59%	0.068%
34	16.263	2199	2206	2210	rBV6	9864	21433	0.35%	0.041%
35	17.004	2327	2332	2337	rBV9	5779	9430	0.15%	0.018%
36	17.110	2342	2350	2354	rBV5	14270	28090	0.46%	0.053%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP102521\
 Data File : BP007707.D
 Acq On : 27 Oct 2021 08:03
 Operator : CG/JU
 Sample : M4303-12
 Misc :
 ALS Vial : 65 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 P015-TW001-02

Integration Parameters: LSCINT.P
 Integrator: RTE
 Smoothing : OFF Filtering: 5
 Sampling : 1 Min Area: 0.1 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SFAM-EPA-BP102521.M
 Title : SVOA CALIBRATION

37	17.322	2380	2386	2396	rBV	2153571	3200988	52.50%	6.049%
38	17.422	2397	2403	2416	rVV2	3205208	4741574	77.77%	8.960%
39	17.516	2416	2419	2427	rVB10	13631	26635	0.44%	0.050%
40	17.704	2447	2451	2454	rBV4	4785	6741	0.11%	0.013%
41	18.004	2497	2502	2506	rBV8	13418	19761	0.32%	0.037%
42	18.222	2532	2539	2544	rBV10	16177	30134	0.49%	0.057%
43	18.292	2548	2551	2553	rVB2	5653	7045	0.12%	0.013%
44	19.239	2708	2712	2719	rBV2	45497	67037	1.10%	0.127%
45	19.304	2719	2723	2728	rBV	49290	71924	1.18%	0.136%
46	19.598	2771	2773	2777	rVB5	15418	17927	0.29%	0.034%
47	19.663	2778	2784	2791	rBV	4200669	5772546	94.68%	10.908%
48	21.416	3077	3082	3095	rBV	2986988	3833453	62.88%	7.244%
49	23.704	3464	3471	3481	rBV2	3099456	6096715	100.00%	11.521%
50	23.863	3491	3498	3512	rVB2	1904713	4023273	65.99%	7.603%


Sum of corrected areas: 52919589

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP102521\
Data File : BP007707.D
Acq On : 27 Oct 2021 08:03
Operator : CG/JU
Sample : M4303-12
Misc :
ALS Vial : 65 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
P015-TW001-02

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SFAM-EPA-BP102521.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

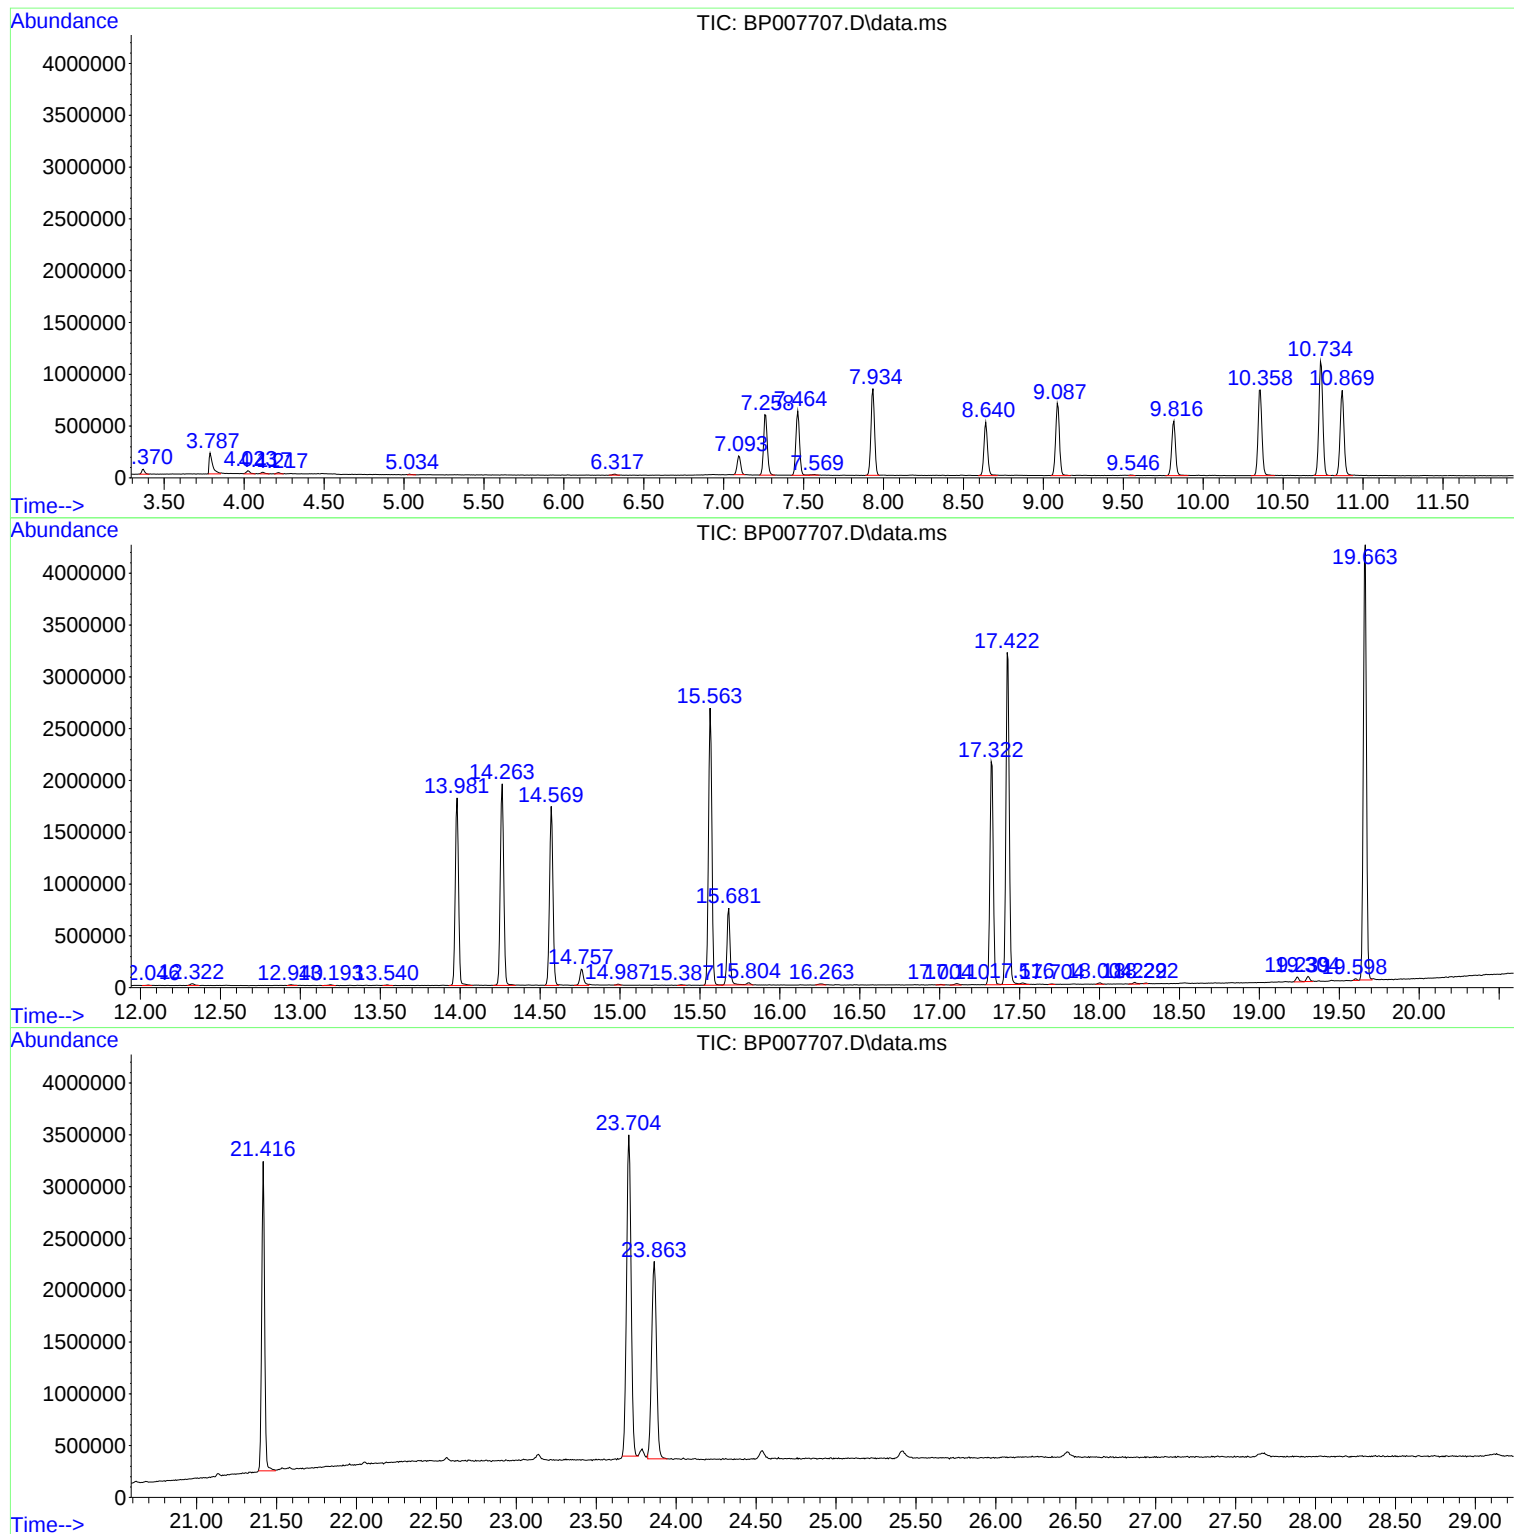

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP102521\
Data File : BP007707.D
Acq On : 27 Oct 2021 08:03
Operator : CG/JU
Sample : M4303-12
Misc :
ALS Vial : 65 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
P015-TW001-02

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SFAM-EPA-BP102521.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP102521\
Data File : BP007707.D
Acq On : 27 Oct 2021 08:03
Operator : CG/JU
Sample : M4303-12
Misc :
ALS Vial : 65 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
P015-TW001-02

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SFAM-EPA-BP102521.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
