

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP102521\
 Data File : BP007708.D
 Acq On : 27 Oct 2021 08:37
 Operator : CG/JU
 Sample : M4303-13
 Misc :
 ALS Vial : 66 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 P018-TW001-02

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SFAM-EPA-BP102521.M
 Title : SVOA CALIBRATION

Signal : TIC: BP007708.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.370	10	14	20	rBV	47881	63899	0.96%	0.126%
2	3.793	83	86	97	rBV	107489	185453	2.79%	0.365%
3	4.022	121	125	130	rVB	33277	50256	0.75%	0.099%
4	4.117	137	141	147	rVB	14569	18793	0.28%	0.037%
5	4.211	153	157	163	rVB4	16849	22666	0.34%	0.045%
6	5.040	294	298	304	rVB3	6161	11015	0.17%	0.022%
7	6.316	510	515	521	rBV3	11769	19747	0.30%	0.039%
8	7.093	642	647	656	rVB	195556	317194	4.76%	0.625%
9	7.263	667	676	685	rBV	664929	1088362	16.35%	2.144%
10	7.463	702	710	719	rBV	706826	1101401	16.54%	2.170%
11	7.934	780	790	798	rBV	602838	970564	14.58%	1.912%
12	8.640	903	910	920	rBV	556866	875984	13.16%	1.726%
13	9.087	976	986	997	rBV	784504	1304834	19.60%	2.571%
14	9.546	1061	1064	1070	rVB8	5445	7585	0.11%	0.015%
15	9.816	1102	1110	1125	rBV	593875	981827	14.75%	1.934%
16	10.357	1193	1202	1218	rBV	930947	1574064	23.64%	3.101%
17	10.734	1258	1266	1274	rBV	831275	1381573	20.75%	2.722%
18	10.869	1281	1289	1303	rBV	794819	1399180	21.01%	2.757%
19	11.393	1376	1378	1384	rVB6	4811	6760	0.10%	0.013%
20	12.328	1529	1537	1540	rBV2	20555	36154	0.54%	0.071%
21	12.363	1540	1543	1552	rVB8	4603	10754	0.16%	0.021%
22	13.540	1740	1743	1753	rVB10	6108	11231	0.17%	0.022%
23	13.981	1808	1818	1824	rBV	1926361	2662172	39.98%	5.245%
24	14.263	1856	1866	1874	rBV	2053568	3068770	46.09%	6.046%
25	14.569	1911	1918	1929	rBV	1331502	1946581	29.24%	3.835%
26	14.757	1945	1950	1958	rBV	167447	264667	3.97%	0.521%
27	14.987	1983	1989	1994	rBV8	12851	18164	0.27%	0.036%
28	15.563	2080	2087	2097	rBV	2817529	4077830	61.24%	8.034%
29	15.681	2100	2107	2118	rBV	795869	1117983	16.79%	2.203%
30	15.804	2124	2128	2135	rVB2	22489	33747	0.51%	0.066%
31	16.245	2198	2203	2204	rBV5	6561	9113	0.14%	0.018%
32	17.110	2345	2350	2353	rBV5	8636	15300	0.23%	0.030%
33	17.322	2380	2386	2397	rBV	1586255	2322143	34.88%	4.575%
34	17.428	2397	2404	2417	rBV	3381494	4999258	75.08%	9.849%
35	17.998	2497	2501	2507	rBV9	7766	11664	0.18%	0.023%
36	18.216	2533	2538	2546	rBV10	19155	35382	0.53%	0.070%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP102521\
 Data File : BP007708.D
 Acq On : 27 Oct 2021 08:37
 Operator : CG/JU
 Sample : M4303-13
 Misc :
 ALS Vial : 66 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 P018-TW001-02

Integration Parameters: LSCINT.P
 Integrator: RTE
 Smoothing : OFF Filtering: 5
 Sampling : 1 Min Area: 0.1 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SFAM-EPA-BP102521.M
 Title : SVOA CALIBRATION

37	18.281	2547	2549	2554	rVB2	7907	10737	0.16%	0.021%
38	19.239	2707	2712	2718	rBV4	47757	73873	1.11%	0.146%
39	19.304	2719	2723	2729	rVV	51532	69659	1.05%	0.137%
40	19.598	2771	2773	2777	rVB5	14634	13915	0.21%	0.027%
41	19.657	2778	2783	2794	rVV	4413274	6116232	91.86%	12.050%
42	19.898	2821	2824	2827	rVB	17693	18316	0.28%	0.036%
43	21.416	3077	3082	3093	rBV	2182106	2848688	42.78%	5.612%
44	23.704	3463	3471	3480	rBV2	3299212	6658347	100.00%	13.118%
45	23.863	3491	3498	3508	rVB2	1392181	2924712	43.93%	5.762%




Sum of corrected areas: 50756549

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP102521\
Data File : BP007708.D
Acq On : 27 Oct 2021 08:37
Operator : CG/JU
Sample : M4303-13
Misc :
ALS Vial : 66 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
P018-TW001-02

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SFAM-EPA-BP102521.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

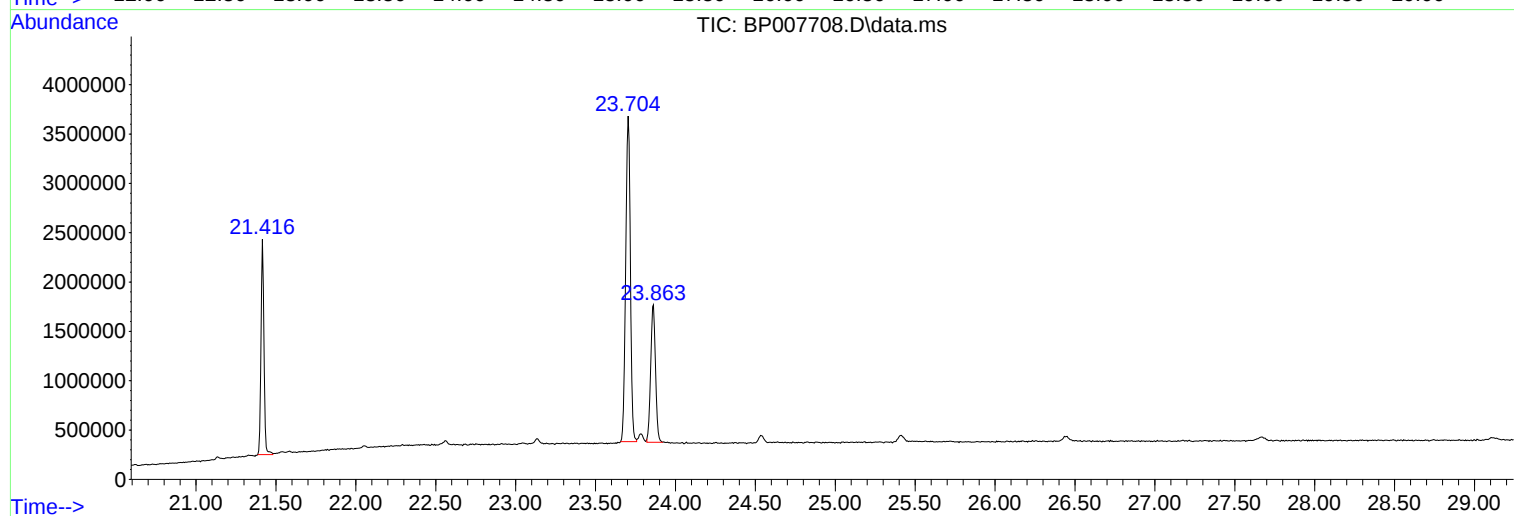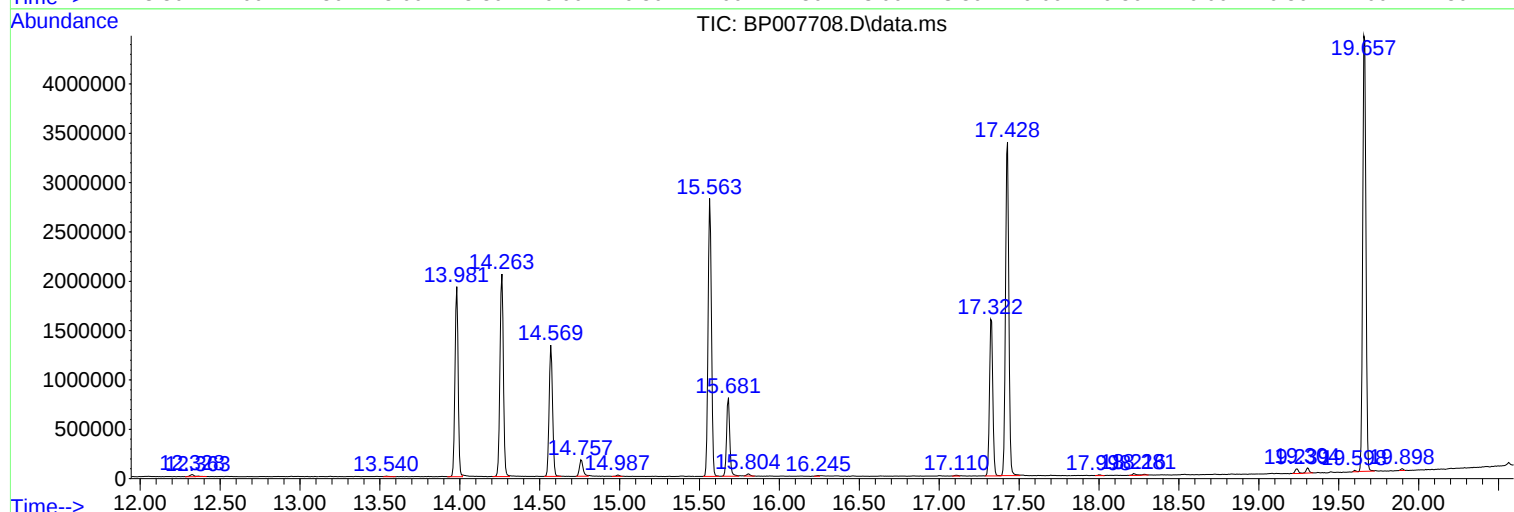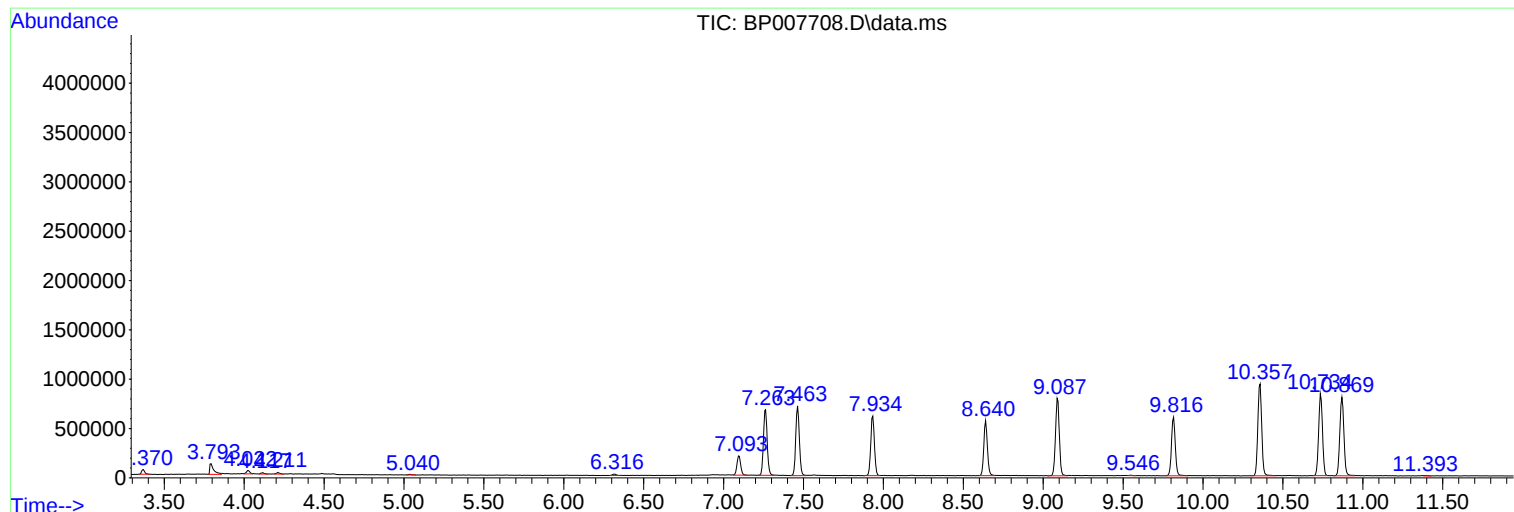

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP102521\
Data File : BP007708.D
Acq On : 27 Oct 2021 08:37
Operator : CG/JU
Sample : M4303-13
Misc :
ALS Vial : 66 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
P018-TW001-02

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SFAM-EPA-BP102521.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP102521\
Data File : BP007708.D
Acq On : 27 Oct 2021 08:37
Operator : CG/JU
Sample : M4303-13
Misc :
ALS Vial : 66 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
P018-TW001-02

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SFAM-EPA-BP102521.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
