

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP102521\
 Data File : BP007709.D
 Acq On : 27 Oct 2021 09:11
 Operator : CG/JU
 Sample : M4303-14
 Misc :
 ALS Vial : 67 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 P019-TW001-02

Integration Parameters: LSCINT.P

Integrator: RTE

Soothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SFAM-EPA-BP102521.M
 Title : SVOA CALIBRATION

Signal : TIC: BP007709.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.369	9	14	18	rVB	38934	48829	0.75%	0.087%
2	3.781	81	84	98	rBV	312766	504829	7.71%	0.898%
3	4.022	121	125	130	rVB	40679	59831	0.91%	0.106%
4	4.117	138	141	145	rVB2	12274	16487	0.25%	0.029%
5	4.211	153	157	161	rBV3	18461	23510	0.36%	0.042%
6	5.040	291	298	307	rBV3	11915	26008	0.40%	0.046%
7	6.316	510	515	521	rVB3	14471	24760	0.38%	0.044%
8	6.934	613	620	622	rBV7	6008	10198	0.16%	0.018%
9	7.093	639	647	655	rBV	234471	377604	5.77%	0.672%
10	7.263	668	676	688	rVB	835010	1328968	20.29%	2.364%
11	7.463	702	710	723	rBV	853449	1331161	20.33%	2.368%
12	7.569	725	728	734	rVB6	5351	8240	0.13%	0.015%
13	7.934	782	790	799	rBV	723914	1141606	17.43%	2.030%
14	8.187	826	833	838	rBV	4531	10883	0.17%	0.019%
15	8.640	903	910	923	rBV	655427	1057866	16.15%	1.881%
16	9.087	979	986	997	rBV	958521	1574045	24.03%	2.800%
17	9.552	1058	1065	1069	rVB8	5706	11165	0.17%	0.020%
18	9.816	1101	1110	1120	rBV	725030	1203223	18.37%	2.140%
19	10.357	1193	1202	1217	rBV	1098135	1893613	28.91%	3.368%
20	10.522	1224	1230	1241	rBV3	19586	40277	0.61%	0.072%
21	10.734	1258	1266	1276	rBV	927841	1624154	24.80%	2.889%
22	10.869	1281	1289	1307	rBV	1094408	1857369	28.36%	3.303%
23	11.393	1370	1378	1386	rBV	2875	8780	0.13%	0.016%
24	12.322	1530	1536	1542	rBV	23121	41265	0.63%	0.073%
25	12.945	1636	1642	1645	rBV7	5324	8889	0.14%	0.016%
26	13.187	1678	1683	1686	rBV7	4829	7150	0.11%	0.013%
27	13.540	1737	1743	1748	rBV9	5603	12110	0.18%	0.022%
28	13.892	1798	1803	1808	rVB9	4685	9372	0.14%	0.017%
29	13.981	1811	1818	1830	rBV	2157063	2942474	44.93%	5.233%
30	14.263	1858	1866	1885	rVB	2431294	3570835	54.52%	6.351%
31	14.569	1910	1918	1932	rBV	1511152	2233124	34.10%	3.972%
32	14.763	1945	1951	1967	rBV	150921	266857	4.07%	0.475%
33	14.987	1984	1989	1993	rVB7	7158	10979	0.17%	0.020%
34	15.392	2051	2058	2061	rBV8	5256	9488	0.14%	0.017%
35	15.563	2080	2087	2096	rBV	3037463	4489095	68.54%	7.984%
36	15.681	2100	2107	2121	rVV	737892	1055991	16.12%	1.878%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP102521\
 Data File : BP007709.D
 Acq On : 27 Oct 2021 09:11
 Operator : CG/JU
 Sample : M4303-14
 Misc :
 ALS Vial : 67 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 P019-TW001-02

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF Filtering: 5
 Sampling : 1 Min Area: 0.1 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SFAM-EPA-BP102521.M
 Title : SVOA CALIBRATION

37	15.804	2123	2128	2135	rVB3	25246	40741	0.62%	0.072%
38	16.139	2178	2185	2188	rBV8	5807	10672	0.16%	0.019%
39	16.257	2199	2205	2211	rVB9	9364	20486	0.31%	0.036%
40	16.351	2218	2221	2225	rVB6	5479	7621	0.12%	0.014%
41	17.004	2329	2332	2338	rVB8	6076	7487	0.11%	0.013%
42	17.110	2345	2350	2353	rBV4	10456	18492	0.28%	0.033%
43	17.322	2379	2386	2397	rBV	1808916	2716305	41.47%	4.831%
44	17.428	2397	2404	2414	rVV	3272088	4879662	74.51%	8.679%
45	17.516	2416	2419	2427	rVB9	19912	33232	0.51%	0.059%
46	17.704	2447	2451	2456	rBV6	4721	7142	0.11%	0.013%
47	18.004	2499	2502	2507	rVB4	11625	16416	0.25%	0.029%
48	18.216	2535	2538	2545	rBV4	20130	32207	0.49%	0.057%
49	18.286	2547	2550	2557	rVB2	8303	12996	0.20%	0.023%
50	19.239	2707	2712	2716	rBV2	50997	75805	1.16%	0.135%
51	19.304	2719	2723	2731	rVV	52606	78591	1.20%	0.140%
52	19.604	2771	2774	2777	rVB5	15959	18226	0.28%	0.032%
53	19.663	2777	2784	2790	rBV	4457603	5976122	91.25%	10.629%
54	21.133	3031	3034	3040	rBV4	47987	76914	1.17%	0.137%
55	21.416	3077	3082	3088	rBV	2533853	3285959	50.17%	5.844%
56	23.704	3463	3471	3480	rBV2	3292024	6549289	100.00%	11.648%
57	23.863	3491	3498	3510	rVB2	1703396	3519823	53.74%	6.260%




Sum of corrected areas: 56225223

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP102521\
Data File : BP007709.D
Acq On : 27 Oct 2021 09:11
Operator : CG/JU
Sample : M4303-14
Misc :
ALS Vial : 67 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
P019-TW001-02

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SFAM-EPA-BP102521.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

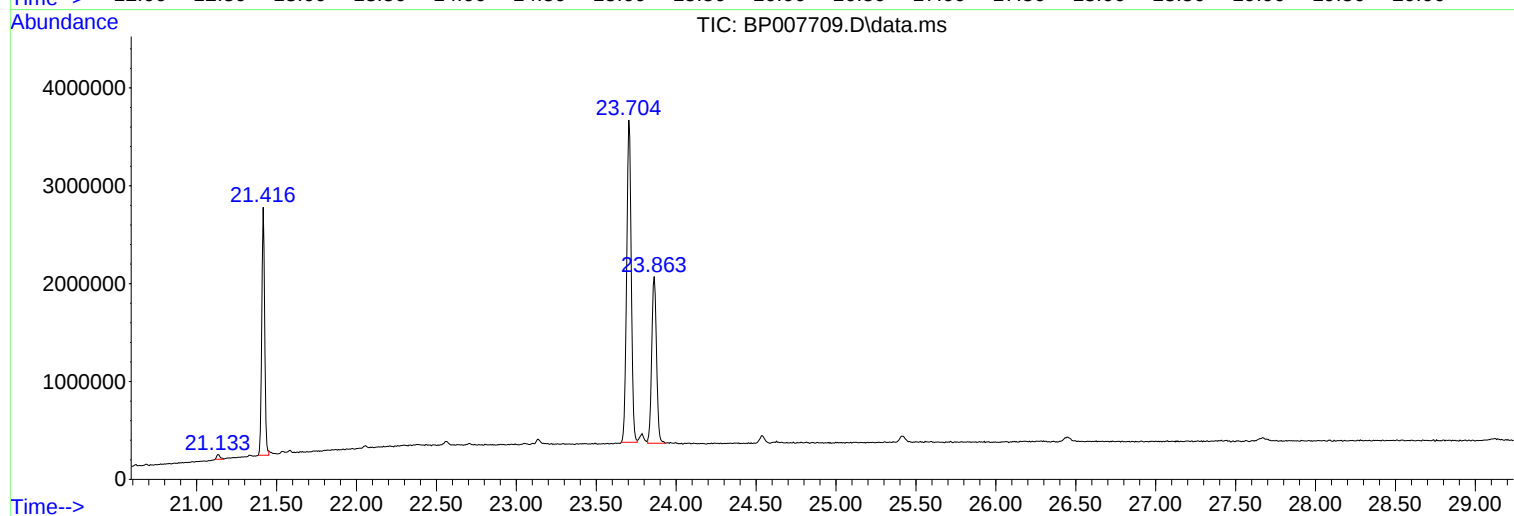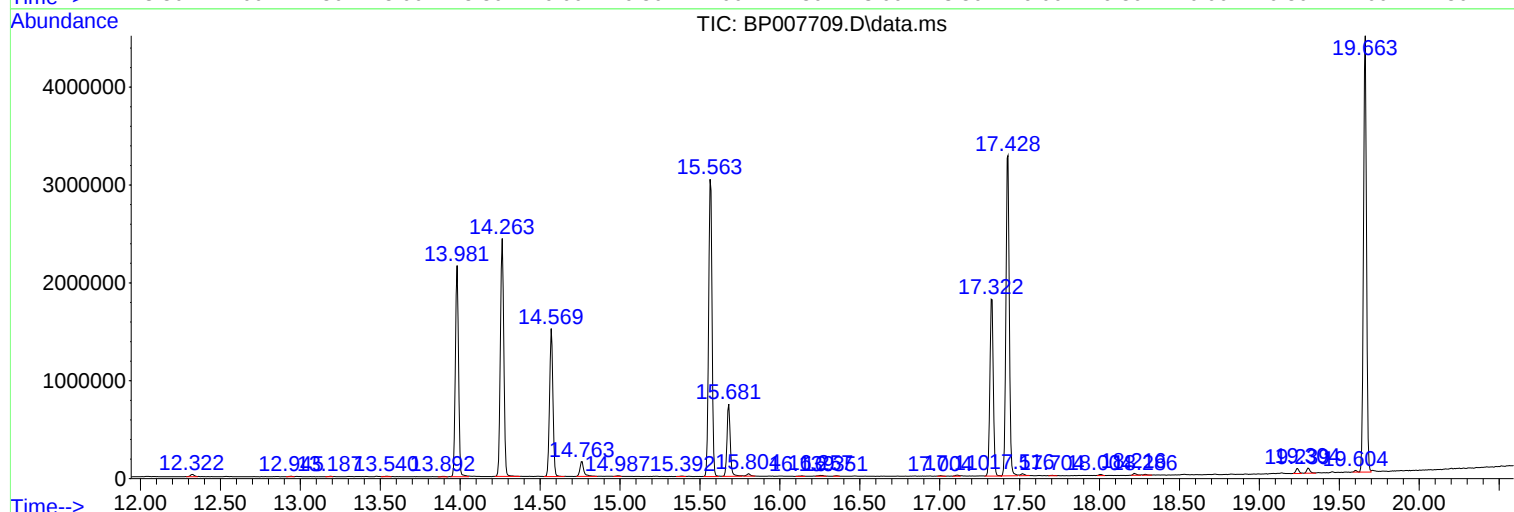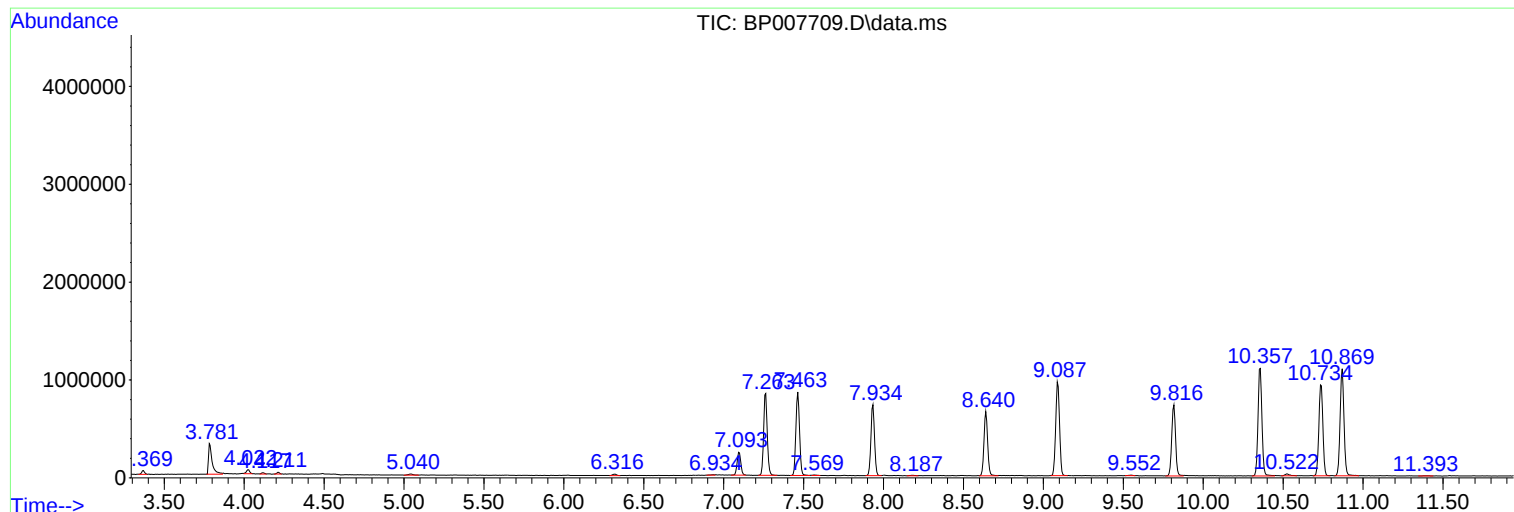

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP102521\
Data File : BP007709.D
Acq On : 27 Oct 2021 09:11
Operator : CG/JU
Sample : M4303-14
Misc :
ALS Vial : 67 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
P019-TW001-02

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SFAM-EPA-BP102521.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP102521\
Data File : BP007709.D
Acq On : 27 Oct 2021 09:11
Operator : CG/JU
Sample : M4303-14
Misc :
ALS Vial : 67 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
P019-TW001-02

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SFAM-EPA-BP102521.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
