

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP102521\
 Data File : BP007710.D
 Acq On : 27 Oct 2021 09:45
 Operator : CG/JU
 Sample : M4303-15
 Misc :
 ALS Vial : 68 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 P021-TW001-02

Integration Parameters: LSCINT.P

Integrator: RTE

Soothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SFAM-EPA-BP102521.M
 Title : SVOA CALIBRATION

Signal : TIC: BP007710.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.364	10	13	19	rBV	41652	56990	1.02%	0.122%
2	3.787	83	85	100	rBV	158206	260276	4.65%	0.559%
3	4.022	120	125	131	rVB	29348	43816	0.78%	0.094%
4	4.117	137	141	149	rVB2	13187	21501	0.38%	0.046%
5	4.211	154	157	162	rVB4	15379	20005	0.36%	0.043%
6	5.034	293	297	307	rBV5	9591	18703	0.33%	0.040%
7	6.316	510	515	523	rVB7	11731	20266	0.36%	0.044%
8	6.940	617	621	625	rBV6	3986	5609	0.10%	0.012%
9	7.093	641	647	654	rVB	209201	332578	5.94%	0.714%
10	7.258	669	675	686	rVB	563566	927214	16.56%	1.991%
11	7.463	703	710	718	rBV	634746	974004	17.40%	2.091%
12	7.534	718	722	736	rVB	67119	121857	2.18%	0.262%
13	7.934	782	790	798	rBV	637620	1012470	18.08%	2.174%
14	8.640	902	910	918	rBV	545759	859945	15.36%	1.846%
15	9.087	977	986	996	rBV	680004	1107557	19.78%	2.378%
16	9.546	1061	1064	1069	rVB6	4926	7126	0.13%	0.015%
17	9.816	1101	1110	1121	rBV	501097	836000	14.93%	1.795%
18	10.357	1193	1202	1215	rBV	818715	1393906	24.90%	2.993%
19	10.522	1223	1230	1240	rBV4	17352	38119	0.68%	0.082%
20	10.734	1258	1266	1277	rVB	858776	1451020	25.92%	3.115%
21	10.869	1282	1289	1303	rVV	752902	1284300	22.94%	2.757%
22	11.540	1398	1403	1406	rBV7	4282	8631	0.15%	0.019%
23	12.322	1530	1536	1542	rVB2	16702	29136	0.52%	0.063%
24	12.940	1637	1641	1645	rBV7	5252	7037	0.13%	0.015%
25	13.193	1677	1684	1688	rBV10	5759	11117	0.20%	0.024%
26	13.481	1728	1733	1737	rBV5	8801	14683	0.26%	0.032%
27	13.545	1740	1744	1748	rVB6	5092	7319	0.13%	0.016%
28	13.981	1810	1818	1825	rBV	1697618	2344566	41.88%	5.034%
29	14.263	1857	1866	1878	rBV	1820403	2607847	46.58%	5.599%
30	14.569	1910	1918	1928	rBV	1345090	1993717	35.61%	4.281%
31	14.763	1942	1951	1961	rBV	172719	291460	5.21%	0.626%
32	14.928	1976	1979	1985	rVB8	4221	6832	0.12%	0.015%
33	14.992	1985	1990	1994	rVB6	10822	15125	0.27%	0.032%
34	15.387	2052	2057	2061	rBV7	6776	12003	0.21%	0.026%
35	15.563	2079	2087	2100	rBV	2405036	3535029	63.14%	7.590%
36	15.681	2100	2107	2121	rVV	649188	926154	16.54%	1.989%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP102521\
 Data File : BP007710.D
 Acq On : 27 Oct 2021 09:45
 Operator : CG/JU
 Sample : M4303-15
 Misc :
 ALS Vial : 68 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 P021-TW001-02

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF Filtering: 5
 Sampling : 1 Min Area: 0.1 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SFAM-EPA-BP102521.M
 Title : SVOA CALIBRATION

37	15.810	2124	2129	2138	rVB3	18320	35444	0.63%	0.076%
38	16.263	2197	2206	2211	rBV3	18531	37891	0.68%	0.081%
39	16.298	2211	2212	2217	rVB5	4663	6484	0.12%	0.014%
40	16.351	2217	2221	2225	rBV7	4963	7578	0.14%	0.016%
41	17.110	2345	2350	2353	rBV2	9921	15424	0.28%	0.033%
42	17.269	2373	2377	2380	rBV6	3680	6201	0.11%	0.013%
43	17.328	2380	2387	2397	rBV	1689970	2420357	43.23%	5.197%
44	17.428	2397	2404	2416	rVV	2930237	4221006	75.39%	9.063%
45	17.698	2446	2450	2451	rBV4	5299	5936	0.11%	0.013%
46	18.010	2498	2503	2507	rVB5	17698	22375	0.40%	0.048%
47	18.222	2535	2539	2545	rBV7	26046	43621	0.78%	0.094%
48	19.139	2692	2695	2700	rVB6	39179	44466	0.79%	0.095%
49	19.239	2708	2712	2715	rBV3	47046	60052	1.07%	0.129%
50	19.304	2720	2723	2727	rVV	45281	54758	0.98%	0.118%
51	19.604	2771	2774	2777	rVB4	12513	13765	0.25%	0.030%
52	19.663	2778	2784	2795	rBV	4002819	5237024	93.54%	11.244%
53	21.416	3077	3082	3094	rBV	2208899	3019621	53.93%	6.483%
54	23.710	3464	3472	3481	rBV2	2775222	5598948	100.00%	12.021%
55	23.863	3491	3498	3509	rVB2	1519542	3120413	55.73%	6.700%




Sum of corrected areas: 46575282

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP102521\
Data File : BP007710.D
Acq On : 27 Oct 2021 09:45
Operator : CG/JU
Sample : M4303-15
Misc :
ALS Vial : 68 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
P021-TW001-02

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SFAM-EPA-BP102521.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

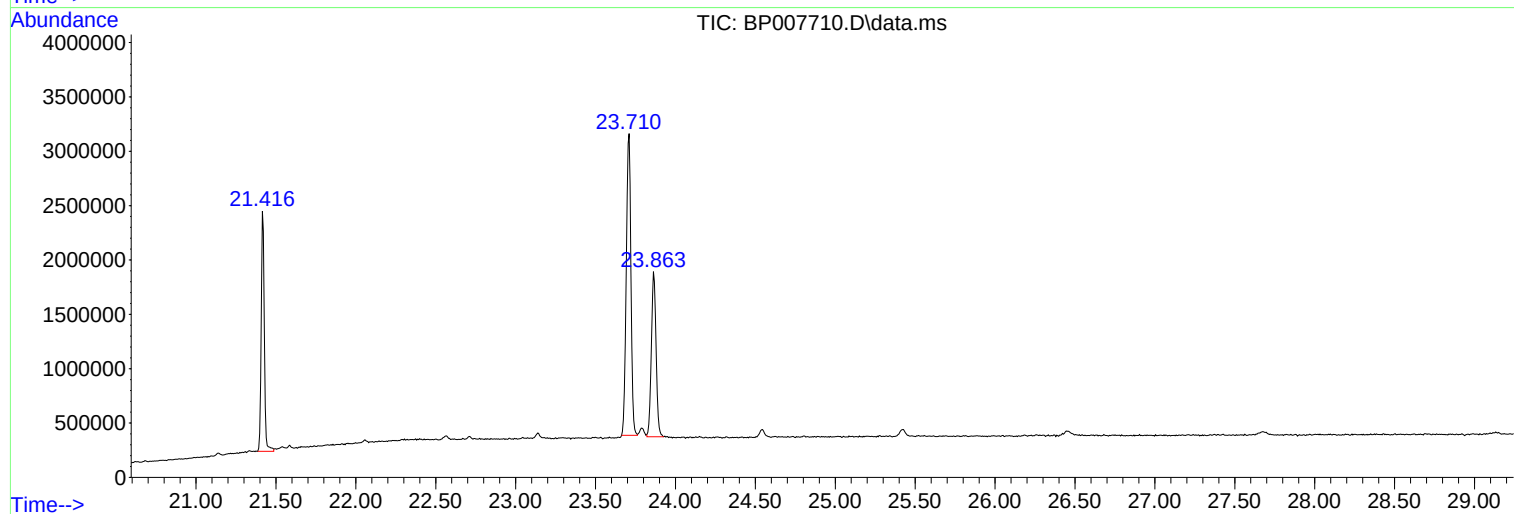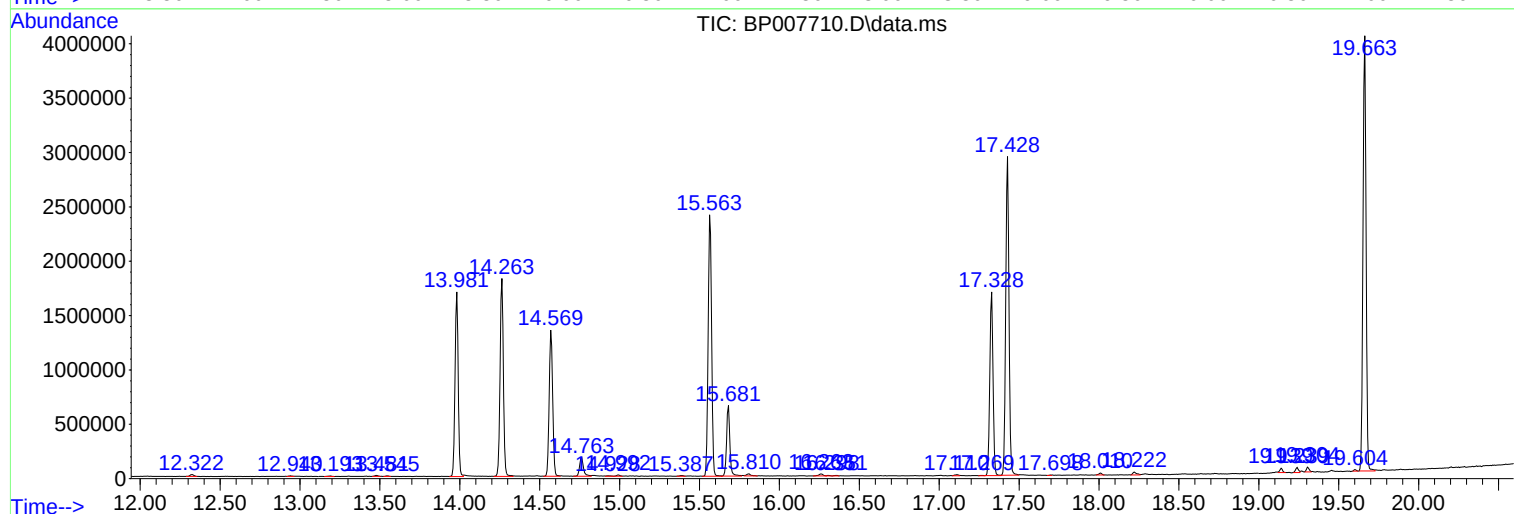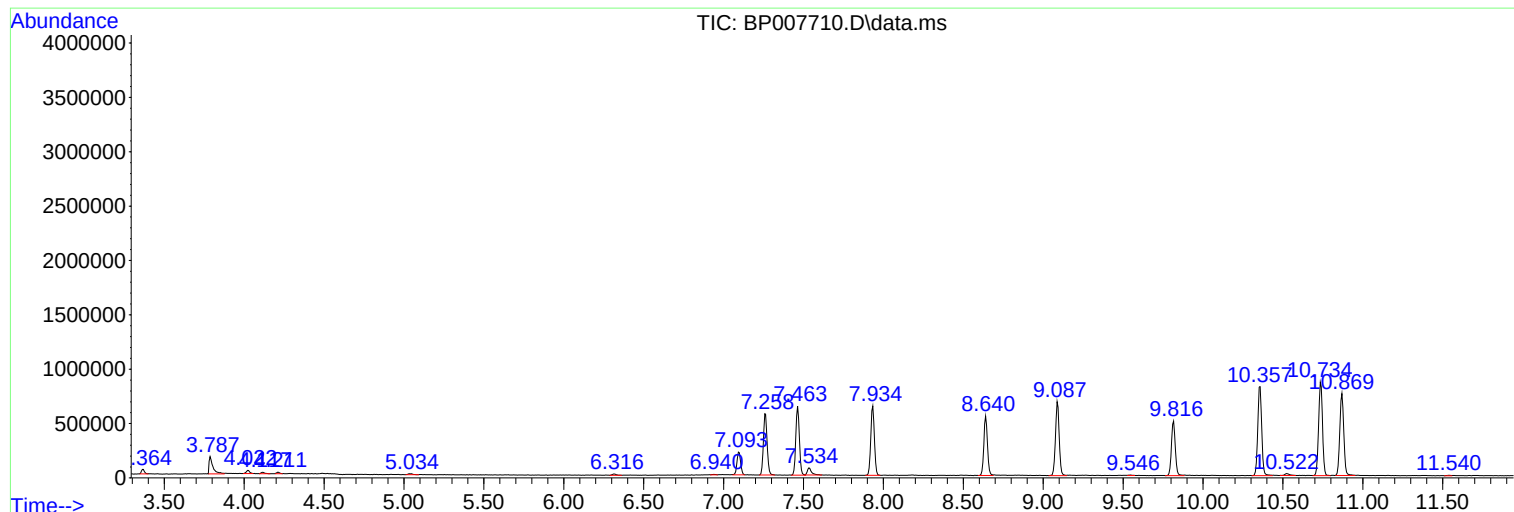

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP102521\
Data File : BP007710.D
Acq On : 27 Oct 2021 09:45
Operator : CG/JU
Sample : M4303-15
Misc :
ALS Vial : 68 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
P021-TW001-02










Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SFAM-EPA-BP102521.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 Ethanol, 2-(2-ethoxyethoxy)- Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
7.534	2.41 ng/ul	121857	1,4-Dichlorobenzene-d4	7.934

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			Ethanol, 2-(2-ethoxyethoxy)-	134	C6H14O3	000111-90-0	90
2			Ethanol, 2-(2-ethoxyethoxy)-	134	C6H14O3	000111-90-0	78
3			Ethanol, 2-(2-ethoxyethoxy)-	134	C6H14O3	000111-90-0	53
4			Ethanol, 2-(2-ethoxyethoxy)-	134	C6H14O3	000111-90-0	50
5			2-Propanol, 1-(1-methylethoxy)-	118	C6H14O2	003944-36-3	45

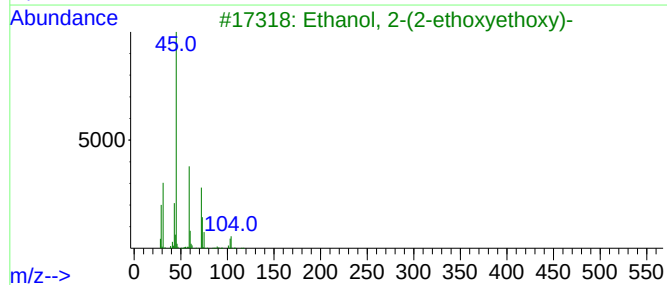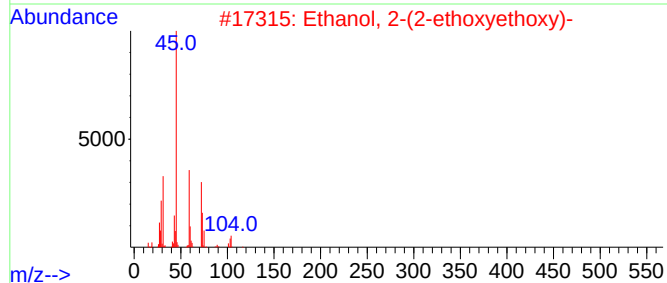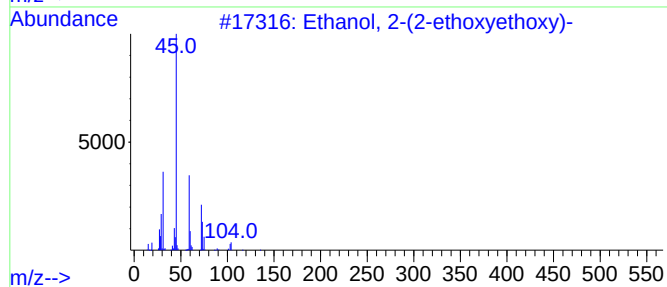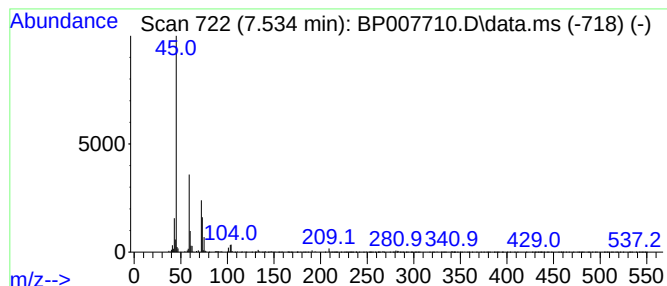

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP102521\
Data File : BP007710.D
Acq On : 27 Oct 2021 09:45
Operator : CG/JU
Sample : M4303-15
Misc :
ALS Vial : 68 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
P021-TW001-02

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SFAM-EPA-BP102521.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
Ethanol, 2-(2-e...	7.534	2.4	ng/ul	121857	1	7.934	1012470	20.0