

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP102521\
 Data File : BP007713.D
 Acq On : 27 Oct 2021 11:27
 Operator : CG/JU
 Sample : M4303-10
 Misc :
 ALS Vial : 63 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 P013-TW001-03

Integration Parameters: LSCINT.P

Integrator: RTE

Smoother: OFF

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 0.1 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SFAM-EPA-BP102521.M
 Title : SVOA CALIBRATION

Signal : TIC: BP007713.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.340	5	9	10	rBV3	13872	16064	0.24%	0.030%
2	3.363	10	13	24	rVB	65322	93865	1.42%	0.177%
3	3.781	82	84	101	rBV	377855	597216	9.04%	1.128%
4	4.022	120	125	131	rBV	68033	103502	1.57%	0.195%
5	4.116	137	141	146	rBV2	15968	21664	0.33%	0.041%
6	4.210	154	157	162	rVB2	26619	36344	0.55%	0.069%
7	4.299	168	172	176	rVB6	4872	8442	0.13%	0.016%
8	4.487	202	204	209	rVB3	8344	9517	0.14%	0.018%
9	4.651	229	232	237	rVB7	5000	7924	0.12%	0.015%
10	5.034	293	297	307	rVB	19904	32808	0.50%	0.062%
11	6.316	510	515	519	rBV7	7438	12913	0.20%	0.024%
12	6.945	618	622	627	rBV7	5007	8131	0.12%	0.015%
13	7.098	641	648	655	rBV	233975	360518	5.46%	0.681%
14	7.263	670	676	690	rVB	824570	1322140	20.01%	2.497%
15	7.463	703	710	719	rBV	230044	361168	5.47%	0.682%
16	7.569	724	728	733	rVB4	9577	13256	0.20%	0.025%
17	7.757	754	760	765	rBV6	7735	14990	0.23%	0.028%
18	7.934	783	790	798	rVB	812710	1272459	19.26%	2.403%
19	8.181	826	832	841	rBV6	9818	24486	0.37%	0.046%
20	8.492	880	885	892	rBV8	6007	12559	0.19%	0.024%
21	8.640	903	910	919	rBV	479675	762395	11.54%	1.440%
22	9.092	975	987	994	rBV	951490	1554771	23.53%	2.936%
23	9.557	1063	1066	1070	rVB6	7643	9079	0.14%	0.017%
24	9.816	1103	1110	1119	rBV	120368	202467	3.06%	0.382%
25	9.898	1119	1124	1129	rVB6	6081	10849	0.16%	0.020%
26	10.357	1195	1202	1209	rBV	257688	428379	6.48%	0.809%
27	10.528	1227	1231	1238	rBV5	9360	17564	0.27%	0.033%
28	10.739	1256	1267	1277	rBV	1059074	1786484	27.04%	3.373%
29	10.869	1281	1289	1305	rBV	1122914	1898314	28.73%	3.584%
30	11.392	1375	1378	1384	rVB5	5494	7407	0.11%	0.014%
31	11.545	1399	1404	1412	rVB5	17122	30322	0.46%	0.057%
32	12.051	1485	1490	1493	rBV7	4003	7272	0.11%	0.014%
33	12.139	1499	1505	1515	rVB3	26738	46306	0.70%	0.087%
34	12.328	1530	1537	1546	rBV2	20057	40938	0.62%	0.077%
35	12.945	1638	1642	1647	rBV6	7891	14900	0.23%	0.028%
36	13.186	1679	1683	1688	rVB7	7665	10547	0.16%	0.020%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP102521\
 Data File : BP007713.D
 Acq On : 27 Oct 2021 11:27
 Operator : CG/JU
 Sample : M4303-10
 Misc :
 ALS Vial : 63 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 P013-TW001-03

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF Filtering: 5
 Sampling : 1 Min Area: 0.1 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SFAM-EPA-BP102521.M
 Title : SVOA CALIBRATION

37	13.545	1738	1744	1748	rBV6	12177	19360	0.29%	0.037%
38	13.898	1796	1804	1810	rBV	89385	145016	2.19%	0.274%
39	13.980	1812	1818	1833	rVV	2081577	2832403	42.87%	5.348%
40	14.263	1857	1866	1877	rBV	2379153	3469821	52.51%	6.552%
41	14.574	1910	1919	1926	rBV	1614386	2385511	36.10%	4.504%
42	14.763	1945	1951	1967	rBV	111344	198931	3.01%	0.376%
43	15.386	2050	2057	2064	rBV6	6999	12991	0.20%	0.025%
44	15.569	2080	2088	2097	rBV	2941297	4373670	66.19%	8.259%
45	15.680	2101	2107	2115	rVV2	87334	134474	2.04%	0.254%
46	15.810	2124	2129	2133	rBV2	22780	35717	0.54%	0.067%
47	15.845	2133	2135	2140	rVB5	7812	9663	0.15%	0.018%
48	15.939	2148	2151	2155	rVB6	4916	7267	0.11%	0.014%
49	16.133	2179	2184	2188	rBV8	5719	10887	0.16%	0.021%
50	16.263	2195	2206	2211	rBV8	10171	29431	0.45%	0.056%
51	16.327	2211	2217	2222	rBV5	17502	31974	0.48%	0.060%
52	16.845	2300	2305	2309	rBV8	4993	8413	0.13%	0.016%
53	17.116	2347	2351	2353	rBV3	7129	9335	0.14%	0.018%
54	17.157	2354	2358	2362	rVB7	9901	15392	0.23%	0.029%
55	17.327	2380	2387	2397	rBV	1967293	2906011	43.98%	5.487%
56	17.427	2397	2404	2417	rVV	3506772	4953001	74.96%	9.352%
57	17.568	2424	2428	2431	rVB	13835	17925	0.27%	0.034%
58	17.904	2482	2485	2491	rVB6	7562	12948	0.20%	0.024%
59	17.998	2497	2501	2505	rBV7	9170	15222	0.23%	0.029%
60	18.192	2531	2534	2537	rBV	10254	12722	0.19%	0.024%
61	18.239	2540	2542	2546	rVB2	13675	16568	0.25%	0.031%
62	18.374	2563	2565	2568	rVB4	8237	8906	0.13%	0.017%
63	19.239	2708	2712	2717	rBV2	53513	70479	1.07%	0.133%
64	19.304	2719	2723	2729	rBV	42280	66124	1.00%	0.125%
65	19.604	2771	2774	2777	rBV4	18163	19230	0.29%	0.036%
66	19.662	2778	2784	2791	rBV	4497898	6028809	91.24%	11.384%
67	21.415	3077	3082	3091	rBV	2629583	3524175	53.34%	6.654%
68	23.709	3464	3472	3480	rBV2	3175579	6607467	100.00%	12.476%
69	23.862	3491	3498	3513	rVB2	1754715	3811814	57.69%	7.198%




Sum of corrected areas: 52959617

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP102521\
Data File : BP007713.D
Acq On : 27 Oct 2021 11:27
Operator : CG/JU
Sample : M4303-10
Misc :
ALS Vial : 63 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
P013-TW001-03

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SFAM-EPA-BP102521.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

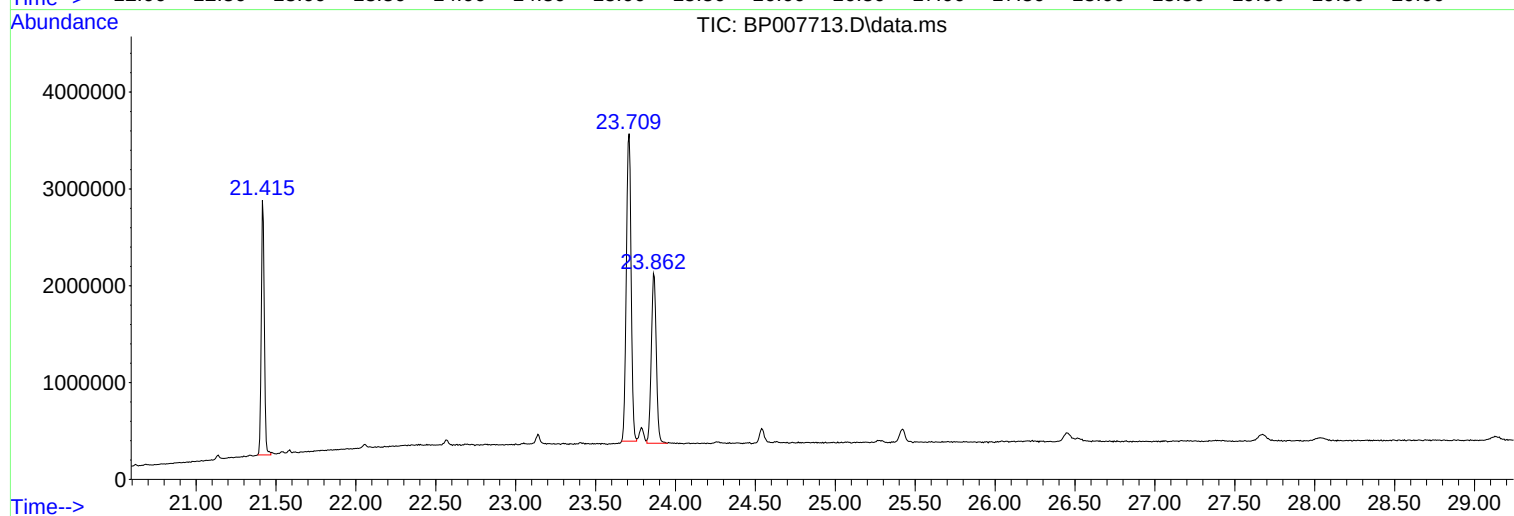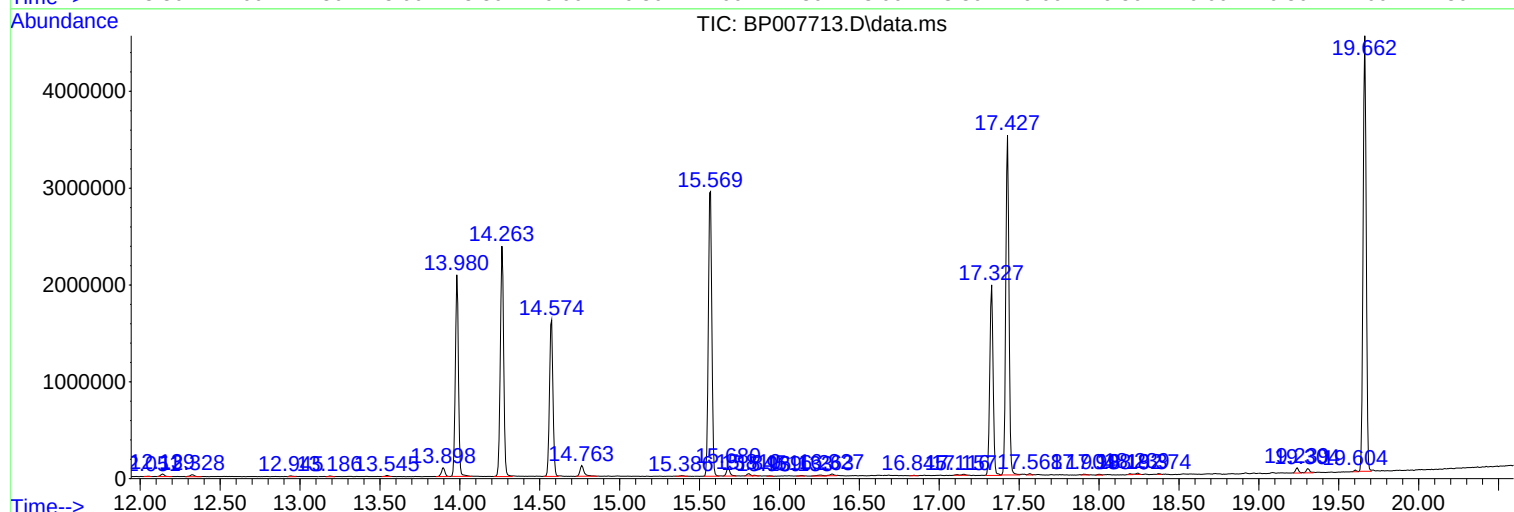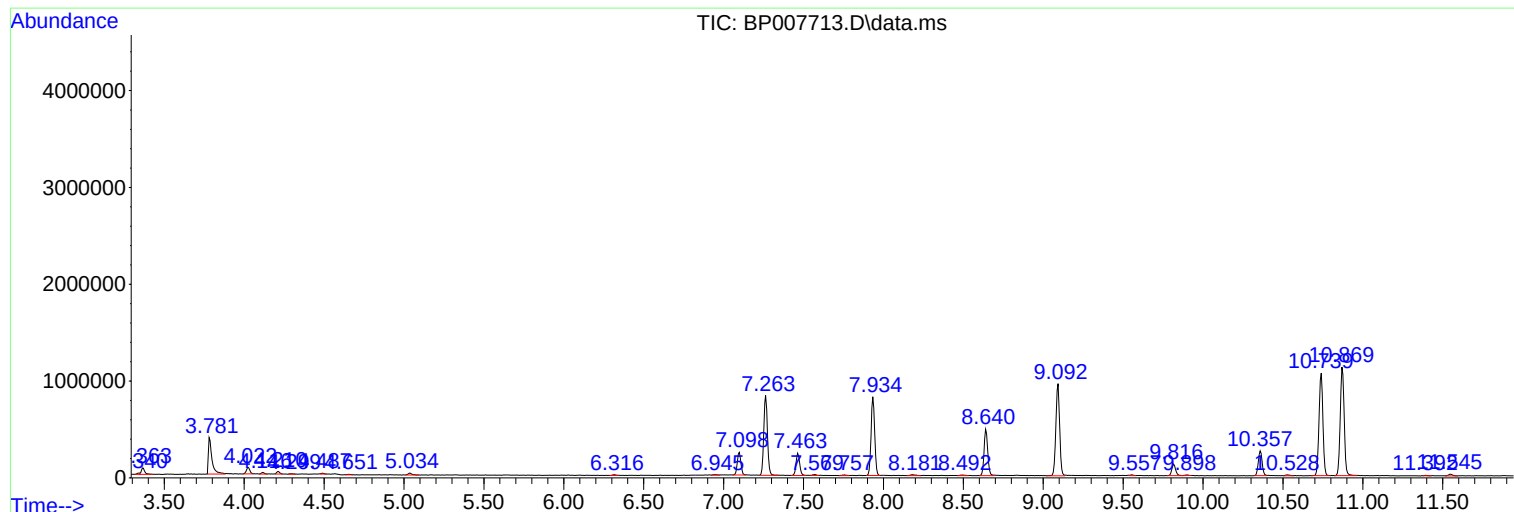

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP102521\
Data File : BP007713.D
Acq On : 27 Oct 2021 11:27
Operator : CG/JU
Sample : M4303-10
Misc :
ALS Vial : 63 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
P013-TW001-03

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SFAM-EPA-BP102521.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP102521\
Data File : BP007713.D
Acq On : 27 Oct 2021 11:27
Operator : CG/JU
Sample : M4303-10
Misc :
ALS Vial : 63 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
P013-TW001-03

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SFAM-EPA-BP102521.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------