

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP102521\
 Data File : BP007714.D
 Acq On : 27 Oct 2021 12:01
 Operator : CG/JU
 Sample : M4304-07
 Misc :
 ALS Vial : 71 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 P066-TW001-01

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SFAM-EPA-BP102521.M
 Title : SVOA CALIBRATION

Signal : TIC: BP007714.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.364	9	13	21	rVB	53530	71380	0.97%	0.124%
2	3.787	83	85	98	rBV	110621	183880	2.51%	0.320%
3	4.023	121	125	130	rVB	34629	49491	0.68%	0.086%
4	4.117	138	141	147	rVB3	14779	20141	0.28%	0.035%
5	4.211	154	157	162	rVB4	15946	20427	0.28%	0.036%
6	5.040	294	298	304	rVB4	8381	14157	0.19%	0.025%
7	6.317	511	515	520	rVB3	14404	21885	0.30%	0.038%
8	7.093	642	647	657	rVB	213639	341920	4.67%	0.595%
9	7.264	669	676	686	rBV	792579	1243994	16.99%	2.165%
10	7.464	703	710	718	rBV	799450	1246184	17.02%	2.169%
11	7.934	782	790	798	rBV	786519	1249603	17.06%	2.175%
12	8.011	798	803	808	rVB8	5572	9243	0.13%	0.016%
13	8.640	903	910	920	rBV	602352	960895	13.12%	1.672%
14	9.093	978	987	1001	rBV	876426	1480428	20.22%	2.576%
15	9.522	1050	1060	1061	rBV10	3737	8997	0.12%	0.016%
16	9.552	1061	1065	1071	rVB8	6239	11274	0.15%	0.020%
17	9.816	1101	1110	1120	rBV	679413	1090823	14.90%	1.898%
18	10.357	1192	1202	1213	rBV	1035696	1750402	23.90%	3.046%
19	10.522	1224	1230	1247	rBV	40928	87460	1.19%	0.152%
20	10.734	1259	1266	1275	rBV	993657	1723092	23.53%	2.998%
21	10.869	1280	1289	1306	rBV	900150	1518360	20.74%	2.642%
22	12.046	1485	1489	1494	rVB7	4410	8745	0.12%	0.015%
23	12.328	1528	1537	1543	rBV2	24444	41649	0.57%	0.072%
24	12.946	1637	1642	1646	rBV6	6269	11034	0.15%	0.019%
25	13.187	1678	1683	1689	rBV8	7457	14608	0.20%	0.025%
26	13.481	1727	1733	1740	rBV10	4295	9669	0.13%	0.017%
27	13.546	1740	1744	1748	rVB5	4978	8328	0.11%	0.014%
28	13.981	1812	1818	1834	rBV	2121194	2889343	39.46%	5.028%
29	14.263	1857	1866	1878	rBV	2301879	3340580	45.62%	5.813%
30	14.569	1911	1918	1928	rBV	1490668	2316518	31.64%	4.031%
31	14.763	1943	1951	1964	rBV	177186	300901	4.11%	0.524%
32	14.993	1983	1990	1996	rVB8	12099	19960	0.27%	0.035%
33	15.387	2053	2057	2061	rBV5	7534	12577	0.17%	0.022%
34	15.569	2080	2088	2099	rBV	2984565	4380688	59.82%	7.623%
35	15.681	2099	2107	2118	rBV	876184	1222402	16.69%	2.127%
36	15.804	2124	2128	2134	rVB2	24061	37195	0.51%	0.065%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP102521\
 Data File : BP007714.D
 Acq On : 27 Oct 2021 12:01
 Operator : CG/JU
 Sample : M4304-07
 Misc :
 ALS Vial : 71 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 P066-TW001-01

Integration Parameters: LSCINT.P
 Integrator: RTE
 Smoothing : OFF Filtering: 5
 Sampling : 1 Min Area: 0.1 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SFAM-EPA-BP102521.M
 Title : SVOA CALIBRATION

37	16.257	2197	2205	2209	rBV2	7158	15216	0.21%	0.026%
38	16.357	2217	2222	2227	rVB9	5423	10294	0.14%	0.018%
39	17.110	2344	2350	2355	rBV3	12318	23314	0.32%	0.041%
40	17.328	2380	2387	2396	rBV	1942432	2779177	37.95%	4.836%
41	17.428	2397	2404	2417	rVV	3758449	5417815	73.99%	9.428%
42	17.704	2448	2451	2455	rBV5	5460	8013	0.11%	0.014%
43	18.010	2499	2503	2506	rBV4	21910	28336	0.39%	0.049%
44	18.216	2534	2538	2545	rBV5	41879	72962	1.00%	0.127%
45	19.239	2707	2712	2716	rBV	54339	76378	1.04%	0.133%
46	19.304	2719	2723	2728	rVV	55089	77062	1.05%	0.134%
47	19.457	2746	2749	2755	rBV7	15566	22120	0.30%	0.038%
48	19.598	2771	2773	2777	rBV4	11250	13183	0.18%	0.023%
49	19.663	2778	2784	2795	rVV	4880858	6627955	90.51%	11.534%
50	21.133	3031	3034	3041	rBV2	90285	144444	1.97%	0.251%
51	21.416	3077	3082	3089	rBV	2620197	3406992	46.53%	5.929%
52	23.710	3464	3472	3481	rBV2	3470413	7322612	100.00%	12.743%
53	23.863	3491	3498	3515	rVB2	1768228	3701260	50.55%	6.441%


Sum of corrected areas: 57465366

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP102521\
Data File : BP007714.D
Acq On : 27 Oct 2021 12:01
Operator : CG/JU
Sample : M4304-07
Misc :
ALS Vial : 71 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
P066-TW001-01

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SFAM-EPA-BP102521.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

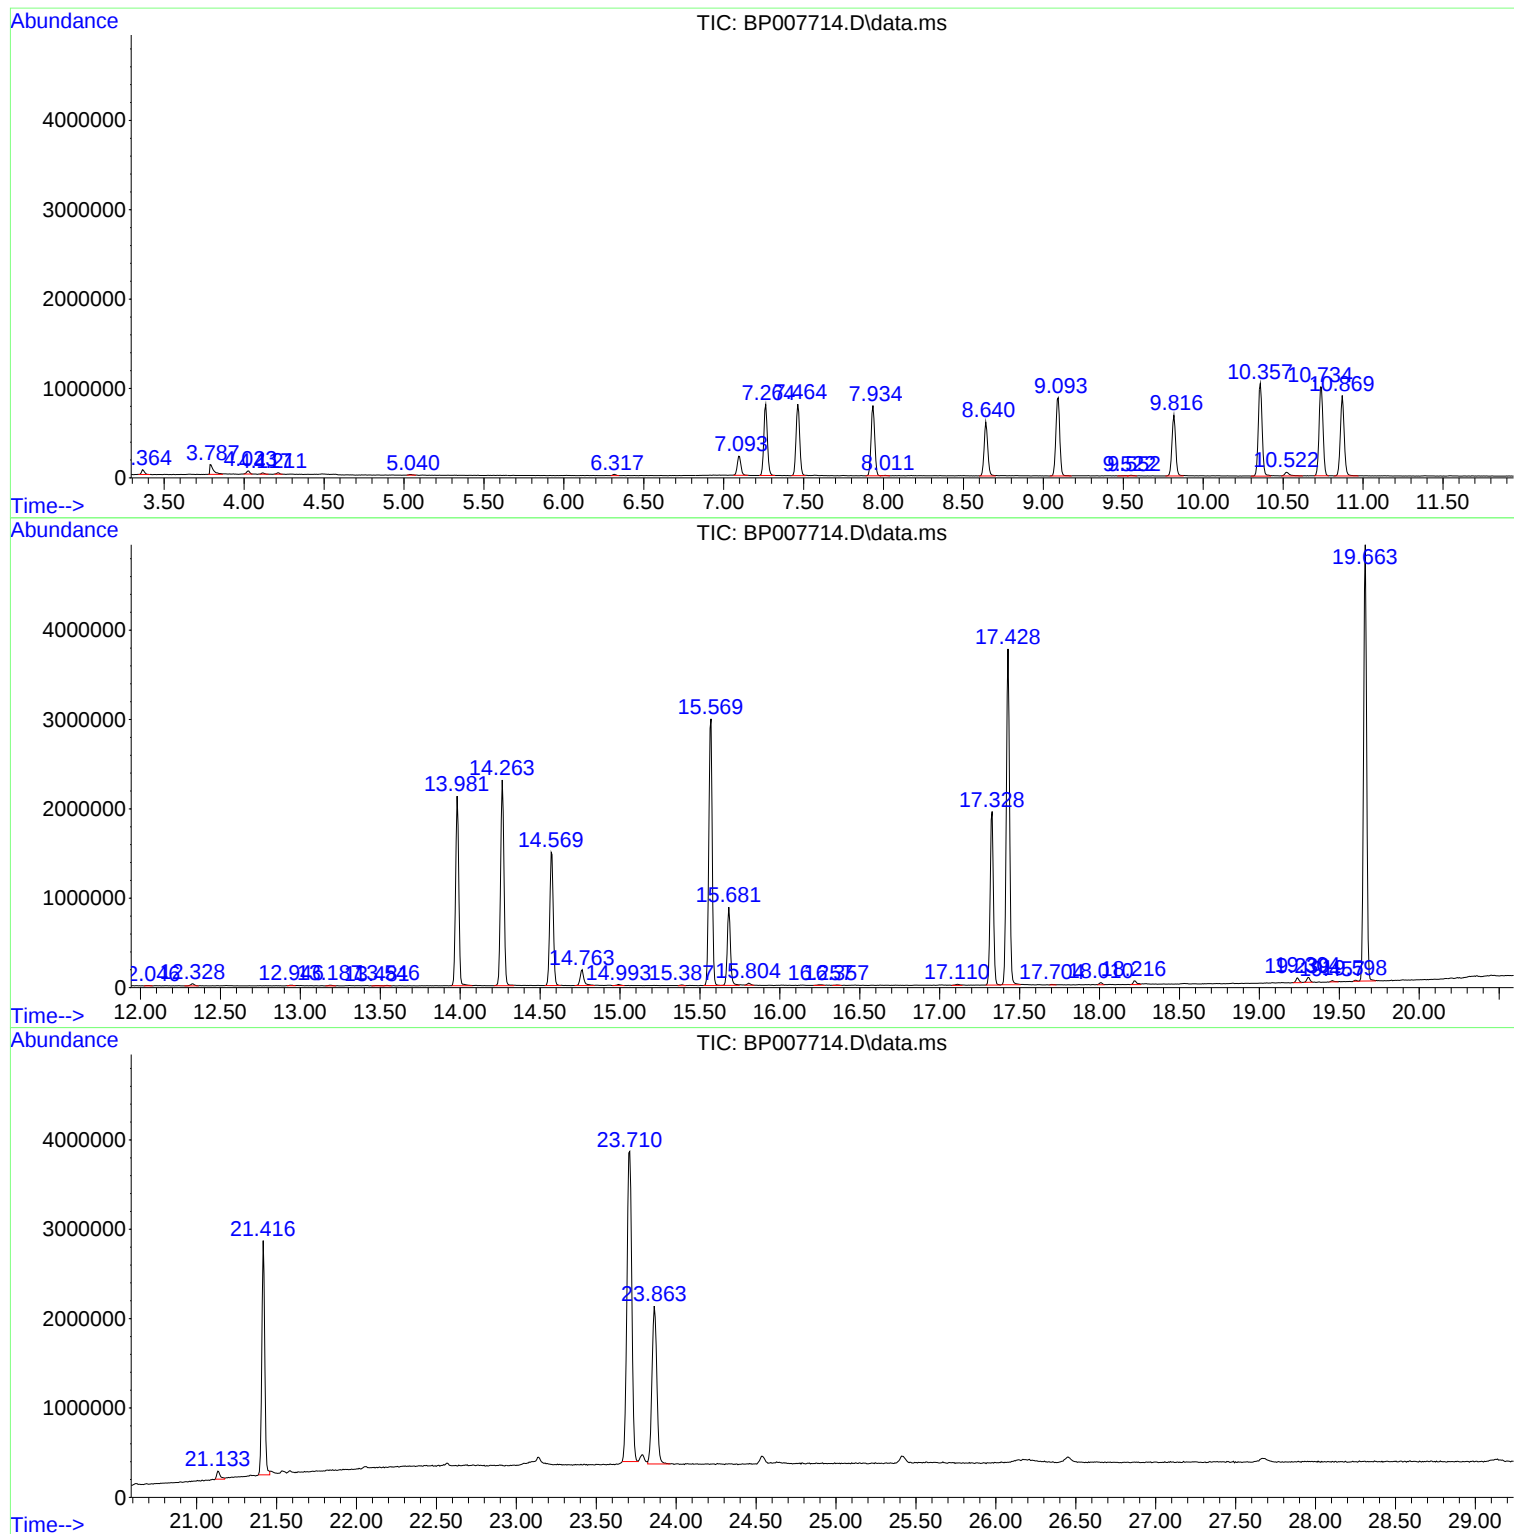

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP102521\
Data File : BP007714.D
Acq On : 27 Oct 2021 12:01
Operator : CG/JU
Sample : M4304-07
Misc :
ALS Vial : 71 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
P066-TW001-01

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SFAM-EPA-BP102521.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP102521\
Data File : BP007714.D
Acq On : 27 Oct 2021 12:01
Operator : CG/JU
Sample : M4304-07
Misc :
ALS Vial : 71 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
P066-TW001-01

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SFAM-EPA-BP102521.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
