

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP102521\
 Data File : BP007715.D
 Acq On : 27 Oct 2021 12:35
 Operator : CG/JU
 Sample : M4304-08
 Misc :
 ALS Vial : 72 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 P067-TW001-01

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SFAM-EPA-BP102521.M
 Title : SVOA CALIBRATION

Signal : TIC: BP007715.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.369	10	14	21	rVB	46404	65323	0.92%	0.122%
2	3.787	83	85	99	rBV	242286	388163	5.49%	0.725%
3	4.028	120	126	131	rBV2	30999	49314	0.70%	0.092%
4	4.116	137	141	145	rBV2	15236	21974	0.31%	0.041%
5	4.211	154	157	164	rVB7	14000	19024	0.27%	0.036%
6	4.487	202	204	210	rBV6	5697	9009	0.13%	0.017%
7	5.034	295	297	301	rVB3	6503	8781	0.12%	0.016%
8	6.316	511	515	520	rBV3	11587	16362	0.23%	0.031%
9	7.099	641	648	656	rVB	182735	301418	4.26%	0.563%
10	7.263	667	676	687	rBV	702618	1114566	15.76%	2.082%
11	7.463	703	710	720	rBV	711339	1097563	15.52%	2.050%
12	7.546	720	724	731	rVB3	14395	27922	0.39%	0.052%
13	7.934	783	790	798	rBV	674497	1058926	14.97%	1.978%
14	8.640	902	910	920	rBV	549371	858892	12.14%	1.604%
15	9.093	978	987	997	rBV	808445	1324312	18.72%	2.474%
16	9.546	1062	1064	1069	rVB5	5546	8168	0.12%	0.015%
17	9.816	1103	1110	1119	rBV	602855	981034	13.87%	1.833%
18	10.357	1194	1202	1216	rBV	960087	1593618	22.53%	2.977%
19	10.522	1224	1230	1242	rBV	63549	122354	1.73%	0.229%
20	10.740	1259	1267	1278	rVB	895445	1498367	21.18%	2.799%
21	10.869	1281	1289	1300	rBV	911360	1559538	22.05%	2.913%
22	12.328	1526	1537	1544	rBV2	21955	38326	0.54%	0.072%
23	12.945	1635	1642	1644	rBV6	6766	10772	0.15%	0.020%
24	13.187	1679	1683	1688	rVB6	7821	11725	0.17%	0.022%
25	13.545	1738	1744	1748	rVV8	5182	8246	0.12%	0.015%
26	13.981	1812	1818	1833	rBV	1892285	2613142	36.94%	4.881%
27	14.263	1856	1866	1876	rBV	2127702	3054639	43.18%	5.706%
28	14.569	1910	1918	1934	rBV	1324414	2015763	28.50%	3.765%
29	14.763	1943	1951	1963	rBV	148705	254617	3.60%	0.476%
30	14.992	1986	1990	1993	rBV6	7096	9677	0.14%	0.018%
31	15.386	2053	2057	2062	rBV4	6853	10652	0.15%	0.020%
32	15.569	2079	2088	2097	rBV	2758905	4147389	58.63%	7.747%
33	15.681	2101	2107	2122	rBV	829614	1164447	16.46%	2.175%
34	15.804	2124	2128	2133	rBV2	17918	28069	0.40%	0.052%
35	16.133	2178	2184	2190	rVB9	6235	11998	0.17%	0.022%
36	16.263	2195	2206	2210	rBV5	13387	35891	0.51%	0.067%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP102521\
 Data File : BP007715.D
 Acq On : 27 Oct 2021 12:35
 Operator : CG/JU
 Sample : M4304-08
 Misc :
 ALS Vial : 72 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 P067-TW001-01

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF Filtering: 5
 Sampling : 1 Min Area: 0.1 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SFAM-EPA-BP102521.M
 Title : SVOA CALIBRATION

37	16.998	2328	2331	2338	rVB9	4830	7734	0.11%	0.014%
38	17.104	2345	2349	2353	rBV4	8408	14431	0.20%	0.027%
39	17.328	2380	2387	2397	rBV	1690120	2455283	34.71%	4.586%
40	17.428	2397	2404	2415	rVV	3817611	5242000	74.11%	9.792%
41	17.522	2416	2420	2427	rVB7	23912	43901	0.62%	0.082%
42	18.010	2495	2503	2506	rBV7	17131	28512	0.40%	0.053%
43	18.222	2531	2539	2548	rBV3	54514	124040	1.75%	0.232%
44	19.239	2708	2712	2719	rBV2	50568	66939	0.95%	0.125%
45	19.304	2719	2723	2728	rBV	53449	76700	1.08%	0.143%
46	19.451	2746	2748	2753	rBV6	13757	16988	0.24%	0.032%
47	19.604	2772	2774	2777	rVB3	13397	10129	0.14%	0.019%
48	19.663	2778	2784	2797	rBV	4967974	6476562	91.56%	12.098%
49	21.133	3031	3034	3039	rBV2	112066	165408	2.34%	0.309%
50	21.416	3077	3082	3096	rBV	2213038	3034508	42.90%	5.668%
51	23.710	3464	3472	3481	rBV2	3600268	7073634	100.00%	13.213%
52	23.862	3491	3498	3513	rVB2	1491464	3157236	44.63%	5.898%




Sum of corrected areas: 53533986

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP102521\
Data File : BP007715.D
Acq On : 27 Oct 2021 12:35
Operator : CG/JU
Sample : M4304-08
Misc :
ALS Vial : 72 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
P067-TW001-01

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SFAM-EPA-BP102521.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

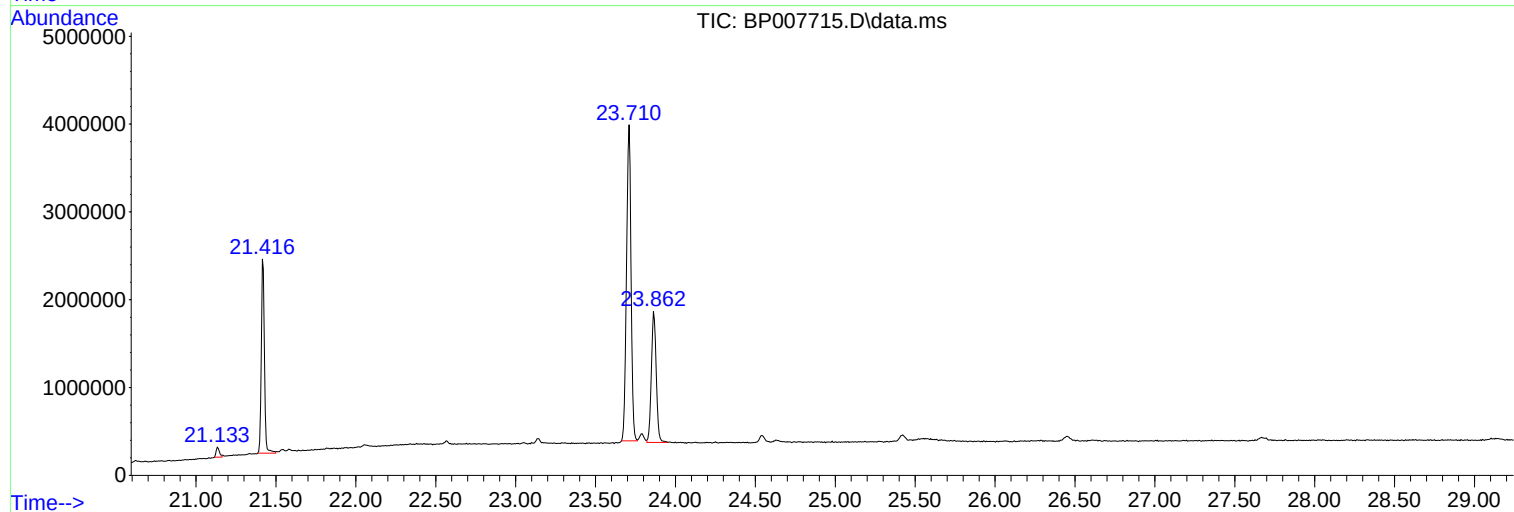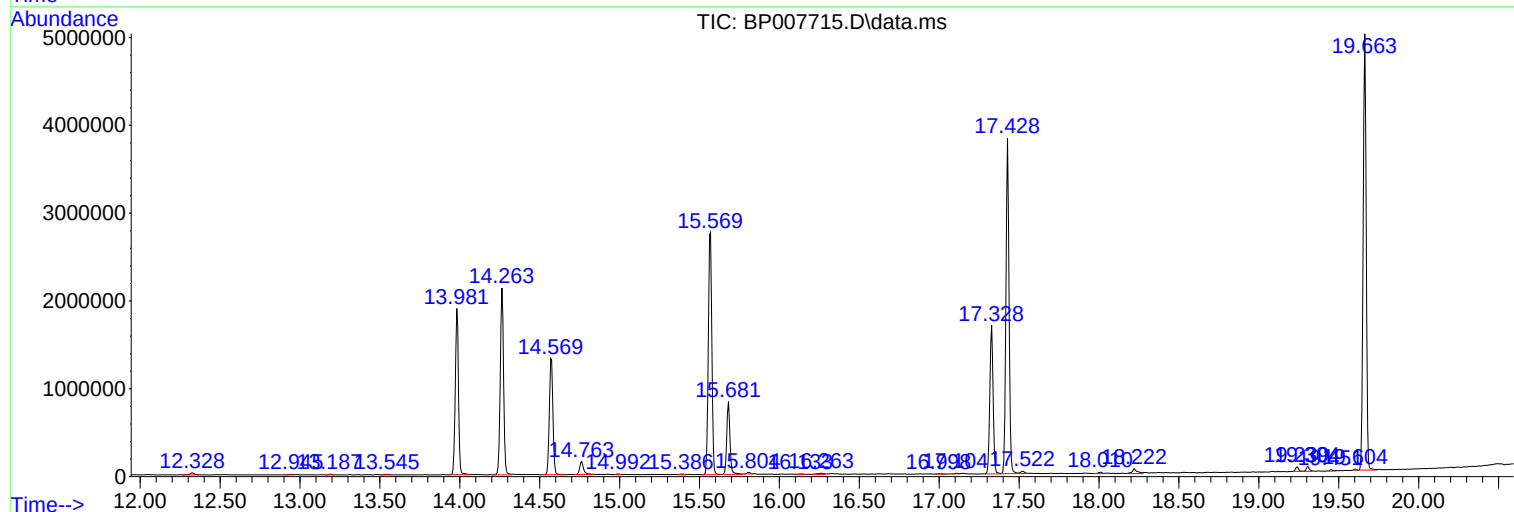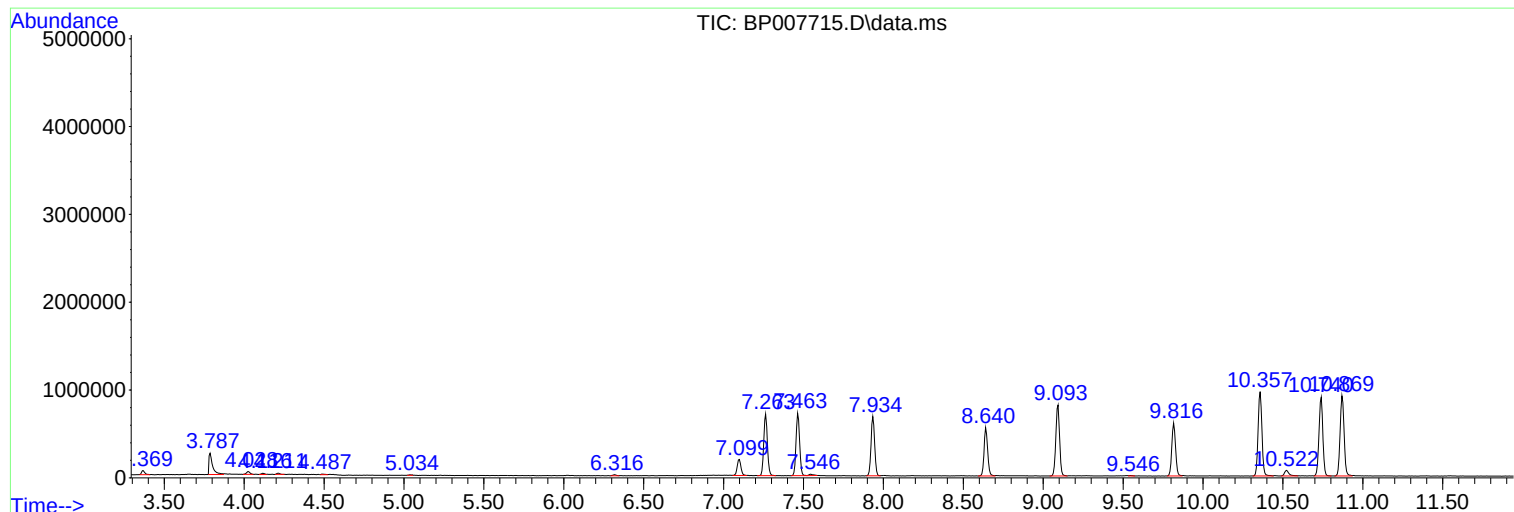

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP102521\
Data File : BP007715.D
Acq On : 27 Oct 2021 12:35
Operator : CG/JU
Sample : M4304-08
Misc :
ALS Vial : 72 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
P067-TW001-01

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SFAM-EPA-BP102521.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP102521\
Data File : BP007715.D
Acq On : 27 Oct 2021 12:35
Operator : CG/JU
Sample : M4304-08
Misc :
ALS Vial : 72 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
P067-TW001-01

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SFAM-EPA-BP102521.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------