

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP102521\
 Data File : BP007716.D
 Acq On : 27 Oct 2021 13:09
 Operator : CG/JU
 Sample : M4304-09
 Misc :
 ALS Vial : 73 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 P068-TW001-01

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SFAM-EPA-BP102521.M
 Title : SVOA CALIBRATION

Signal : TIC: BP007716.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.369	10	14	20	rVB	51469	63959	0.92%	0.113%
2	3.793	84	86	95	rBV	94618	158337	2.27%	0.280%
3	4.022	121	125	131	rVB	37478	56322	0.81%	0.100%
4	4.116	137	141	147	rVB2	14645	20076	0.29%	0.036%
5	4.216	153	158	163	rBV5	16257	24943	0.36%	0.044%
6	5.040	294	298	303	rVB4	6174	9792	0.14%	0.017%
7	5.634	393	399	402	rBV8	3763	9256	0.13%	0.016%
8	6.316	510	515	523	rVB3	12715	22105	0.32%	0.039%
9	7.093	640	647	658	rVB	214943	357392	5.13%	0.633%
10	7.263	669	676	685	rVB	769396	1211550	17.38%	2.146%
11	7.463	703	710	722	rBV	796322	1232139	17.67%	2.182%
12	7.569	724	728	734	rVB9	5611	9853	0.14%	0.017%
13	7.934	783	790	799	rBV	772115	1221121	17.52%	2.163%
14	8.640	903	910	919	rBV	629635	979637	14.05%	1.735%
15	9.087	978	986	996	rBV	878823	1461394	20.96%	2.588%
16	9.269	1012	1017	1021	rBV8	5846	9390	0.13%	0.017%
17	9.551	1060	1065	1069	rVB6	6989	11760	0.17%	0.021%
18	9.816	1102	1110	1124	rBV	679075	1119920	16.06%	1.983%
19	10.357	1194	1202	1212	rBV	1061226	1795604	25.76%	3.180%
20	10.522	1223	1230	1240	rBV	82690	156956	2.25%	0.278%
21	10.734	1257	1266	1275	rBV	1022000	1754879	25.17%	3.108%
22	10.869	1281	1289	1299	rBV	126428	232270	3.33%	0.411%
23	12.040	1486	1488	1495	rVB8	3742	6984	0.10%	0.012%
24	12.322	1530	1536	1542	rBV	24492	44291	0.64%	0.078%
25	13.187	1679	1683	1686	rBV6	6582	7369	0.11%	0.013%
26	13.475	1726	1732	1737	rBV9	5267	10440	0.15%	0.018%
27	13.539	1739	1743	1748	rVB5	6306	9201	0.13%	0.016%
28	13.981	1810	1818	1824	rBV	2098298	2871105	41.18%	5.085%
29	14.263	1857	1866	1878	rBV	2315644	3451094	49.50%	6.112%
30	14.569	1911	1918	1932	rVB	1663912	2440505	35.01%	4.322%
31	14.757	1942	1950	1964	rBV	175116	306738	4.40%	0.543%
32	14.992	1985	1990	1993	rBV7	4783	8437	0.12%	0.015%
33	15.386	2053	2057	2061	rBV7	5474	7932	0.11%	0.014%
34	15.563	2079	2087	2099	rBV	3064209	4439302	63.68%	7.862%
35	15.681	2100	2107	2114	rBV	847041	1192089	17.10%	2.111%
36	15.804	2124	2128	2133	rVB3	22269	33684	0.48%	0.060%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP102521\
 Data File : BP007716.D
 Acq On : 27 Oct 2021 13:09
 Operator : CG/JU
 Sample : M4304-09
 Misc :
 ALS Vial : 73 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 P068-TW001-01

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF Filtering: 5
 Sampling : 1 Min Area: 0.1 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SFAM-EPA-BP102521.M
 Title : SVOA CALIBRATION

37	16.010	2160	2163	2170	rVB9	4522	8473	0.12%	0.015%
38	16.128	2181	2183	2188	rBV6	5215	7604	0.11%	0.013%
39	16.257	2199	2205	2210	rBV5	14518	26953	0.39%	0.048%
40	17.004	2326	2332	2337	rBV9	7003	14212	0.20%	0.025%
41	17.110	2345	2350	2355	rBV2	11142	19627	0.28%	0.035%
42	17.327	2379	2387	2397	rBV	2008100	3003778	43.09%	5.320%
43	17.427	2397	2404	2415	rVV	3506028	5279519	75.73%	9.350%
44	18.004	2497	2502	2507	rBV3	24108	35867	0.51%	0.064%
45	18.216	2534	2538	2547	rBV	51971	81177	1.16%	0.144%
46	18.516	2585	2589	2592	rBV5	8628	13151	0.19%	0.023%
47	19.233	2708	2711	2716	rBV2	50227	64285	0.92%	0.114%
48	19.304	2719	2723	2729	rBV	56389	82572	1.18%	0.146%
49	19.451	2746	2748	2752	rBV4	19284	18969	0.27%	0.034%
50	19.598	2771	2773	2777	rVB4	16903	17683	0.25%	0.031%
51	19.657	2778	2783	2790	rVV	4577596	6488374	93.07%	11.491%
52	20.563	2934	2937	2942	rVB2	81252	96653	1.39%	0.171%
53	21.133	3031	3034	3043	rBV4	79448	103046	1.48%	0.183%
54	21.416	3077	3082	3089	rBV	2758901	3625312	52.00%	6.421%
55	23.704	3463	3471	3480	rBV2	3467111	6971536	100.00%	12.347%
56	23.862	3491	3498	3507	rVB2	1828268	3756214	53.88%	6.653%




Sum of corrected areas: 56462831

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP102521\
Data File : BP007716.D
Acq On : 27 Oct 2021 13:09
Operator : CG/JU
Sample : M4304-09
Misc :
ALS Vial : 73 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
P068-TW001-01

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SFAM-EPA-BP102521.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

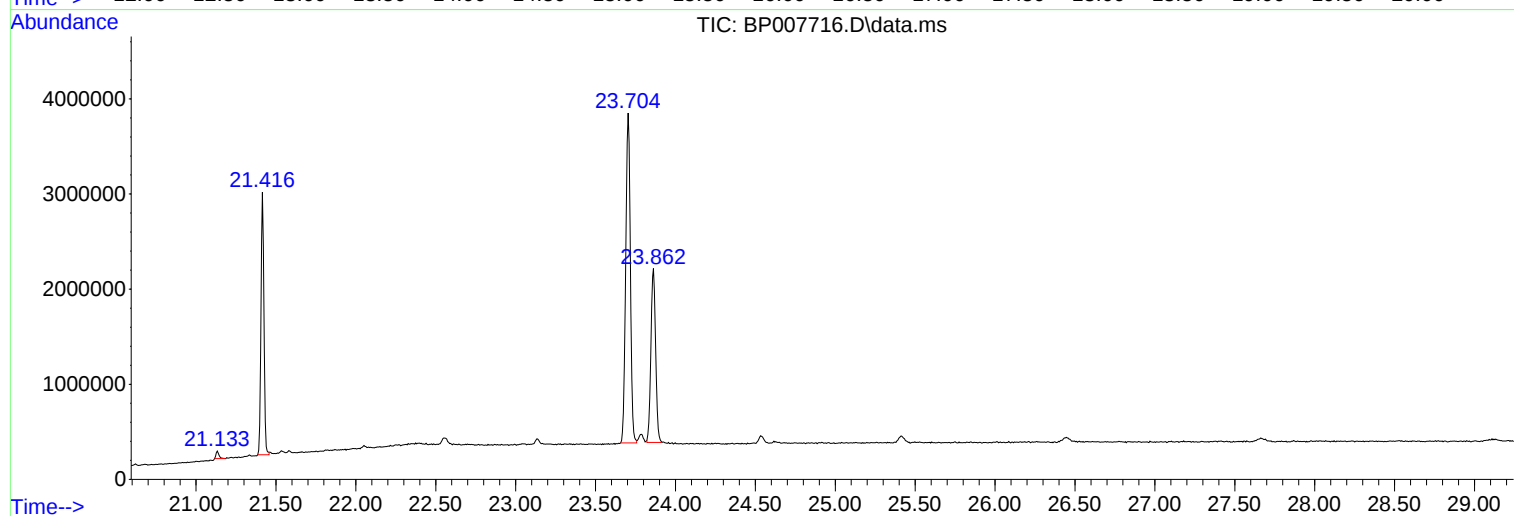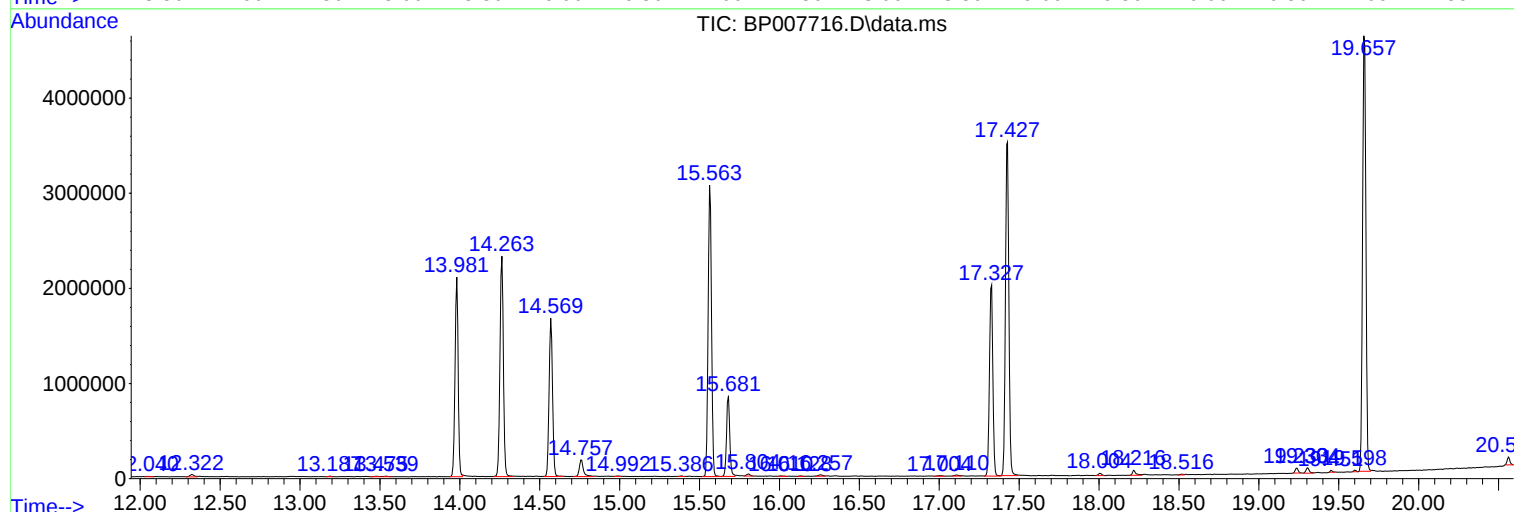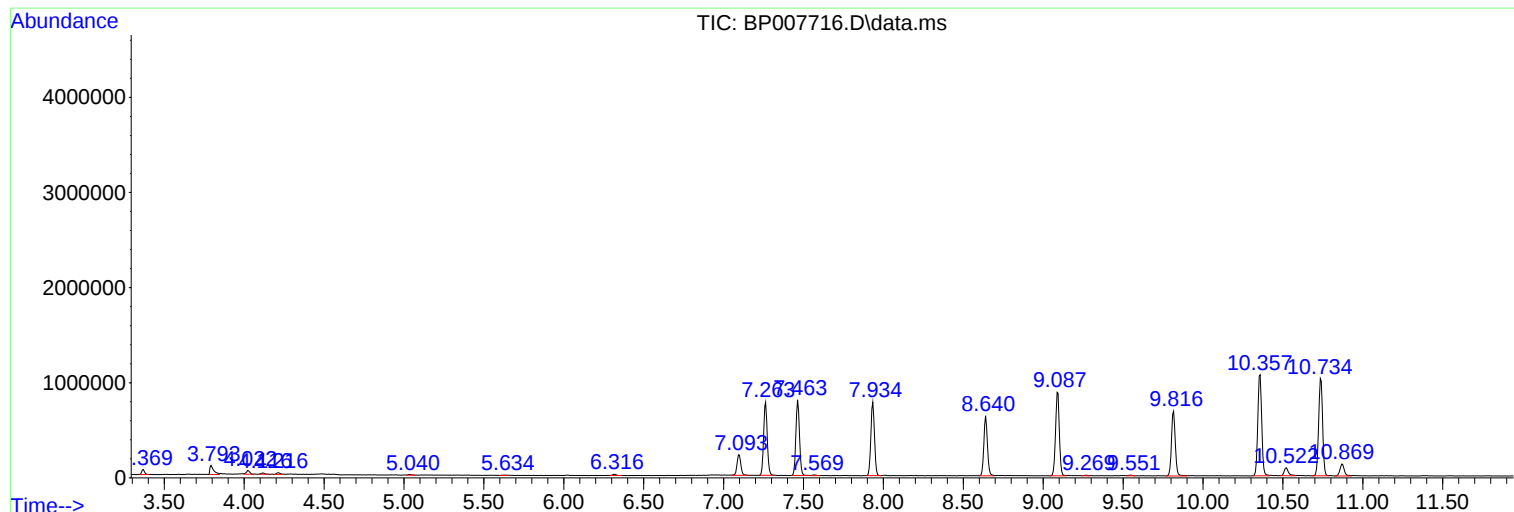

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP102521\
Data File : BP007716.D
Acq On : 27 Oct 2021 13:09
Operator : CG/JU
Sample : M4304-09
Misc :
ALS Vial : 73 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
P068-TW001-01

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SFAM-EPA-BP102521.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP102521\
Data File : BP007716.D
Acq On : 27 Oct 2021 13:09
Operator : CG/JU
Sample : M4304-09
Misc :
ALS Vial : 73 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
P068-TW001-01

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SFAM-EPA-BP102521.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------