

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP102521\
 Data File : BP007717.D
 Acq On : 27 Oct 2021 13:43
 Operator : CG/JU
 Sample : M4304-10
 Misc :
 ALS Vial : 74 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 P069-TW001-01

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SFAM-EPA-BP102521.M
 Title : SVOA CALIBRATION

Signal : TIC: BP007717.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.370	10	14	19	rBV	42414	53052	0.67%	0.081%
2	3.787	82	85	103	rBV	254695	413122	5.25%	0.629%
3	4.028	121	126	133	rVB	41967	66899	0.85%	0.102%
4	4.122	137	142	149	rVB3	15156	24610	0.31%	0.037%
5	4.211	154	157	161	rVB2	16041	21509	0.27%	0.033%
6	5.040	294	298	301	rVB3	7505	10065	0.13%	0.015%
7	6.316	510	515	523	rVB	14964	24189	0.31%	0.037%
8	7.093	641	647	662	rVB	280150	449727	5.72%	0.685%
9	7.263	669	676	686	rVB	872228	1418554	18.04%	2.159%
10	7.463	703	710	722	rBV	928586	1459142	18.55%	2.221%
11	7.569	724	728	733	rVB7	6895	12600	0.16%	0.019%
12	7.934	781	790	799	rBV	835363	1332768	16.95%	2.029%
13	8.640	903	910	921	rBV	753225	1213016	15.42%	1.846%
14	9.087	979	986	1000	rBV	1026596	1697138	21.58%	2.583%
15	9.222	1005	1009	1013	rVV7	4851	8172	0.10%	0.012%
16	9.546	1060	1064	1070	rVB8	6059	11203	0.14%	0.017%
17	9.816	1100	1110	1121	rBV	792199	1315842	16.73%	2.003%
18	10.357	1193	1202	1217	rBV	1235655	2100471	26.71%	3.197%
19	10.516	1223	1229	1242	rBV	73624	136690	1.74%	0.208%
20	10.734	1258	1266	1275	rBV	1083869	1911110	24.30%	2.909%
21	10.869	1281	1289	1299	rBV	1155220	1928612	24.52%	2.936%
22	12.046	1481	1489	1496	rVB	3582	9335	0.12%	0.014%
23	12.322	1530	1536	1543	rBV	26283	45436	0.58%	0.069%
24	12.940	1637	1641	1647	rBV8	4203	7950	0.10%	0.012%
25	13.187	1678	1683	1687	rBV5	6342	10370	0.13%	0.016%
26	13.475	1727	1732	1737	rBV8	4648	8959	0.11%	0.014%
27	13.540	1739	1743	1748	rVB5	5664	9263	0.12%	0.014%
28	13.981	1811	1818	1835	rVV	2351164	3286381	41.79%	5.002%
29	14.263	1854	1866	1881	rBV	2734215	3983575	50.65%	6.064%
30	14.569	1911	1918	1930	rBV	1825198	2649777	33.69%	4.033%
31	14.757	1944	1950	1964	rBV	220561	355108	4.52%	0.541%
32	14.987	1983	1989	1995	rVB9	13438	21432	0.27%	0.033%
33	15.387	2052	2057	2063	rBV9	5986	9706	0.12%	0.015%
34	15.563	2080	2087	2098	rBV	3522720	5125212	65.17%	7.801%
35	15.681	2100	2107	2119	rVV	964638	1355819	17.24%	2.064%
36	15.804	2123	2128	2132	rVB	25412	39506	0.50%	0.060%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP102521\
 Data File : BP007717.D
 Acq On : 27 Oct 2021 13:43
 Operator : CG/JU
 Sample : M4304-10
 Misc :
 ALS Vial : 74 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 P069-TW001-01

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF Filtering: 5
 Sampling : 1 Min Area: 0.1 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SFAM-EPA-BP102521.M
 Title : SVOA CALIBRATION

37	16.004	2157	2162	2165	rBV6	4620	8146	0.10%	0.012%
38	16.257	2198	2205	2210	rBV10	7530	17225	0.22%	0.026%
39	16.351	2218	2221	2227	rVB7	6463	12010	0.15%	0.018%
40	17.010	2327	2333	2335	rVB6	5593	8594	0.11%	0.013%
41	17.104	2344	2349	2353	rBV3	13828	22545	0.29%	0.034%
42	17.328	2379	2387	2396	rBV	2162878	3239425	41.19%	4.931%
43	17.428	2397	2404	2416	rVV	3911829	5896752	74.98%	8.976%
44	17.522	2416	2420	2425	rVB7	12710	22548	0.29%	0.034%
45	18.004	2497	2502	2509	rVB2	30738	44246	0.56%	0.067%
46	18.216	2534	2538	2544	rBV2	58012	87719	1.12%	0.134%
47	18.286	2547	2550	2556	rVB	10750	15360	0.20%	0.023%
48	19.239	2707	2712	2717	rBV	59232	83953	1.07%	0.128%
49	19.304	2719	2723	2728	rVV	62593	82882	1.05%	0.126%
50	19.457	2745	2749	2756	rBV7	19889	34409	0.44%	0.052%
51	19.598	2770	2773	2777	rBV4	19546	24987	0.32%	0.038%
52	19.663	2777	2784	2791	rBV	5137521	7190140	91.42%	10.944%
53	21.133	3030	3034	3042	rBV2	135120	229697	2.92%	0.350%
54	21.416	3077	3082	3088	rBV	2983893	3878236	49.31%	5.903%
55	22.551	3271	3275	3285	rVB4	155181	273783	3.48%	0.417%
56	23.704	3463	3471	3480	rBV2	3880633	7864882	100.00%	11.971%
57	23.863	3490	3498	3508	rVB2	1994793	4133644	52.56%	6.292%




Sum of corrected areas: 65697503

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP102521\
Data File : BP007717.D
Acq On : 27 Oct 2021 13:43
Operator : CG/JU
Sample : M4304-10
Misc :
ALS Vial : 74 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
P069-TW001-01

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SFAM-EPA-BP102521.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

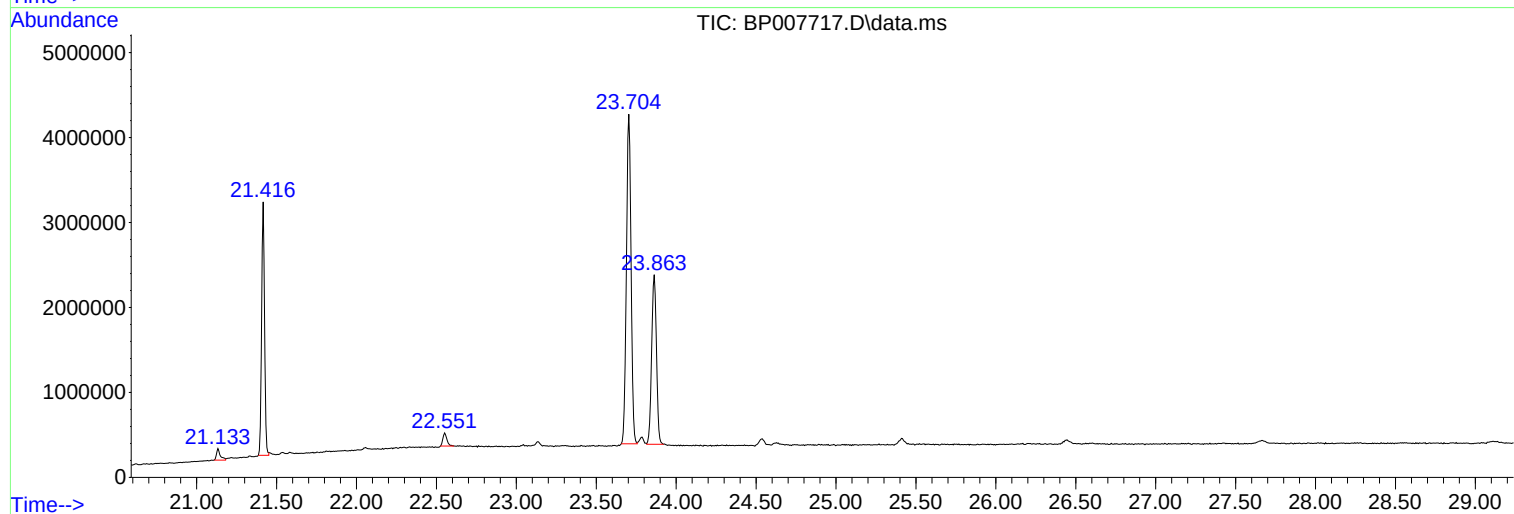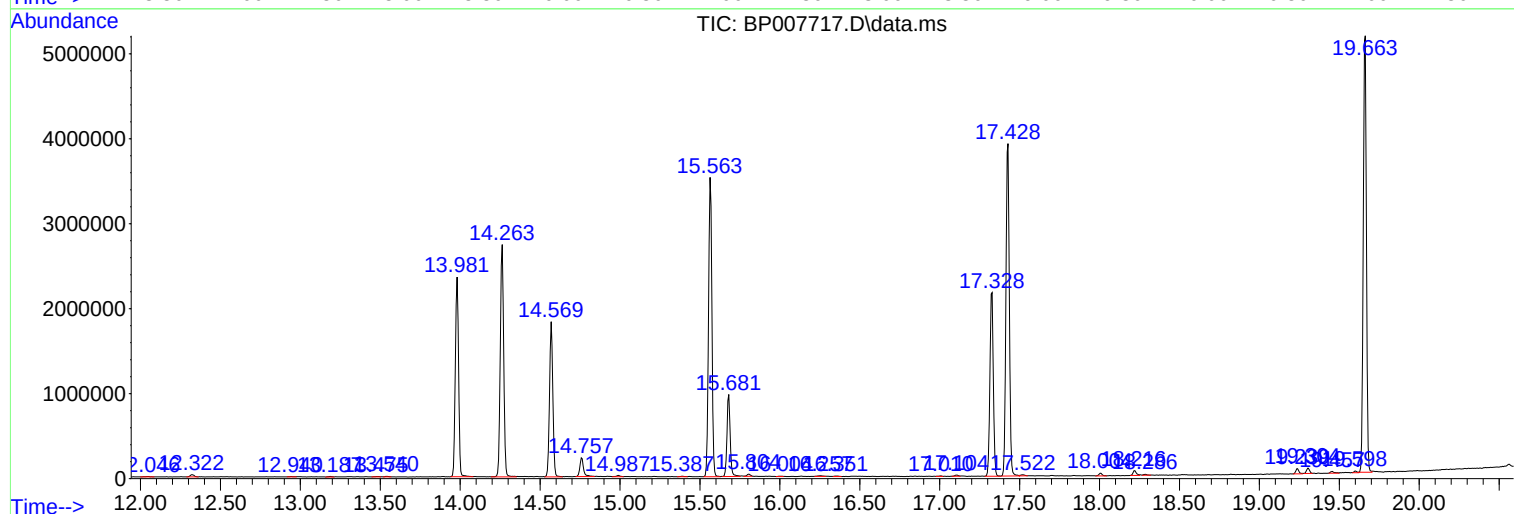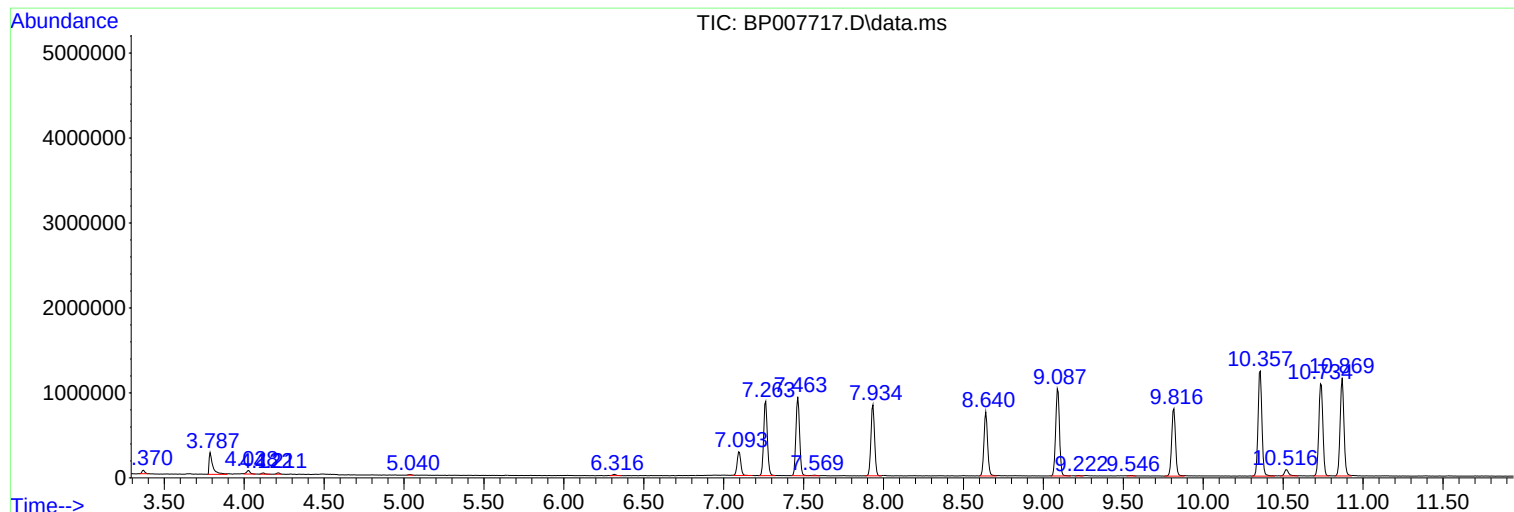

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP102521\
Data File : BP007717.D
Acq On : 27 Oct 2021 13:43
Operator : CG/JU
Sample : M4304-10
Misc :
ALS Vial : 74 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
P069-TW001-01

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SFAM-EPA-BP102521.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP102521\
Data File : BP007717.D
Acq On : 27 Oct 2021 13:43
Operator : CG/JU
Sample : M4304-10
Misc :
ALS Vial : 74 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
P069-TW001-01

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SFAM-EPA-BP102521.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------