

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP102521\
 Data File : BP007718.D
 Acq On : 27 Oct 2021 14:17
 Operator : CG/JU
 Sample : M4304-11
 Misc :
 ALS Vial : 75 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 P073-TW001-01

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SFAM-EPA-BP102521.M
 Title : SVOA CALIBRATION

Signal : TIC: BP007718.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.364	9	13	19	rBV	41711	56146	0.75%	0.097%
2	3.787	82	85	100	rBV	198583	317988	4.23%	0.547%
3	4.022	121	125	130	rVB	38441	59032	0.78%	0.102%
4	4.117	137	141	149	rVB2	14814	26666	0.35%	0.046%
5	4.211	153	157	165	rVB5	16927	26013	0.35%	0.045%
6	5.034	293	297	302	rVB3	5882	11093	0.15%	0.019%
7	6.316	511	515	520	rVB4	12644	19591	0.26%	0.034%
8	7.093	641	647	658	rVB	216479	351324	4.67%	0.604%
9	7.263	668	676	687	rVB	740532	1218182	16.19%	2.096%
10	7.463	703	710	722	rVV	779215	1200608	15.96%	2.066%
11	7.934	783	790	798	rBV	656701	1061969	14.12%	1.827%
12	7.999	798	801	809	rVB8	5613	11855	0.16%	0.020%
13	8.640	901	910	918	rBV	630703	987580	13.13%	1.699%
14	9.087	979	986	998	rBV	892150	1471704	19.56%	2.532%
15	9.816	1102	1110	1125	rBV	667750	1089625	14.48%	1.875%
16	10.352	1194	1201	1218	rBV	1044598	1774699	23.59%	3.053%
17	10.516	1224	1229	1239	rBV	81254	148969	1.98%	0.256%
18	10.734	1259	1266	1277	rVB	895177	1526168	20.29%	2.626%
19	10.869	1281	1289	1299	rBV	974751	1667401	22.17%	2.869%
20	12.051	1484	1490	1494	rBV9	4472	7876	0.10%	0.014%
21	12.322	1531	1536	1544	rBV	23503	41563	0.55%	0.072%
22	12.940	1637	1641	1647	rBV5	8120	13675	0.18%	0.024%
23	13.187	1675	1683	1687	rBV5	10504	17121	0.23%	0.029%
24	13.481	1729	1733	1737	rBV6	7030	10550	0.14%	0.018%
25	13.545	1737	1744	1746	rBV6	5733	8029	0.11%	0.014%
26	13.981	1810	1818	1831	rBV	2164765	3028249	40.26%	5.210%
27	14.263	1854	1866	1876	rBV	2364600	3561248	47.34%	6.127%
28	14.569	1910	1918	1931	rBV	1433840	2108199	28.03%	3.627%
29	14.757	1943	1950	1961	rBV	184269	304982	4.05%	0.525%
30	14.987	1985	1989	1996	rBV5	18773	29573	0.39%	0.051%
31	15.387	2053	2057	2062	rBV3	12036	18451	0.25%	0.032%
32	15.563	2079	2087	2098	rBV	3281315	4723650	62.79%	8.127%
33	15.681	2100	2107	2123	rVV	875276	1255390	16.69%	2.160%
34	15.804	2123	2128	2134	rVB3	23173	39837	0.53%	0.069%
35	16.010	2160	2163	2168	rVB6	4713	7559	0.10%	0.013%
36	16.134	2179	2184	2189	rBV9	5174	8975	0.12%	0.015%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP102521\
 Data File : BP007718.D
 Acq On : 27 Oct 2021 14:17
 Operator : CG/JU
 Sample : M4304-11
 Misc :
 ALS Vial : 75 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 P073-TW001-01

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF Filtering: 5
 Sampling : 1 Min Area: 0.1 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SFAM-EPA-BP102521.M
 Title : SVOA CALIBRATION

37	16.257	2199	2205	2210	rBV	19675	37141	0.49%	0.064%
38	16.469	2236	2241	2245	rBV7	7052	11517	0.15%	0.020%
39	16.998	2328	2331	2335	rBV6	5699	7684	0.10%	0.013%
40	17.104	2344	2349	2358	rBV7	12768	29276	0.39%	0.050%
41	17.322	2380	2386	2396	rBV	1756262	2562348	34.06%	4.409%
42	17.428	2397	2404	2415	rVV	3804311	5683348	75.55%	9.778%
43	17.522	2416	2420	2428	rVB10	19164	32498	0.43%	0.056%
44	17.628	2433	2438	2443	rBV7	5100	10360	0.14%	0.018%
45	17.704	2447	2451	2454	rBV3	4864	7902	0.11%	0.014%
46	18.004	2498	2502	2507	rBV	34005	43498	0.58%	0.075%
47	18.216	2534	2538	2546	rBV2	98739	152317	2.02%	0.262%
48	18.286	2547	2550	2554	rVB	20135	25187	0.33%	0.043%
49	19.233	2707	2711	2716	rBV2	57311	81712	1.09%	0.141%
50	19.304	2719	2723	2731	rVB	63288	91373	1.21%	0.157%
51	19.451	2745	2748	2754	rBV2	51361	71520	0.95%	0.123%
52	19.604	2771	2774	2777	rBV5	14945	15495	0.21%	0.027%
53	19.663	2777	2784	2791	rBV	5013878	6976489	92.74%	12.003%
54	21.133	3031	3034	3040	rBV4	101953	148120	1.97%	0.255%
55	21.416	3077	3082	3094	rBV	2380519	3109747	41.34%	5.350%
56	23.704	3463	3471	3480	rBV	3694854	7522529	100.00%	12.943%
57	23.863	3491	3498	3512	rVB2	1590621	3290354	43.74%	5.661%




Sum of corrected areas: 58121955

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP102521\
Data File : BP007718.D
Acq On : 27 Oct 2021 14:17
Operator : CG/JU
Sample : M4304-11
Misc :
ALS Vial : 75 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
P073-TW001-01

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SFAM-EPA-BP102521.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

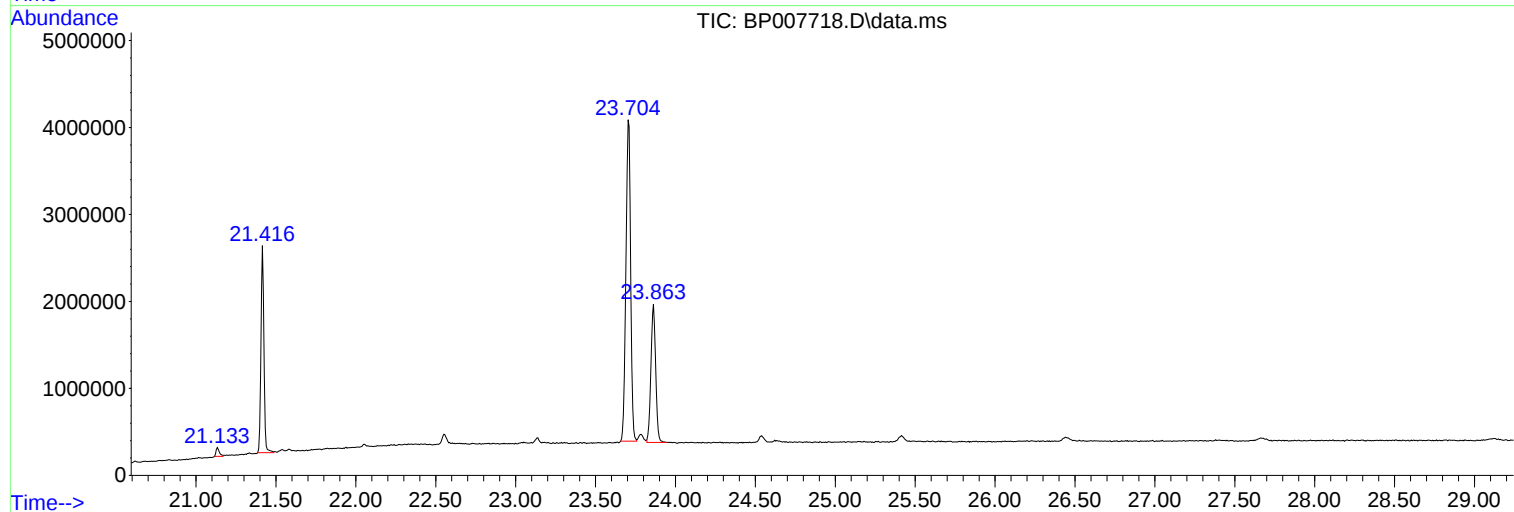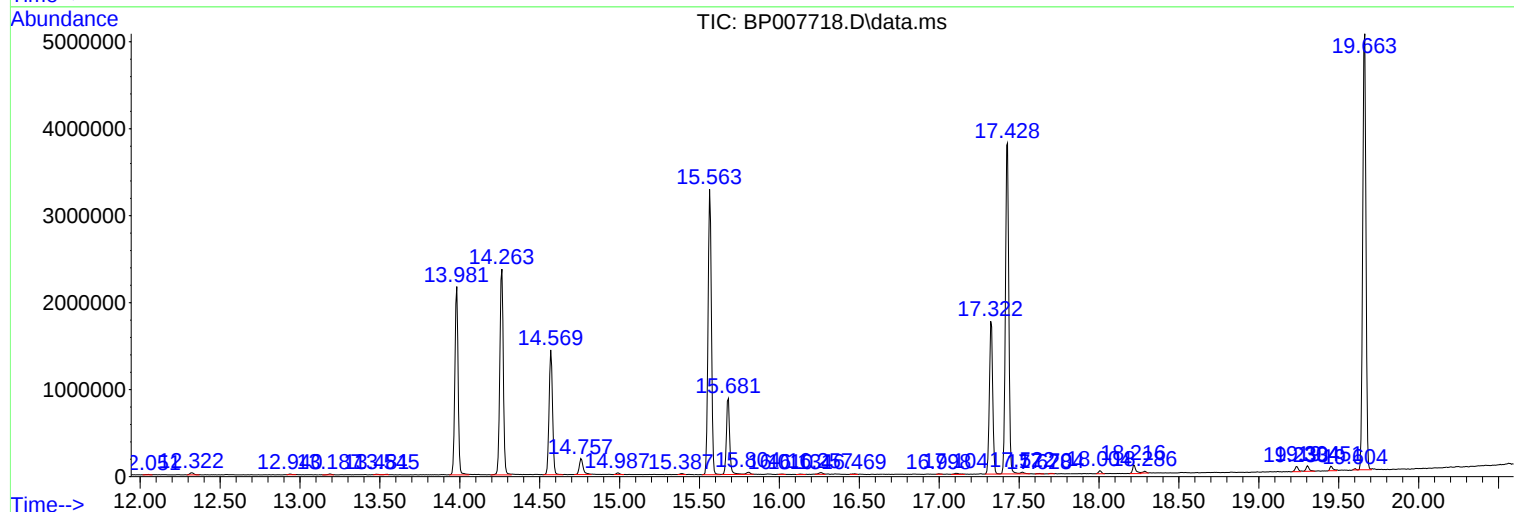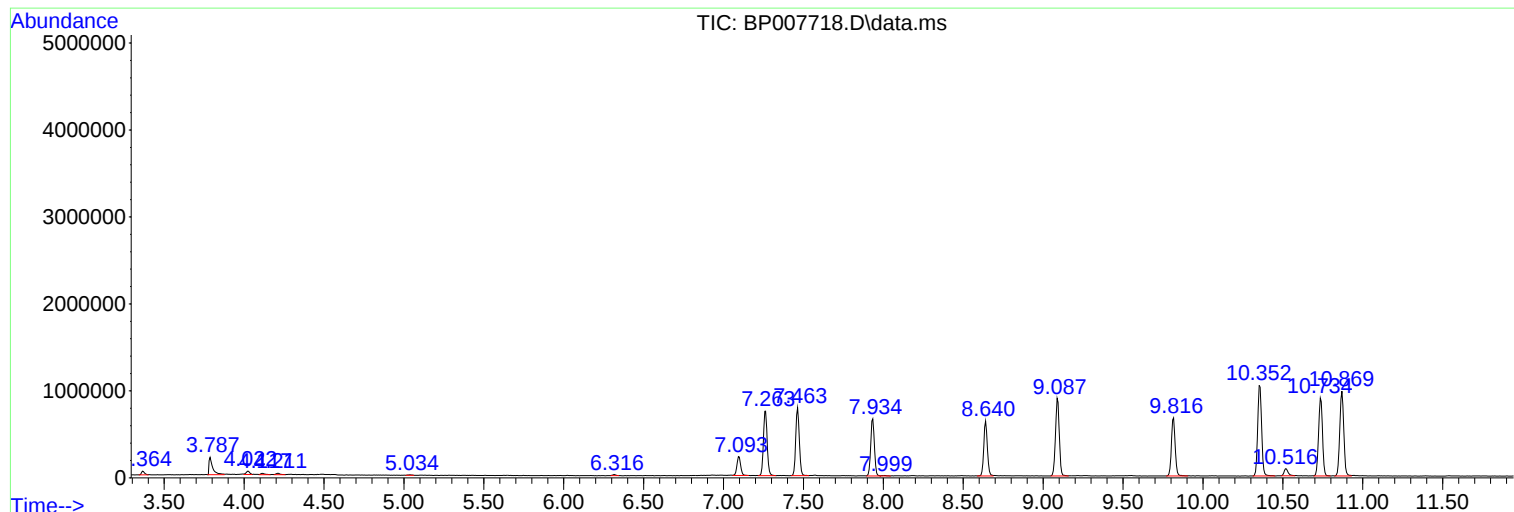

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP102521\
Data File : BP007718.D
Acq On : 27 Oct 2021 14:17
Operator : CG/JU
Sample : M4304-11
Misc :
ALS Vial : 75 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
P073-TW001-01

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SFAM-EPA-BP102521.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP102521\
Data File : BP007718.D
Acq On : 27 Oct 2021 14:17
Operator : CG/JU
Sample : M4304-11
Misc :
ALS Vial : 75 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
P073-TW001-01

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SFAM-EPA-BP102521.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------