

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP102521\
 Data File : BP007721.D
 Acq On : 27 Oct 2021 16:05
 Operator : CG/JU
 Sample : PB140206BL
 Misc :
 ALS Vial : 78 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SBLK206

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SFAM-EPA-BP102521.M
 Title : SVOA CALIBRATION

Signal : TIC: BP007721.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.364	10	13	20	rBV	61087	79207	1.36%	0.137%
2	3.781	81	84	106	rBV	799182	1264843	21.67%	2.188%
3	4.111	137	140	146	rVB2	13481	21466	0.37%	0.037%
4	7.099	641	648	664	rVB	876375	1424425	24.41%	2.463%
5	7.264	669	676	689	rVB	718243	1149943	19.70%	1.989%
6	7.464	703	710	724	rVB	928333	1448457	24.82%	2.505%
7	7.934	783	790	800	rVB	790551	1246074	21.35%	2.155%
8	8.640	902	910	922	rBV	1113516	1766009	30.26%	3.054%
9	9.093	978	987	997	rBV	807009	1360592	23.31%	2.353%
10	9.816	1103	1110	1124	rBV	647363	1065550	18.26%	1.843%
11	10.358	1194	1202	1213	rBV	1095498	1806079	30.95%	3.124%
12	10.740	1257	1267	1275	rBV	1055360	1784580	30.58%	3.086%
13	10.869	1281	1289	1309	rBV	1079775	1851629	31.73%	3.202%
14	12.328	1530	1537	1542	rBV	20353	39404	0.68%	0.068%
15	13.540	1739	1743	1748	rVB7	5871	9634	0.17%	0.017%
16	13.981	1811	1818	1832	rBV	2017032	2748721	47.10%	4.754%
17	14.263	1858	1866	1876	rBV	2227493	3197726	54.79%	5.530%
18	14.569	1911	1918	1933	rBV	1747629	2498473	42.81%	4.321%
19	14.757	1944	1950	1965	rBV	866189	1308111	22.42%	2.262%
20	15.563	2080	2087	2097	rBV	2822394	4116457	70.54%	7.119%
21	15.681	2101	2107	2117	rBV	727210	997312	17.09%	1.725%
22	15.804	2124	2128	2133	rVB2	18882	29105	0.50%	0.050%
23	16.351	2219	2221	2229	rVB9	4280	7569	0.13%	0.013%
24	16.998	2327	2331	2338	rVB10	4848	8428	0.14%	0.015%
25	17.110	2344	2350	2355	rBV2	10602	17074	0.29%	0.030%
26	17.322	2379	2386	2396	rBV	2100873	3074732	52.69%	5.318%
27	17.422	2397	2403	2416	rBV2	3081728	4506846	77.23%	7.794%
28	19.233	2707	2711	2716	rBV3	45473	63923	1.10%	0.111%
29	19.304	2719	2723	2728	rVV	44701	60715	1.04%	0.105%
30	19.657	2777	2783	2797	rBV	4174355	5544737	95.01%	9.589%
31	21.416	3077	3082	3094	rBV	2731116	3627581	62.16%	6.274%
32	23.704	3463	3471	3480	rBV	3009757	5835861	100.00%	10.093%
33	23.857	3491	3497	3512	rVB2	1829736	3860098	66.14%	6.676%




Sum of corrected areas: 57821361

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP102521\
Data File : BP007721.D
Acq On : 27 Oct 2021 16:05
Operator : CG/JU
Sample : PB140206BL
Misc :
ALS Vial : 78 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK206

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SFAM-EPA-BP102521.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

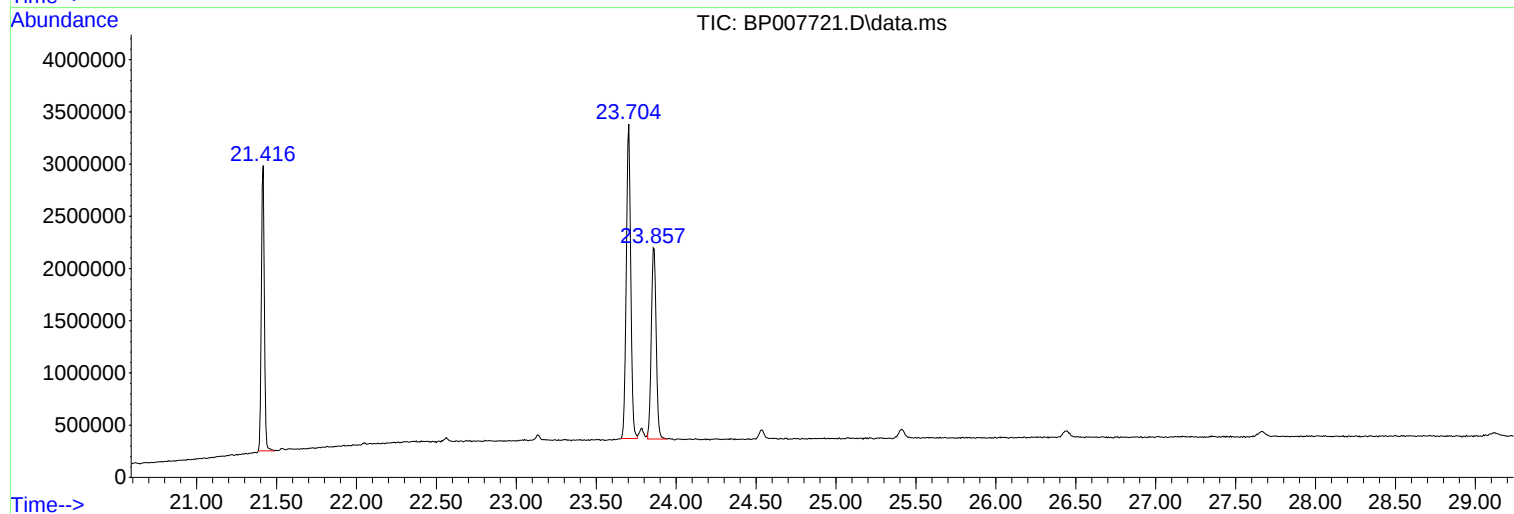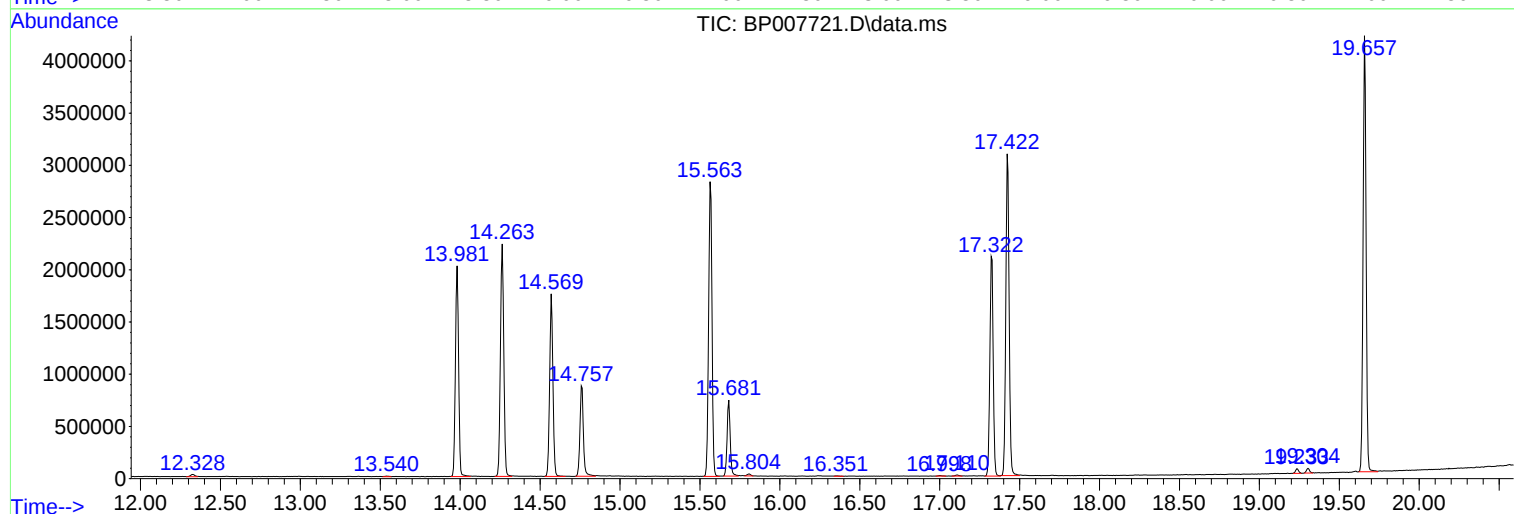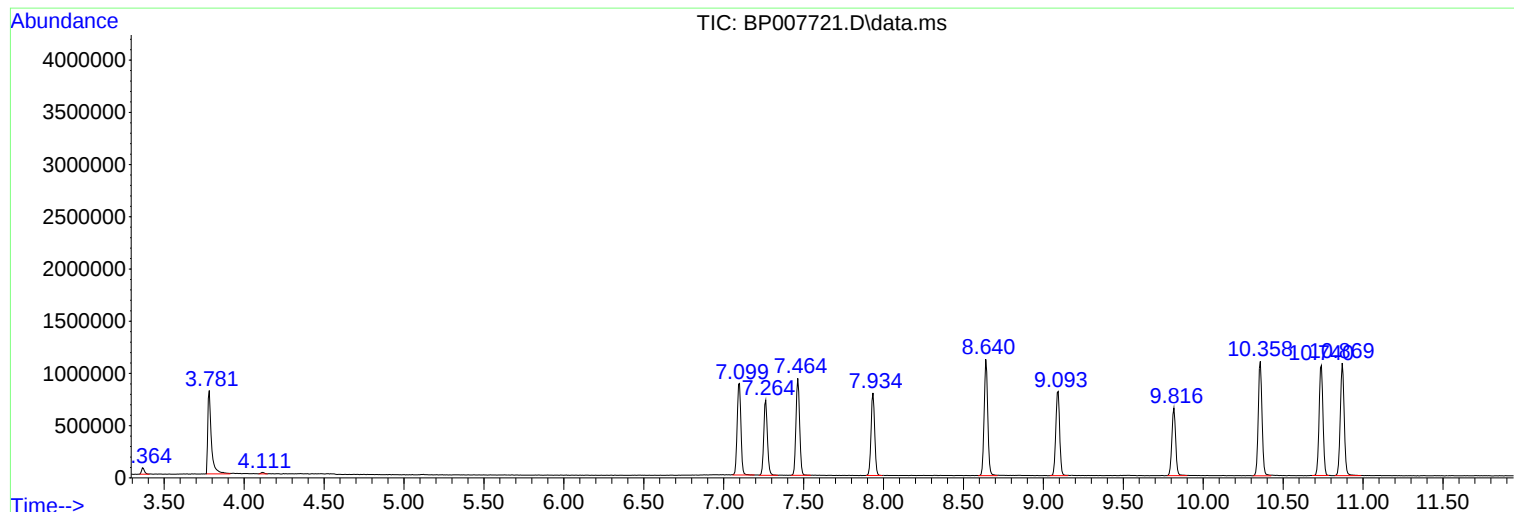

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP102521\
Data File : BP007721.D
Acq On : 27 Oct 2021 16:05
Operator : CG/JU
Sample : PB140206BL
Misc :
ALS Vial : 78 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK206

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SFAM-EPA-BP102521.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP102521\
Data File : BP007721.D
Acq On : 27 Oct 2021 16:05
Operator : CG/JU
Sample : PB140206BL
Misc :
ALS Vial : 78 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK206

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SFAM-EPA-BP102521.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
