

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP102521\
 Data File : BP007724.D
 Acq On : 27 Oct 2021 17:47
 Operator : CG/JU
 Sample : M4304-12
 Misc :
 ALS Vial : 81 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 P075-TW001-01

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SFAM-EPA-BP102521.M
 Title : SVOA CALIBRATION

Signal : TIC: BP007724.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.363	9	13	20	rVB	46253	60172	0.82%	0.101%
2	3.787	83	85	99	rBV	202184	329104	4.48%	0.554%
3	4.022	121	125	132	rVB	40218	59118	0.80%	0.099%
4	4.116	137	141	146	rVB	13764	19656	0.27%	0.033%
5	4.216	154	158	165	rVB3	14796	22570	0.31%	0.038%
6	5.046	294	299	304	rVB4	11244	19071	0.26%	0.032%
7	6.316	510	515	521	rBV2	15248	23820	0.32%	0.040%
8	7.093	642	647	657	rVB	227140	371797	5.06%	0.625%
9	7.263	669	676	689	rVB	752419	1229086	16.72%	2.067%
10	7.463	703	710	722	rBV	809202	1253196	17.05%	2.108%
11	7.934	781	790	797	rBV	738812	1173902	15.97%	1.974%
12	8.004	799	802	807	rVB3	6638	8668	0.12%	0.015%
13	8.640	903	910	920	rBV	639640	1010081	13.74%	1.699%
14	9.087	978	986	997	rBV	920226	1493346	20.32%	2.512%
15	9.263	1012	1016	1025	rVB10	3976	10393	0.14%	0.017%
16	9.545	1062	1064	1070	rVB6	10424	15974	0.22%	0.027%
17	9.816	1101	1110	1122	rBV	686972	1152181	15.68%	1.938%
18	10.357	1194	1202	1213	rBV	1056382	1806621	24.58%	3.039%
19	10.528	1225	1231	1237	rBV5	10815	21953	0.30%	0.037%
20	10.734	1258	1266	1277	rBV	980558	1683239	22.90%	2.831%
21	10.869	1282	1289	1308	rVB	954962	1668407	22.70%	2.806%
22	12.051	1486	1490	1497	rVB10	4737	9163	0.12%	0.015%
23	12.322	1531	1536	1542	rBV2	22141	37639	0.51%	0.063%
24	13.186	1678	1683	1688	rBV7	5972	11502	0.16%	0.019%
25	13.410	1717	1721	1725	rVB6	7026	9702	0.13%	0.016%
26	13.480	1727	1733	1737	rBV8	5916	10979	0.15%	0.018%
27	13.539	1740	1743	1750	rVB5	6453	10908	0.15%	0.018%
28	13.980	1811	1818	1824	rBV	2173480	3043033	41.41%	5.118%
29	14.263	1855	1866	1876	rBV	2415784	3590517	48.86%	6.039%
30	14.569	1911	1918	1925	rBV	1608786	2327312	31.67%	3.914%
31	14.757	1943	1950	1964	rBV	185713	313848	4.27%	0.528%
32	14.933	1975	1980	1983	rBV7	4961	7943	0.11%	0.013%
33	14.986	1985	1989	1994	rVB8	10610	17316	0.24%	0.029%
34	15.386	2052	2057	2062	rBV4	12245	19275	0.26%	0.032%
35	15.563	2080	2087	2099	rBV	3272565	4772747	64.94%	8.027%
36	15.680	2101	2107	2122	rVV	872529	1244496	16.93%	2.093%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP102521\
 Data File : BP007724.D
 Acq On : 27 Oct 2021 17:47
 Operator : CG/JU
 Sample : M4304-12
 Misc :
 ALS Vial : 81 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 P075-TW001-01

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF Filtering: 5
 Sampling : 1 Min Area: 0.1 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SFAM-EPA-BP102521.M
 Title : SVOA CALIBRATION

37	15.804	2123	2128	2137	rVB2	25866	43750	0.60%	0.074%
38	15.939	2147	2151	2156	rBV8	4243	8038	0.11%	0.014%
39	16.251	2200	2204	2210	rBV8	6811	15161	0.21%	0.025%
40	16.351	2217	2221	2228	rBV9	6168	10624	0.14%	0.018%
41	16.469	2234	2241	2244	rBV9	4931	12276	0.17%	0.021%
42	16.510	2244	2248	2251	rVB6	4751	8317	0.11%	0.014%
43	16.727	2282	2285	2292	rVB9	3813	7373	0.10%	0.012%
44	17.010	2327	2333	2335	rBV5	7770	14142	0.19%	0.024%
45	17.104	2345	2349	2361	rVB3	10676	28283	0.38%	0.048%
46	17.321	2379	2386	2396	rVV	1998032	2889853	39.32%	4.860%
47	17.421	2396	2403	2415	rVV2	3775509	5597007	76.16%	9.413%
48	17.516	2416	2419	2427	rVB8	20216	35574	0.48%	0.060%
49	17.621	2434	2437	2442	rBV7	4744	8328	0.11%	0.014%
50	17.698	2445	2450	2454	rBV6	6444	10905	0.15%	0.018%
51	17.863	2472	2478	2481	rBV7	4514	10818	0.15%	0.018%
52	18.004	2498	2502	2508	rVB3	23934	32778	0.45%	0.055%
53	18.216	2534	2538	2545	rBV3	37309	57491	0.78%	0.097%
54	18.286	2547	2550	2555	rVB	13486	20165	0.27%	0.034%
55	19.233	2707	2711	2716	rBV2	58247	83031	1.13%	0.140%
56	19.304	2719	2723	2727	rBV	59644	76317	1.04%	0.128%
57	19.451	2746	2748	2753	rBV5	11445	12666	0.17%	0.021%
58	19.598	2770	2773	2777	rBV6	15851	21128	0.29%	0.036%
59	19.657	2777	2783	2790	rBV	5008711	6798679	92.51%	11.435%
60	21.133	3030	3034	3040	rBV2	135103	213948	2.91%	0.360%
61	21.415	3077	3082	3097	rBV	2653940	3549086	48.29%	5.969%
62	23.703	3463	3471	3479	rBV2	3669292	7349149	100.00%	12.360%
63	23.856	3491	3497	3510	rVB2	1759949	3683620	50.12%	6.195%




Sum of corrected areas: 59457242

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP102521\
Data File : BP007724.D
Acq On : 27 Oct 2021 17:47
Operator : CG/JU
Sample : M4304-12
Misc :
ALS Vial : 81 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
P075-TW001-01

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SFAM-EPA-BP102521.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

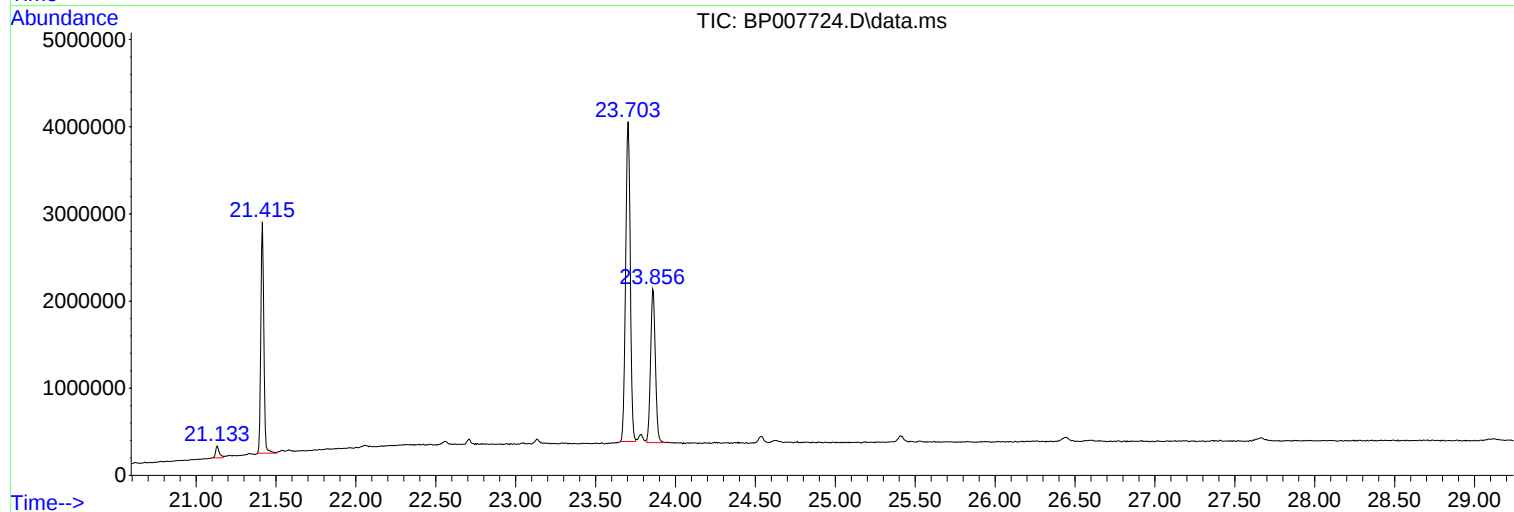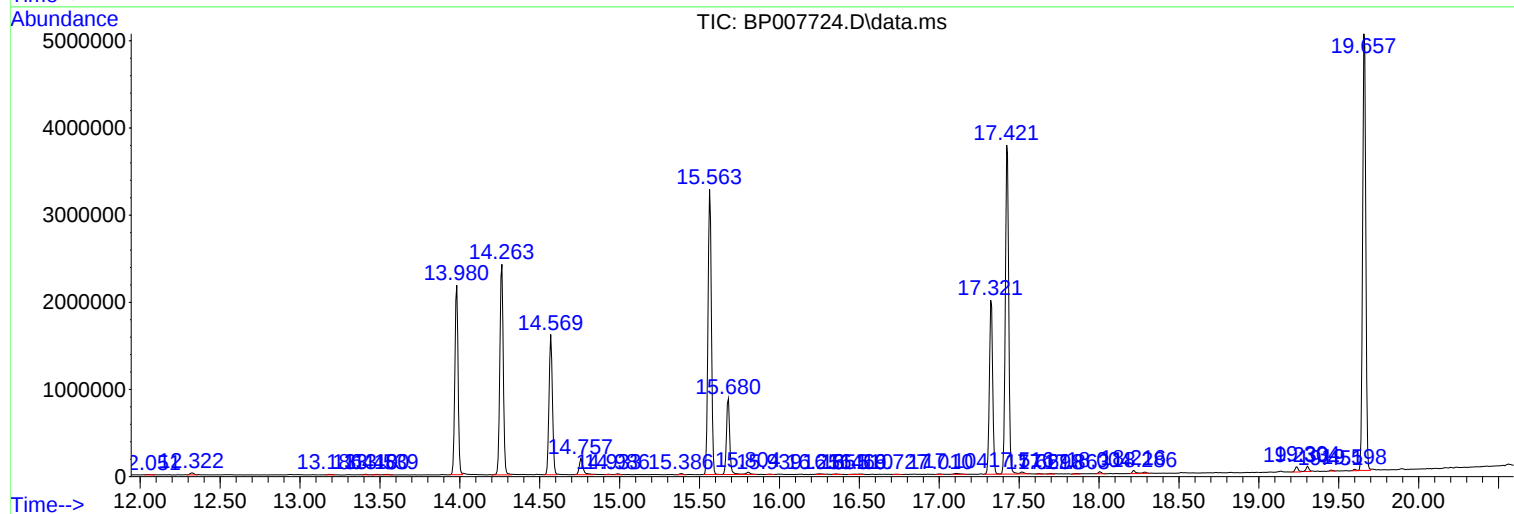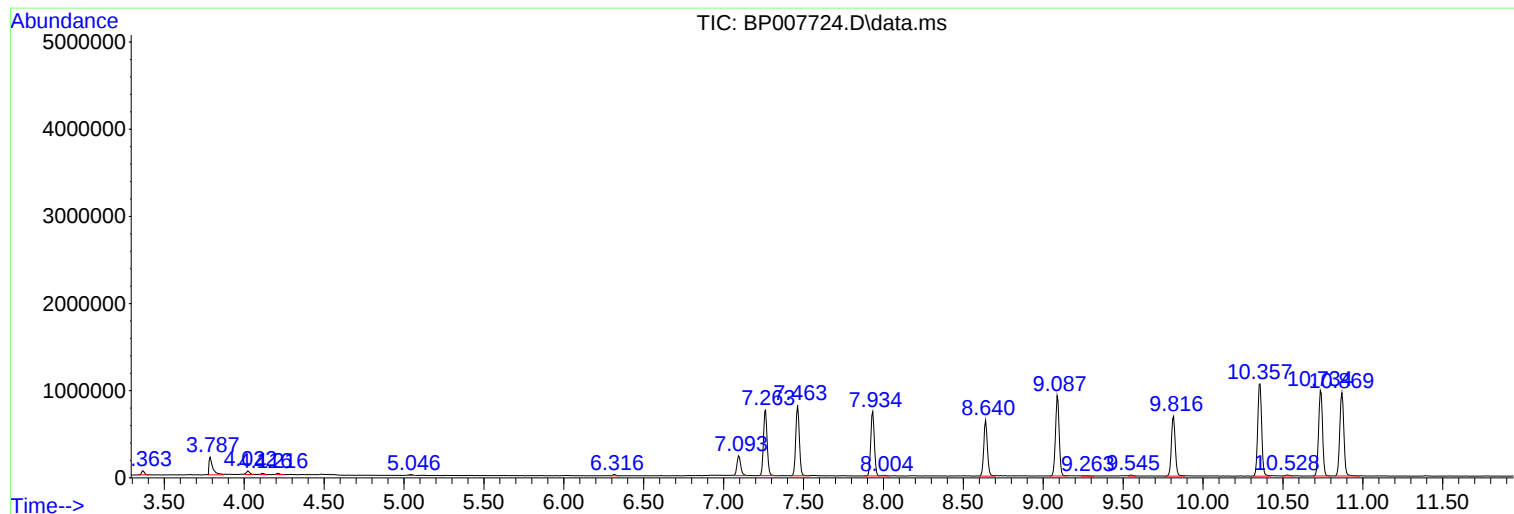

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP102521\
Data File : BP007724.D
Acq On : 27 Oct 2021 17:47
Operator : CG/JU
Sample : M4304-12
Misc :
ALS Vial : 81 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
P075-TW001-01

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SFAM-EPA-BP102521.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP102521\
Data File : BP007724.D
Acq On : 27 Oct 2021 17:47
Operator : CG/JU
Sample : M4304-12
Misc :
ALS Vial : 81 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
P075-TW001-01

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SFAM-EPA-BP102521.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
