

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP102521\
 Data File : BP007725.D
 Acq On : 27 Oct 2021 18:21
 Operator : CG/JU
 Sample : M4318-01
 Misc :
 ALS Vial : 82 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 P008-TW001-02

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SFAM-EPA-BP102521.M
 Title : SVOA CALIBRATION

Signal : TIC: BP007725.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.364	10	13	19	rBV	53334	64069	0.90%	0.108%
2	3.787	82	85	101	rBV	204401	328629	4.61%	0.552%
3	4.022	119	125	131	rBV	36745	60544	0.85%	0.102%
4	4.117	137	141	147	rVB2	14630	21240	0.30%	0.036%
5	4.211	152	157	161	rBV2	16919	23874	0.34%	0.040%
6	5.040	293	298	304	rVB4	15383	24113	0.34%	0.040%
7	6.316	509	515	519	rBV2	14606	21019	0.30%	0.035%
8	7.093	641	647	656	rVB	225034	363397	5.10%	0.610%
9	7.258	668	675	684	rBV	761341	1200124	16.85%	2.015%
10	7.463	702	710	721	rBV	764510	1225774	17.21%	2.058%
11	7.552	721	725	733	rVB4	8380	19623	0.28%	0.033%
12	7.934	782	790	797	rBV	798957	1274412	17.89%	2.140%
13	8.005	800	802	808	rVB4	5627	7947	0.11%	0.013%
14	8.640	902	910	918	rBV	628321	997141	14.00%	1.674%
15	8.693	918	919	923	rVB4	8826	9210	0.13%	0.015%
16	9.087	979	986	994	rBV	869601	1432701	20.12%	2.406%
17	9.546	1060	1064	1069	rVB5	6884	11560	0.16%	0.019%
18	9.816	1101	1110	1118	rBV	676357	1110135	15.59%	1.864%
19	10.352	1194	1201	1215	rBV	1058380	1761719	24.74%	2.958%
20	10.522	1223	1230	1241	rBV2	19183	42519	0.60%	0.071%
21	10.734	1257	1266	1274	rBV	1073542	1836045	25.78%	3.083%
22	10.869	1279	1289	1304	rBV	973893	1675043	23.52%	2.813%
23	11.387	1372	1377	1383	rVB5	5282	10711	0.15%	0.018%
24	12.322	1530	1536	1541	rBV2	20518	36673	0.51%	0.062%
25	12.934	1637	1640	1648	rBV7	6459	11540	0.16%	0.019%
26	13.181	1677	1682	1689	rVB9	8041	14525	0.20%	0.024%
27	13.404	1718	1720	1725	rBV6	5440	8013	0.11%	0.013%
28	13.475	1725	1732	1736	rVV9	5703	10789	0.15%	0.018%
29	13.545	1739	1744	1750	rVB7	5663	11241	0.16%	0.019%
30	13.893	1799	1803	1808	rVB8	4649	7412	0.10%	0.012%
31	13.981	1811	1818	1834	rBV	2124712	2955448	41.50%	4.963%
32	14.263	1856	1866	1875	rBV	2333519	3440763	48.31%	5.778%
33	14.569	1911	1918	1930	rBV	1756514	2551688	35.83%	4.285%
34	14.757	1940	1950	1960	rBV	188381	314388	4.41%	0.528%
35	14.987	1984	1989	1993	rVB7	16183	22218	0.31%	0.037%
36	15.387	2052	2057	2063	rVV6	9619	16068	0.23%	0.027%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP102521\
 Data File : BP007725.D
 Acq On : 27 Oct 2021 18:21
 Operator : CG/JU
 Sample : M4318-01
 Misc :
 ALS Vial : 82 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 P008-TW001-02

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF Filtering: 5
 Sampling : 1 Min Area: 0.1 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SFAM-EPA-BP102521.M
 Title : SVOA CALIBRATION

37	15.563	2080	2087	2098	rBV	3134540	4626164	64.96%	7.768%
38	15.681	2100	2107	2119	rVV	888653	1246770	17.51%	2.094%
39	15.804	2120	2128	2133	rVB3	23190	42164	0.59%	0.071%
40	16.245	2200	2203	2208	rBV7	6408	12043	0.17%	0.020%
41	16.469	2236	2241	2244	rBV7	5739	9511	0.13%	0.016%
42	17.110	2341	2350	2353	rBV3	13110	25541	0.36%	0.043%
43	17.322	2379	2386	2394	rBV	2171930	3116276	43.76%	5.233%
44	17.422	2396	2403	2415	rVV	3874742	5471289	76.83%	9.187%
45	17.516	2416	2419	2427	rVB10	16577	31868	0.45%	0.054%
46	17.698	2447	2450	2458	rVB7	4613	8501	0.12%	0.014%
47	17.763	2458	2461	2467	rBV6	5122	7254	0.10%	0.012%
48	18.004	2498	2502	2508	rVB2	18070	26330	0.37%	0.044%
49	18.216	2534	2538	2547	rBV3	32704	52868	0.74%	0.089%
50	18.286	2547	2550	2555	rVB	12992	15820	0.22%	0.027%
51	19.233	2707	2711	2718	rBV2	54909	76145	1.07%	0.128%
52	19.304	2718	2723	2727	rBV	60173	83911	1.18%	0.141%
53	19.598	2770	2773	2776	rBV4	21433	23431	0.33%	0.039%
54	19.657	2777	2783	2791	rBV	4912272	6639065	93.22%	11.148%
55	21.127	3030	3033	3042	rBV4	98972	166155	2.33%	0.279%
56	21.416	3076	3082	3095	rBV	2804668	3847686	54.03%	6.461%
57	23.704	3463	3471	3479	rBV2	3497449	7121698	100.00%	11.958%
58	23.857	3490	3497	3509	rVB2	1879382	3981026	55.90%	6.685%




Sum of corrected areas: 59553831

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP102521\
Data File : BP007725.D
Acq On : 27 Oct 2021 18:21
Operator : CG/JU
Sample : M4318-01
Misc :
ALS Vial : 82 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
P008-TW001-02

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SFAM-EPA-BP102521.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

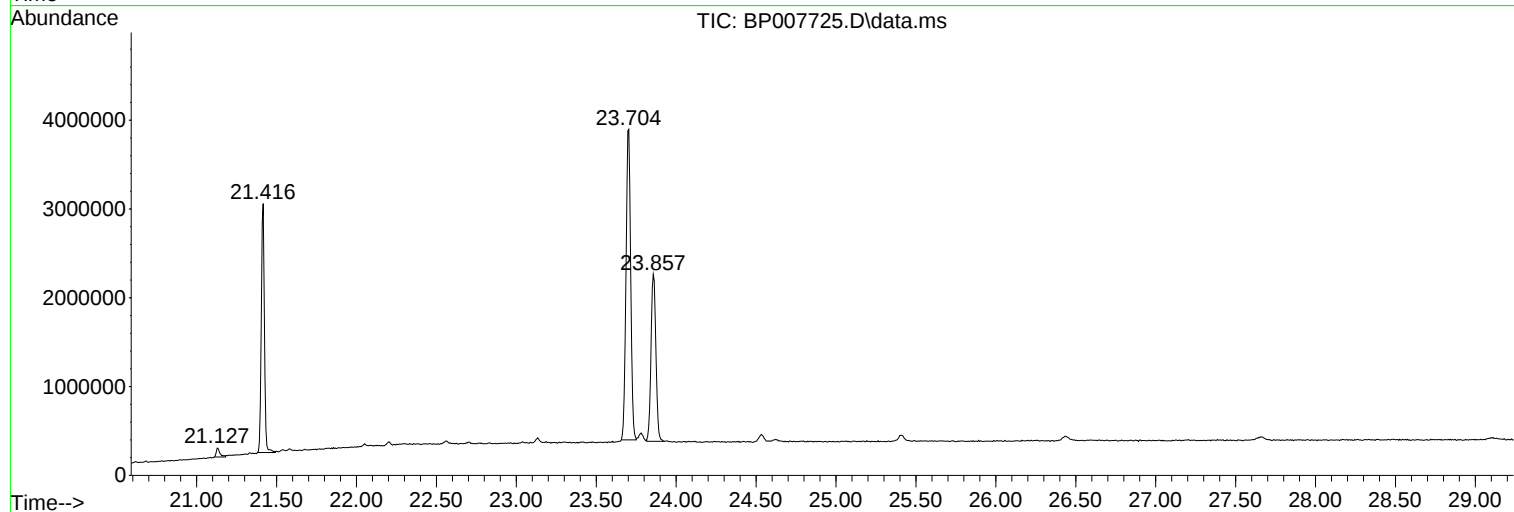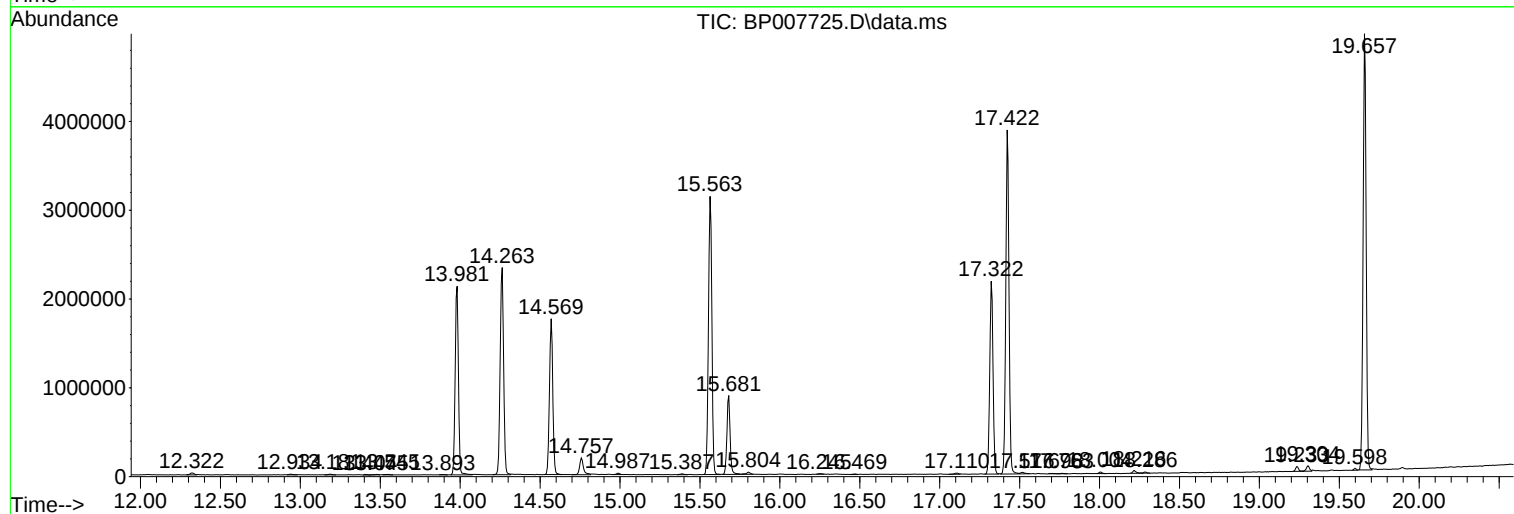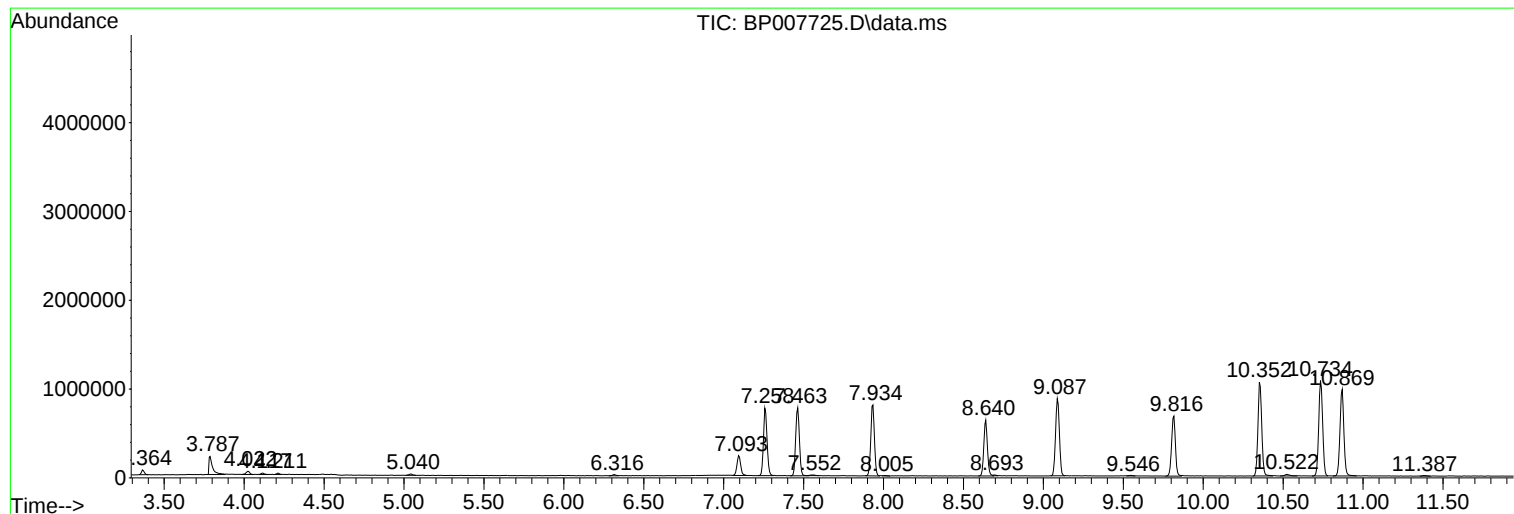

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP102521\
Data File : BP007725.D
Acq On : 27 Oct 2021 18:21
Operator : CG/JU
Sample : M4318-01
Misc :
ALS Vial : 82 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
P008-TW001-02

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SFAM-EPA-BP102521.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP102521\
Data File : BP007725.D
Acq On : 27 Oct 2021 18:21
Operator : CG/JU
Sample : M4318-01
Misc :
ALS Vial : 82 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
P008-TW001-02

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SFAM-EPA-BP102521.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------