

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP102521\
 Data File : BP007726.D
 Acq On : 27 Oct 2021 18:55
 Operator : CG/JU
 Sample : M4318-02
 Misc :
 ALS Vial : 83 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 P016-TW001-02

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SFAM-EPA-BP102521.M
 Title : SVOA CALIBRATION

Signal : TIC: BP007726.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.364	10	13	19	rBV	51064	65136	1.11%	0.121%
2	3.781	81	84	104	rBV	361256	595663	10.18%	1.104%
3	4.022	121	125	132	rVB	37714	58298	1.00%	0.108%
4	4.111	136	140	147	rBV2	17530	28812	0.49%	0.053%
5	4.211	154	157	163	rVB6	16270	22715	0.39%	0.042%
6	5.040	293	298	303	rBV2	13300	20180	0.34%	0.037%
7	6.311	510	514	519	rBV3	12371	19054	0.33%	0.035%
8	7.093	641	647	659	rVB	199959	331902	5.67%	0.615%
9	7.258	668	675	686	rVB	674964	1071747	18.31%	1.986%
10	7.463	702	710	720	rBV	634295	981479	16.77%	1.819%
11	7.569	723	728	733	rBV8	4165	7360	0.13%	0.014%
12	7.934	782	790	798	rBV	776847	1260074	21.53%	2.335%
13	8.005	798	802	805	rBV5	4854	5915	0.10%	0.011%
14	8.181	821	832	833	rBV5	2933	6573	0.11%	0.012%
15	8.640	903	910	920	rBV	506927	806795	13.78%	1.495%
16	9.087	978	986	996	rBV	785852	1268472	21.67%	2.351%
17	9.269	1011	1017	1023	rVB	3794	6549	0.11%	0.012%
18	9.546	1057	1064	1071	rVB7	7661	16121	0.28%	0.030%
19	9.816	1099	1110	1117	rBV	520578	880247	15.04%	1.631%
20	10.352	1191	1201	1218	rBV	853580	1444584	24.68%	2.677%
21	10.522	1224	1230	1235	rBV2	15966	28799	0.49%	0.053%
22	10.734	1258	1266	1276	rVB	1085311	1815391	31.01%	3.364%
23	10.869	1281	1289	1303	rBV	1367553	2369985	40.49%	4.392%
24	12.322	1530	1536	1541	rBV	20020	36176	0.62%	0.067%
25	12.934	1634	1640	1646	rBV10	3812	8114	0.14%	0.015%
26	13.187	1678	1683	1689	rVB7	5316	9899	0.17%	0.018%
27	13.298	1698	1702	1708	rBV8	3604	7612	0.13%	0.014%
28	13.410	1716	1721	1727	rBV10	6654	11107	0.19%	0.021%
29	13.475	1727	1732	1737	rVV6	6580	9588	0.16%	0.018%
30	13.540	1738	1743	1748	rVV7	5552	9549	0.16%	0.018%
31	13.893	1796	1803	1806	rBV9	3610	6679	0.11%	0.012%
32	13.981	1811	1818	1824	rBV	1827792	2494498	42.61%	4.623%
33	14.263	1855	1866	1878	rBV	2006685	3000606	51.26%	5.561%
34	14.481	1899	1903	1910	rBV10	4352	7621	0.13%	0.014%
35	14.569	1910	1918	1930	rBV	1737722	2540942	43.41%	4.709%
36	14.757	1942	1950	1964	rBV	139150	246686	4.21%	0.457%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP102521\
 Data File : BP007726.D
 Acq On : 27 Oct 2021 18:55
 Operator : CG/JU
 Sample : M4318-02
 Misc :
 ALS Vial : 83 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 P016-TW001-02

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF Filtering: 5
 Sampling : 1 Min Area: 0.1 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SFAM-EPA-BP102521.M
 Title : SVOA CALIBRATION

37	14.992	1985	1990	2002	rVB	12241	24483	0.42%	0.045%
38	15.387	2052	2057	2061	rBV8	5649	9759	0.17%	0.018%
39	15.428	2061	2064	2070	rVB8	5265	7787	0.13%	0.014%
40	15.563	2080	2087	2096	rBV	2763473	3943319	67.37%	7.308%
41	15.675	2100	2106	2119	rBV	606706	887970	15.17%	1.646%
42	15.804	2124	2128	2133	rVB3	19838	29812	0.51%	0.055%
43	15.992	2157	2160	2163	rBV5	4744	7838	0.13%	0.015%
44	16.134	2178	2184	2189	rBV9	4228	9018	0.15%	0.017%
45	16.245	2197	2203	2204	rBV6	6069	8354	0.14%	0.015%
46	16.351	2218	2221	2228	rVB9	4462	8236	0.14%	0.015%
47	16.469	2233	2241	2244	rBV8	5156	8650	0.15%	0.016%
48	16.728	2282	2285	2291	rVB8	3889	6415	0.11%	0.012%
49	16.998	2329	2331	2339	rVB8	4512	7563	0.13%	0.014%
50	17.104	2344	2349	2353	rBV2	10493	18258	0.31%	0.034%
51	17.257	2370	2375	2379	rBV7	3967	6710	0.11%	0.012%
52	17.322	2379	2386	2395	rVV	2163033	3130600	53.48%	5.802%
53	17.422	2396	2403	2415	rVV	3167488	4556688	77.84%	8.445%
54	17.522	2415	2420	2425	rVB7	21140	37694	0.64%	0.070%
55	17.698	2447	2450	2457	rBV6	6865	11246	0.19%	0.021%
56	18.004	2497	2502	2506	rBV	24565	32626	0.56%	0.060%
57	18.216	2534	2538	2545	rBV4	39846	61181	1.05%	0.113%
58	18.516	2586	2589	2591	rBV4	7098	10595	0.18%	0.020%
59	19.233	2707	2711	2718	rBV2	51201	81900	1.40%	0.152%
60	19.304	2719	2723	2726	rVV2	46645	59098	1.01%	0.110%
61	19.451	2745	2748	2753	rBV6	13803	19518	0.33%	0.036%
62	19.598	2770	2773	2777	rBV5	18486	20430	0.35%	0.038%
63	19.657	2777	2783	2790	rBV	4292904	5574857	95.24%	10.332%
64	21.133	3030	3034	3042	rBV2	156853	246453	4.21%	0.457%
65	21.416	3076	3082	3091	rBV	2801745	3823019	65.31%	7.085%
66	23.698	3463	3470	3480	rBV2	2980184	5853577	100.00%	10.848%
67	23.857	3490	3497	3513	rVB2	1876281	3955182	67.57%	7.330%




Sum of corrected areas: 53959764

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP102521\
Data File : BP007726.D
Acq On : 27 Oct 2021 18:55
Operator : CG/JU
Sample : M4318-02
Misc :
ALS Vial : 83 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
P016-TW001-02

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SFAM-EPA-BP102521.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

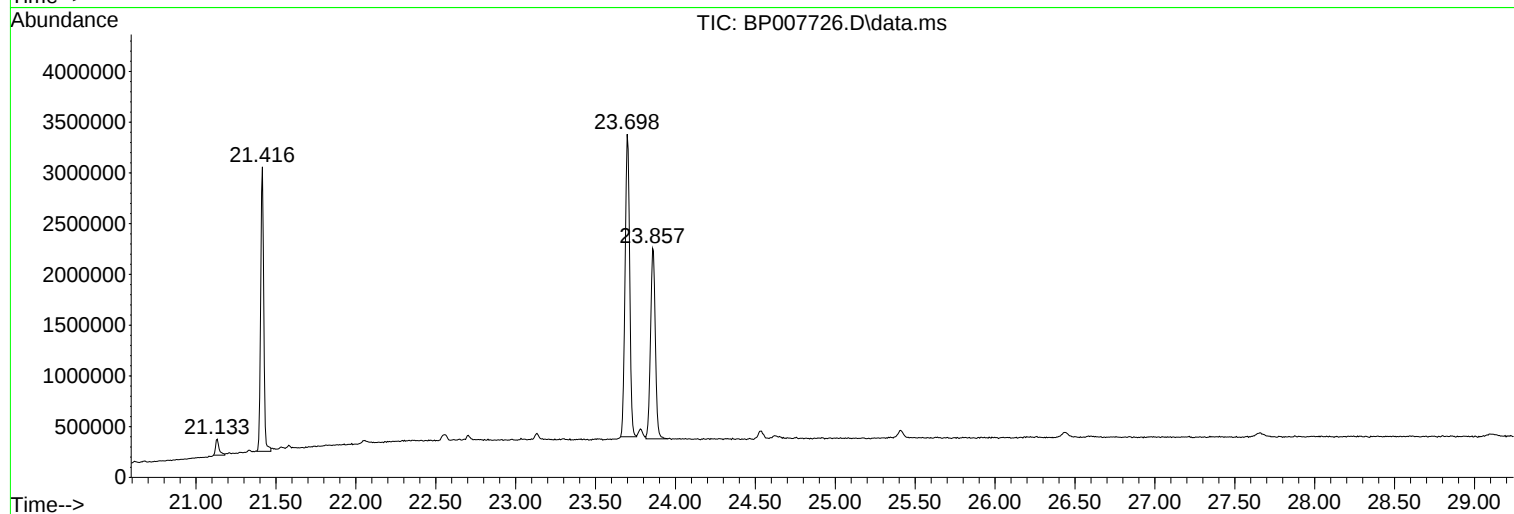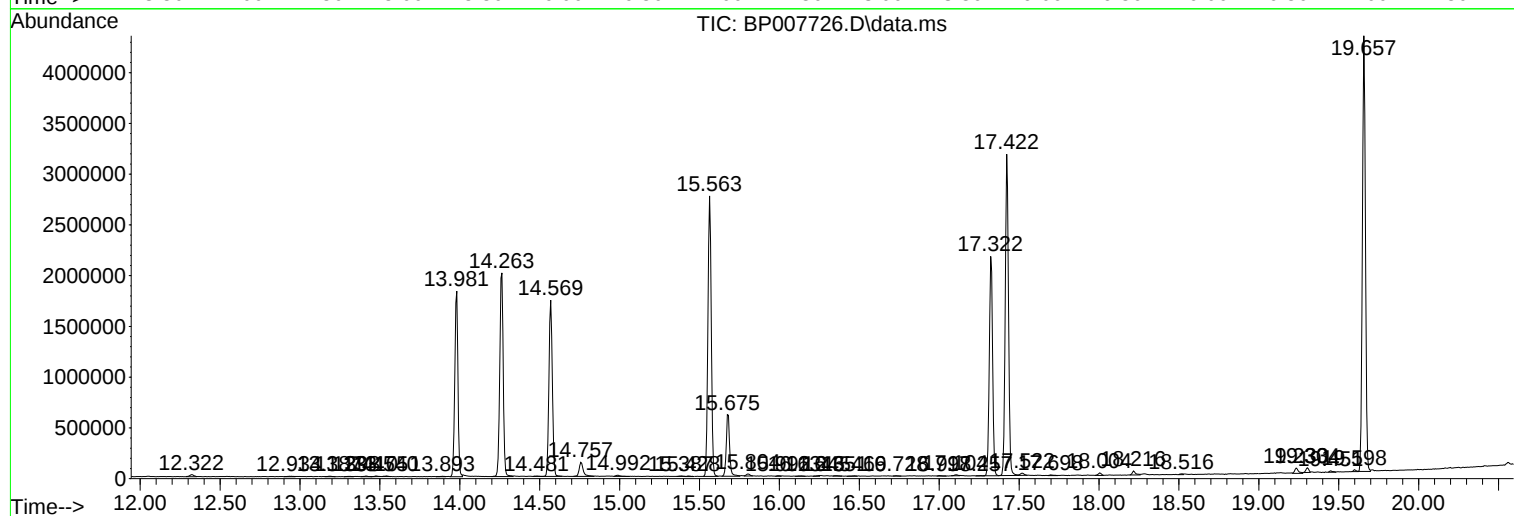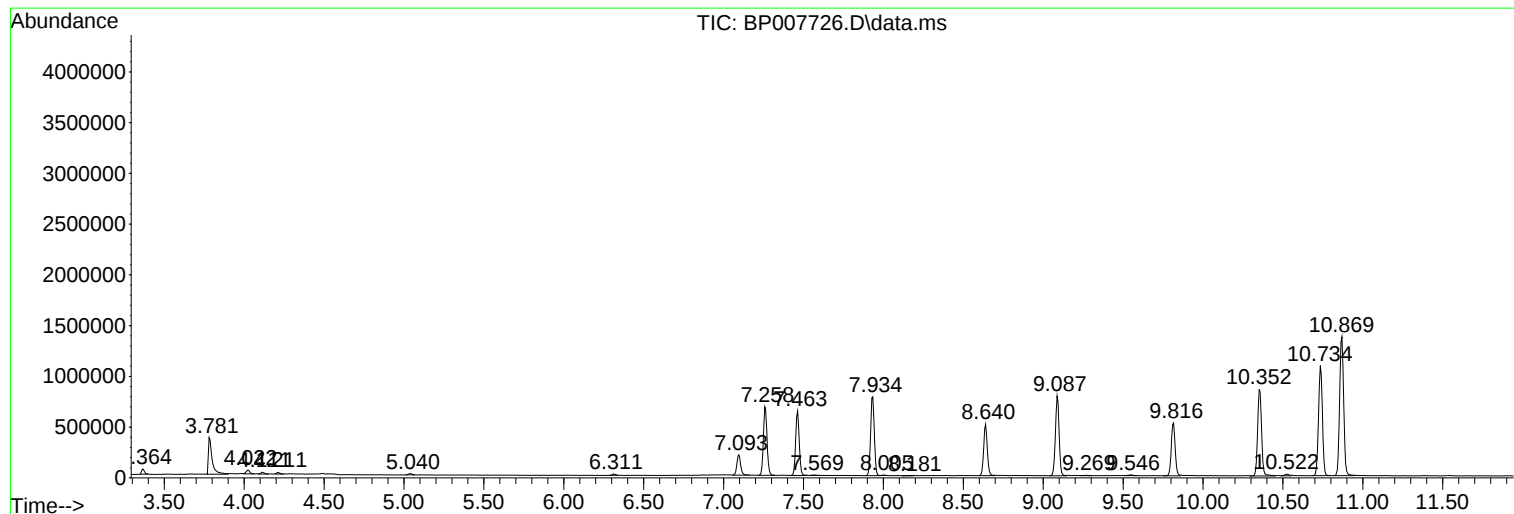

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP102521\
Data File : BP007726.D
Acq On : 27 Oct 2021 18:55
Operator : CG/JU
Sample : M4318-02
Misc :
ALS Vial : 83 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
P016-TW001-02

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SFAM-EPA-BP102521.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP102521\
Data File : BP007726.D
Acq On : 27 Oct 2021 18:55
Operator : CG/JU
Sample : M4318-02
Misc :
ALS Vial : 83 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
P016-TW001-02

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SFAM-EPA-BP102521.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
