

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP102521\
 Data File : BP007733.D
 Acq On : 27 Oct 2021 22:53
 Operator : CG/JU
 Sample : M4215-20
 Misc :
 ALS Vial : 90 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 JDGF7

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SFAM-EPA-BP102521.M
 Title : SVOA CALIBRATION

Signal : TIC: BP007733.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.364	10	13	20	rBV	48570	63809	1.13%	0.114%
2	3.652	59	62	71	rBV7	6070	13037	0.23%	0.023%
3	3.787	83	85	100	rBV	137360	231799	4.11%	0.415%
4	4.028	122	126	130	rVB2	13568	18023	0.32%	0.032%
5	4.117	137	141	148	rVB	14848	19629	0.35%	0.035%
6	4.211	155	157	162	rVB5	8163	7686	0.14%	0.014%
7	5.034	294	297	304	rVB4	7160	11869	0.21%	0.021%
8	5.111	308	310	318	rVB9	4558	8281	0.15%	0.015%
9	6.311	509	514	520	rVB7	5815	12157	0.22%	0.022%
10	7.093	640	647	660	rVB	953679	1484784	26.33%	2.656%
11	7.258	669	675	684	rBV	742981	1187199	21.05%	2.124%
12	7.464	702	710	719	rBV	962503	1524315	27.03%	2.727%
13	7.928	782	789	799	rBV	705131	1139619	20.21%	2.039%
14	8.005	799	802	805	rVB4	5549	6671	0.12%	0.012%
15	8.640	902	910	922	rBV	1145069	1854486	32.89%	3.318%
16	9.087	979	986	999	rBV	880493	1421047	25.20%	2.542%
17	9.546	1060	1064	1069	rVB3	8418	13094	0.23%	0.023%
18	9.811	1102	1109	1123	rBV	668985	1110702	19.70%	1.987%
19	10.046	1145	1149	1151	rBV4	4240	6485	0.12%	0.012%
20	10.352	1193	1201	1218	rBV	1150334	1900063	33.70%	3.399%
21	10.516	1223	1229	1241	rBV	122721	219839	3.90%	0.393%
22	10.734	1257	1266	1276	rBV	973084	1627422	28.86%	2.911%
23	10.869	1281	1289	1298	rBV	978979	1704621	30.23%	3.049%
24	12.322	1529	1536	1546	rVB2	19491	36106	0.64%	0.065%
25	13.181	1676	1682	1688	rBV9	5310	9254	0.16%	0.017%
26	13.475	1729	1732	1737	rBV4	4916	7131	0.13%	0.013%
27	13.540	1739	1743	1747	rVB6	5175	8541	0.15%	0.015%
28	13.975	1811	1817	1833	rBV	1825168	2663554	47.24%	4.765%
29	14.257	1854	1865	1879	rBV	2199645	3271287	58.01%	5.852%
30	14.569	1910	1918	1927	rBV	1497656	2216057	39.30%	3.964%
31	14.757	1940	1950	1965	rBV	790912	1183499	20.99%	2.117%
32	14.857	1965	1967	1974	rVB8	4519	7688	0.14%	0.014%
33	14.987	1984	1989	1993	rBV7	13133	18846	0.33%	0.034%
34	15.210	2024	2027	2032	rVB7	4100	6038	0.11%	0.011%
35	15.381	2051	2056	2061	rBV7	4114	7976	0.14%	0.014%
36	15.434	2061	2065	2069	rVB6	4328	5728	0.10%	0.010%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP102521\
 Data File : BP007733.D
 Acq On : 27 Oct 2021 22:53
 Operator : CG/JU
 Sample : M4215-20
 Misc :
 ALS Vial : 90 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 JDGF7

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF Filtering: 5
 Sampling : 1 Min Area: 0.1 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SFAM-EPA-BP102521.M
 Title : SVOA CALIBRATION

37	15.563	2079	2087	2096	rBV	2887519	4166685	73.89%	7.454%
38	15.675	2100	2106	2123	rVV	634313	870761	15.44%	1.558%
39	15.804	2123	2128	2133	rVB	35351	51060	0.91%	0.091%
40	15.928	2145	2149	2156	rVB9	3395	6769	0.12%	0.012%
41	16.016	2160	2164	2167	rVV6	4456	7253	0.13%	0.013%
42	16.351	2216	2221	2228	rVB6	5187	11049	0.20%	0.020%
43	16.934	2315	2320	2324	rVB8	4105	7511	0.13%	0.013%
44	17.004	2327	2332	2335	rVB7	4403	7218	0.13%	0.013%
45	17.110	2344	2350	2353	rBV2	11204	21060	0.37%	0.038%
46	17.322	2379	2386	2395	rBV	1937198	2689562	47.70%	4.811%
47	17.422	2396	2403	2415	rVV2	3076452	4461107	79.11%	7.981%
48	17.516	2415	2419	2432	rVB6	32388	59053	1.05%	0.106%
49	18.004	2498	2502	2507	rVV	34460	41325	0.73%	0.074%
50	18.216	2534	2538	2545	rBV2	53396	77424	1.37%	0.139%
51	18.287	2548	2550	2554	rVB	12791	13404	0.24%	0.024%
52	19.234	2707	2711	2715	rBV3	43042	59020	1.05%	0.106%
53	19.304	2719	2723	2726	rVV	37707	42954	0.76%	0.077%
54	19.445	2744	2747	2752	rBV6	21325	31892	0.57%	0.057%
55	19.657	2777	2783	2789	rBV	4078612	5406758	95.88%	9.672%
56	21.128	3030	3033	3041	rBV3	154269	240022	4.26%	0.429%
57	21.410	3076	3081	3092	rBV	2407203	3365210	59.68%	6.020%
58	21.580	3107	3110	3114	rBV4	51503	67812	1.20%	0.121%
59	23.698	3463	3470	3478	rBV2	2876111	5638932	100.00%	10.088%
60	23.857	3490	3497	3510	rVB2	1658660	3527763	62.56%	6.311%




Sum of corrected areas: 55899946

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP102521\
Data File : BP007733.D
Acq On : 27 Oct 2021 22:53
Operator : CG/JU
Sample : M4215-20
Misc :
ALS Vial : 90 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
JDGF7

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SFAM-EPA-BP102521.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

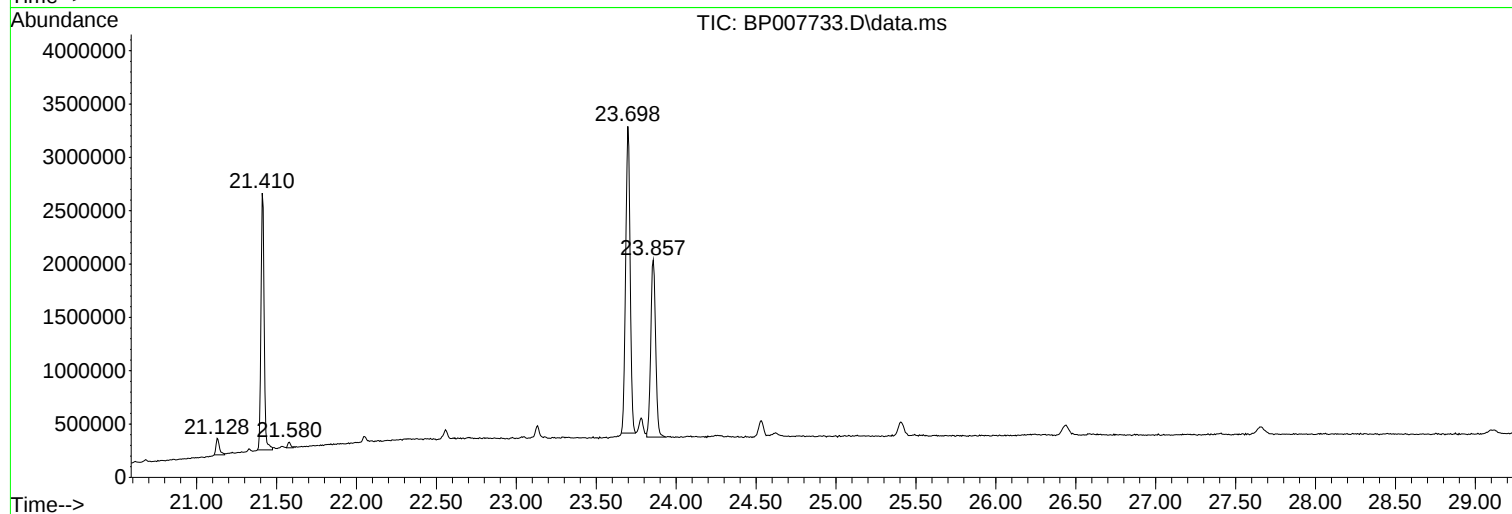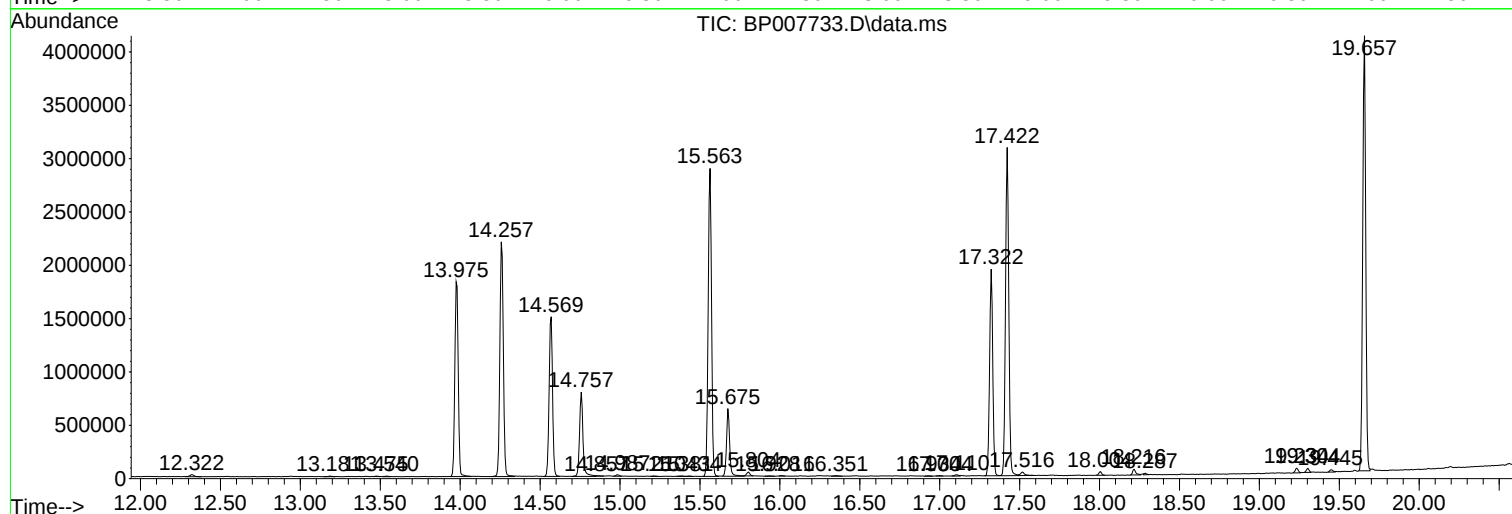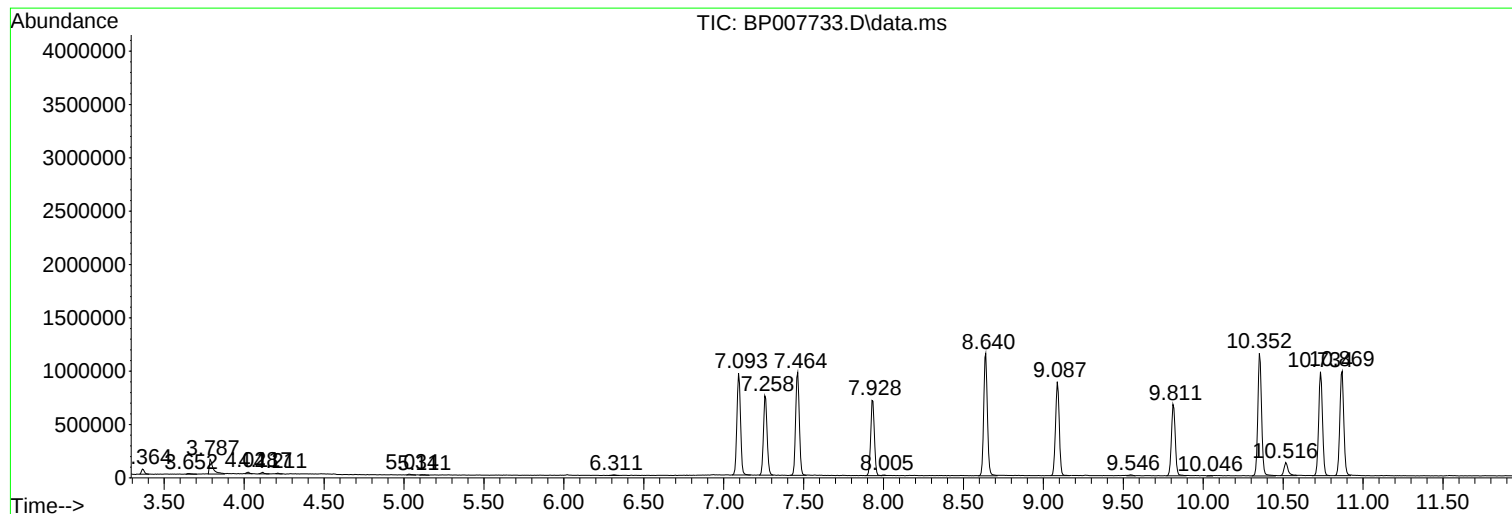

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP102521\
Data File : BP007733.D
Acq On : 27 Oct 2021 22:53
Operator : CG/JU
Sample : M4215-20
Misc :
ALS Vial : 90 Sample Multiplier: 1










Instrument :
BNA_P
ClientSampleId :
JDGF7

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SFAM-EPA-BP102521.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 Ethanol, 2-(2-butoxyethoxy)- Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.	
10.516	2.70 ng/ul	219839	Naphthalene-d8	10.734	
Hit# of 5	Tentative ID	MW	MolForm	CAS#	Qual
1	Ethanol, 2-(2-butoxyethoxy)-	162	C8H18O3	000112-34-5	91
2	Ethanol, 2-(2-butoxyethoxy)-	162	C8H18O3	000112-34-5	90
3	Ethanol, 2-(2-butoxyethoxy)-	162	C8H18O3	000112-34-5	90
4	Ethanol, 2-(2-butoxyethoxy)-	162	C8H18O3	000112-34-5	90
5	Ethanol, 2-(2-butoxyethoxy)-	162	C8H18O3	000112-34-5	83

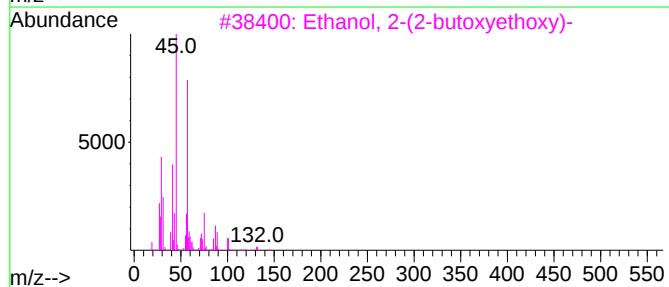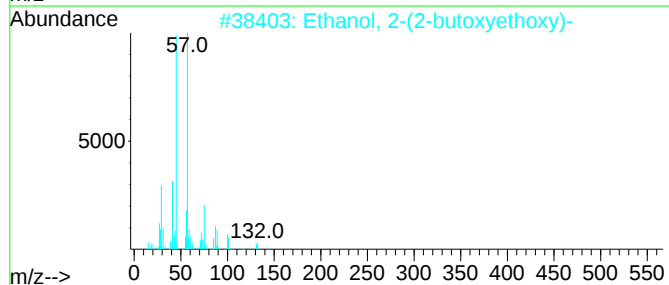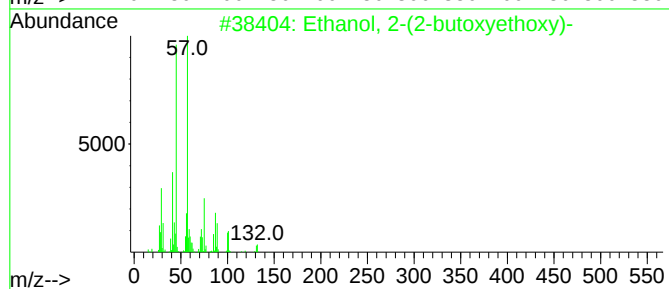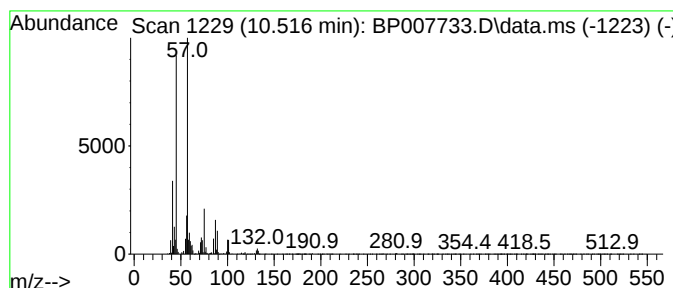

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP102521\
Data File : BP007733.D
Acq On : 27 Oct 2021 22:53
Operator : CG/JU
Sample : M4215-20
Misc :
ALS Vial : 90 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
JDGF7

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SFAM-EPA-BP102521.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
Ethanol, 2-(2-b...	10.516	2.7	ng/u1	219839	2	10.734	1627420	20.0