

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP102521\
 Data File : BP007734.D
 Acq On : 27 Oct 2021 23:27
 Operator : CG/JU
 Sample : M4215-13
 Misc :
 ALS Vial : 91 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 JDGE0

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SFAM-EPA-BP102521.M
 Title : SVOA CALIBRATION

Signal : TIC: BP007734.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.364	9	13	18	rBV	36489	44043	0.88%	0.085%
2	3.793	83	86	97	rBV	88399	150944	3.03%	0.291%
3	4.022	122	125	133	rVB3	12560	20174	0.41%	0.039%
4	4.111	137	140	146	rVB	12026	17890	0.36%	0.034%
5	4.211	154	157	163	rVB8	6153	9321	0.19%	0.018%
6	5.046	294	299	305	rVB5	7318	15126	0.30%	0.029%
7	5.117	307	311	316	rVB7	3483	6124	0.12%	0.012%
8	6.016	459	464	469	rBV7	3183	6122	0.12%	0.012%
9	6.316	512	515	521	rVB7	4320	6411	0.13%	0.012%
10	7.093	640	647	662	rVB	857027	1324699	26.60%	2.553%
11	7.258	669	675	687	rVB	664063	1069976	21.48%	2.062%
12	7.463	703	710	722	rBV	871927	1359721	27.30%	2.621%
13	7.928	782	789	797	rBV	693988	1137705	22.84%	2.193%
14	8.005	797	802	805	rVB6	4813	8811	0.18%	0.017%
15	8.187	829	833	836	rBV6	3532	6330	0.13%	0.012%
16	8.640	903	910	922	rBV	1034043	1640487	32.94%	3.162%
17	9.087	977	986	1000	rBV	781254	1273627	25.57%	2.455%
18	9.546	1060	1064	1068	rVB5	6607	10501	0.21%	0.020%
19	9.810	1101	1109	1117	rBV	592107	976068	19.60%	1.881%
20	10.352	1192	1201	1211	rBV	1003817	1683305	33.80%	3.245%
21	10.516	1224	1229	1242	rBV	53817	102580	2.06%	0.198%
22	10.734	1259	1266	1274	rBV	989385	1640204	32.93%	3.162%
23	10.869	1281	1289	1308	rBV	852802	1521053	30.54%	2.932%
24	12.322	1531	1536	1546	rVB3	15201	31461	0.63%	0.061%
25	13.187	1678	1683	1687	rVB7	6324	8267	0.17%	0.016%
26	13.540	1738	1743	1747	rBV6	4764	8079	0.16%	0.016%
27	13.981	1811	1818	1832	rBV	1720446	2438754	48.97%	4.701%
28	14.257	1854	1865	1880	rBV	1982087	3006983	60.38%	5.796%
29	14.487	1899	1904	1907	rBV7	2855	5152	0.10%	0.010%
30	14.569	1910	1918	1929	rVV	1552011	2276213	45.71%	4.388%
31	14.757	1942	1950	1967	rBV	693795	1029587	20.67%	1.985%
32	14.981	1983	1988	1993	rBV8	9418	16026	0.32%	0.031%
33	15.381	2052	2056	2060	rBV7	3989	7212	0.14%	0.014%
34	15.563	2080	2087	2100	rBV	2661980	3849594	77.30%	7.420%
35	15.675	2100	2106	2123	rVV	556275	776896	15.60%	1.498%
36	15.804	2123	2128	2134	rVB	32713	51802	1.04%	0.100%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP102521\
 Data File : BP007734.D
 Acq On : 27 Oct 2021 23:27
 Operator : CG/JU
 Sample : M4215-13
 Misc :
 ALS Vial : 91 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 JDGE0

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF Filtering: 5
 Sampling : 1 Min Area: 0.1 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SFAM-EPA-BP102521.M
 Title : SVOA CALIBRATION

37	16.122	2178	2182	2183	rBV4	3993	6208	0.12%	0.012%
38	16.463	2236	2240	2247	rVB9	3644	6317	0.13%	0.012%
39	16.810	2294	2299	2302	rBV7	3181	5773	0.12%	0.011%
40	17.004	2326	2332	2334	rBV7	4419	7057	0.14%	0.014%
41	17.110	2345	2350	2355	rBV	9278	16975	0.34%	0.033%
42	17.322	2379	2386	2396	rBV	2000798	2781661	55.85%	5.362%
43	17.422	2396	2403	2415	rVV	2982532	4139031	83.11%	7.978%
44	17.516	2416	2419	2426	rVB9	15986	29114	0.58%	0.056%
45	17.710	2446	2452	2455	rBV7	4916	9036	0.18%	0.017%
46	18.004	2497	2502	2508	rBV	37194	47329	0.95%	0.091%
47	18.216	2533	2538	2544	rBV6	24814	41762	0.84%	0.080%
48	18.281	2547	2549	2555	rVB2	8296	13032	0.26%	0.025%
49	19.133	2692	2694	2698	rVB5	11846	13649	0.27%	0.026%
50	19.233	2707	2711	2716	rBV2	44548	60905	1.22%	0.117%
51	19.304	2719	2723	2727	rBV	33793	44504	0.89%	0.086%
52	19.598	2770	2773	2776	rBV5	13302	18496	0.37%	0.036%
53	19.657	2777	2783	2789	rBV	3684602	4975145	99.90%	9.590%
54	21.127	3029	3033	3043	rBV3	129764	235984	4.74%	0.455%
55	21.410	3076	3081	3095	rBV	2471390	3407070	68.41%	6.567%
56	23.698	3463	3470	3479	rVB2	2582792	4980202	100.00%	9.600%
57	23.857	3490	3497	3511	rVB2	1679494	3502801	70.33%	6.752%




Sum of corrected areas: 51879299

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP102521\
Data File : BP007734.D
Acq On : 27 Oct 2021 23:27
Operator : CG/JU
Sample : M4215-13
Misc :
ALS Vial : 91 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
JDGE0

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SFAM-EPA-BP102521.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

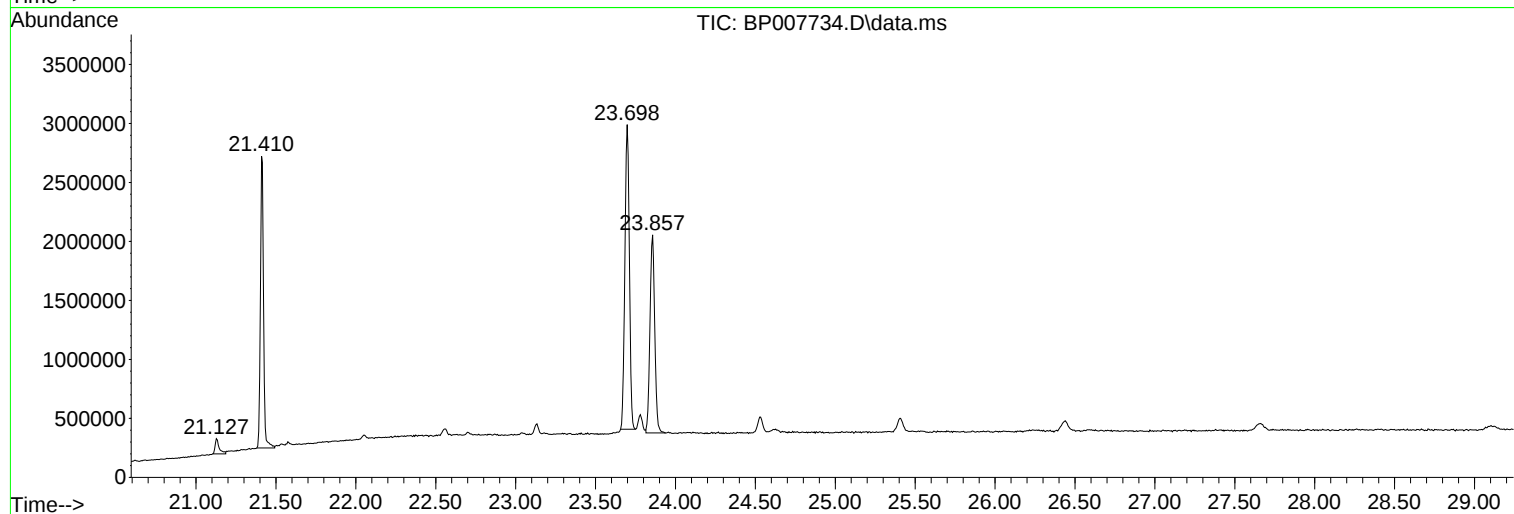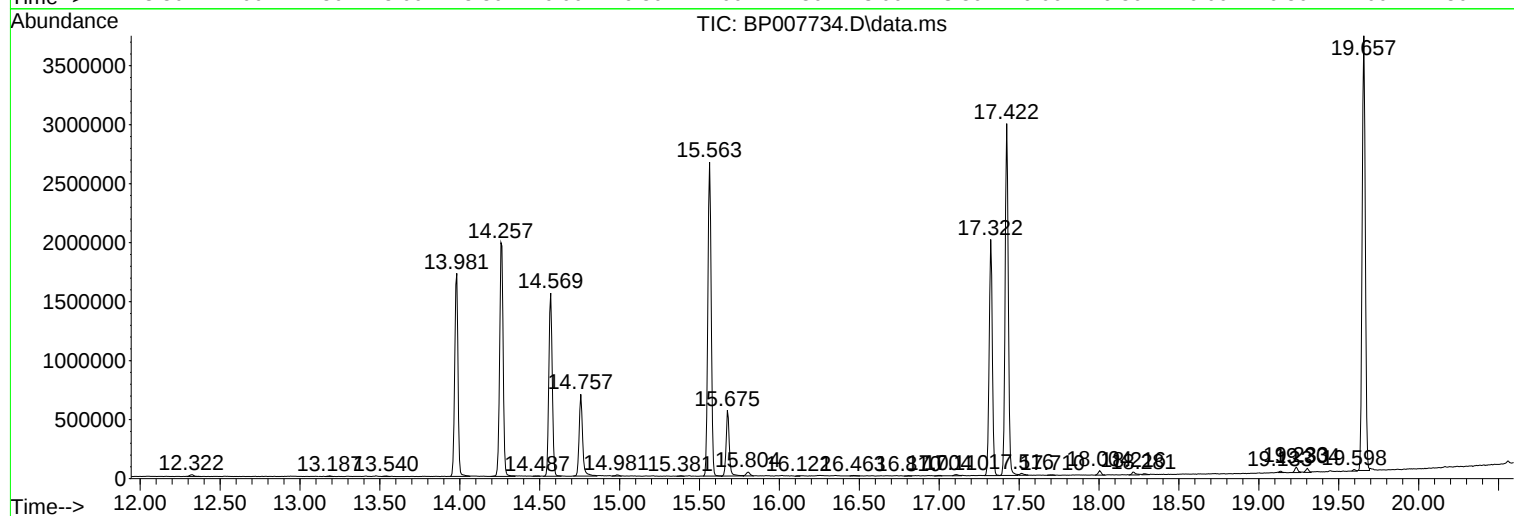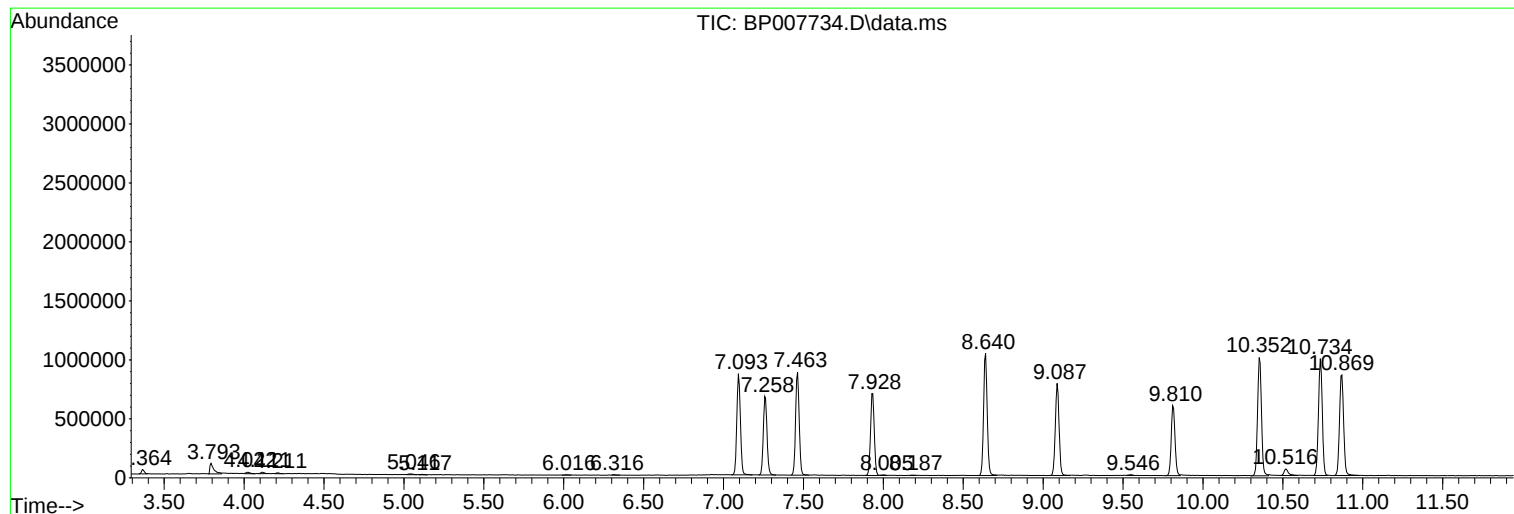

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP102521\
Data File : BP007734.D
Acq On : 27 Oct 2021 23:27
Operator : CG/JU
Sample : M4215-13
Misc :
ALS Vial : 91 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
JDGE0

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SFAM-EPA-BP102521.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP102521\
Data File : BP007734.D
Acq On : 27 Oct 2021 23:27
Operator : CG/JU
Sample : M4215-13
Misc :
ALS Vial : 91 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
JDGE0

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SFAM-EPA-BP102521.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------