

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP102521\
 Data File : BP007736.D
 Acq On : 28 Oct 2021 00:35
 Operator : CG/JU
 Sample : M4215-14
 Misc :
 ALS Vial : 93 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 JDGE8

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SFAM-EPA-BP102521.M
 Title : SVOA CALIBRATION

Signal : TIC: BP007736.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.369	12	14	17	rBV4	6166	6061	0.12%	0.015%
2	4.022	120	125	131	rBV	50967	73637	1.44%	0.176%
3	4.116	137	141	146	rBV	15801	20826	0.41%	0.050%
4	4.211	154	157	166	rVB3	23536	33232	0.65%	0.080%
5	4.487	201	204	208	rVB4	8581	10968	0.22%	0.026%
6	5.034	293	297	302	rBV	17238	23315	0.46%	0.056%
7	6.316	510	515	521	rBV2	18485	30579	0.60%	0.073%
8	6.940	618	621	624	rVB3	5840	7683	0.15%	0.018%
9	7.093	640	647	663	rVB	435602	693284	13.59%	1.659%
10	7.257	668	675	685	rBV	378322	600518	11.77%	1.437%
11	7.463	703	710	717	rBV	455777	723237	14.18%	1.731%
12	7.569	725	728	735	rVB6	6604	9535	0.19%	0.023%
13	7.751	755	759	761	rBV3	4667	6161	0.12%	0.015%
14	7.934	783	790	798	rBV	980651	1596715	31.31%	3.821%
15	8.075	809	814	824	rVB	3534	7903	0.15%	0.019%
16	8.175	827	831	837	rVB8	8274	16131	0.32%	0.039%
17	8.493	880	885	889	rBV6	5973	10701	0.21%	0.026%
18	8.640	901	910	922	rBV	517596	858132	16.83%	2.054%
19	8.757	922	930	938	rVB3	11492	26451	0.52%	0.063%
20	8.834	938	943	945	rBV6	3808	5644	0.11%	0.014%
21	9.087	978	986	994	rBV	424550	696058	13.65%	1.666%
22	9.263	1011	1016	1020	rVB7	3246	5186	0.10%	0.012%
23	9.546	1058	1064	1068	rVB3	8306	14193	0.28%	0.034%
24	9.810	1101	1109	1117	rBV	251037	426265	8.36%	1.020%
25	10.351	1193	1201	1211	rBV	502775	863156	16.92%	2.066%
26	10.734	1256	1266	1276	rBV	1403073	2308502	45.26%	5.525%
27	10.869	1280	1289	1304	rBV	246552	449812	8.82%	1.077%
28	12.322	1530	1536	1542	rVB4	6551	12642	0.25%	0.030%
29	13.186	1678	1683	1690	rVB4	3937	6458	0.13%	0.015%
30	13.892	1800	1803	1806	rBV4	4666	6647	0.13%	0.016%
31	13.975	1811	1817	1832	rVV	625117	879334	17.24%	2.104%
32	14.257	1858	1865	1877	rBV	1137200	1647567	32.30%	3.943%
33	14.569	1910	1918	1931	rBV	2173132	3217534	63.09%	7.700%
34	14.757	1944	1950	1963	rBV2	163225	276284	5.42%	0.661%
35	14.922	1974	1978	1981	rBV6	2737	5326	0.10%	0.013%
36	14.986	1984	1989	1993	rBV6	11037	16695	0.33%	0.040%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP102521\
 Data File : BP007736.D
 Acq On : 28 Oct 2021 00:35
 Operator : CG/JU
 Sample : M4215-14
 Misc :
 ALS Vial : 93 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 JDGE8

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF Filtering: 5
 Sampling : 1 Min Area: 0.1 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SFAM-EPA-BP102521.M
 Title : SVOA CALIBRATION

37	15.380	2052	2056	2058	rBV5	4246	5683	0.11%	0.014%
38	15.433	2061	2065	2069	rVB7	4793	8126	0.16%	0.019%
39	15.563	2078	2087	2100	rBV	1535981	2250011	44.12%	5.385%
40	15.675	2100	2106	2113	rBV	131418	194384	3.81%	0.465%
41	15.798	2124	2127	2133	rVB2	17473	23859	0.47%	0.057%
42	15.928	2146	2149	2152	rBV5	4667	5947	0.12%	0.014%
43	16.927	2316	2319	2326	rVB6	5601	10010	0.20%	0.024%
44	17.104	2344	2349	2355	rBV3	12929	22432	0.44%	0.054%
45	17.322	2379	2386	2395	rVV	2725557	3945170	77.35%	9.442%
46	17.422	2397	2403	2416	rVV	1775142	2482149	48.67%	5.940%
47	17.522	2416	2420	2425	rVB8	16235	25179	0.49%	0.060%
48	17.616	2432	2436	2444	rVB2	15090	21327	0.42%	0.051%
49	18.004	2498	2502	2507	rVB4	16064	21348	0.42%	0.051%
50	18.216	2533	2538	2545	rBV5	30171	55461	1.09%	0.133%
51	19.233	2708	2711	2715	rBV3	26595	35613	0.70%	0.085%
52	19.298	2720	2722	2726	rVV	12784	13936	0.27%	0.033%
53	19.445	2745	2747	2750	rBV4	14865	16226	0.32%	0.039%
54	19.598	2770	2773	2776	rBV3	18645	20329	0.40%	0.049%
55	19.657	2777	2783	2790	rBV	2279851	3135474	61.48%	7.504%
56	21.127	3030	3033	3040	rBV5	109390	160839	3.15%	0.385%
57	21.410	3076	3081	3098	rBV	3492559	4913193	96.33%	11.759%
58	23.127	3370	3373	3378	rVB	203149	300688	5.90%	0.720%
59	23.698	3463	3470	3478	rVB2	1530527	3041682	59.64%	7.280%
60	23.780	3480	3484	3489	rVV	223624	382607	7.50%	0.916%
61	23.857	3490	3497	3511	rVB2	2418078	5100136	100.00%	12.206%




Sum of corrected areas: 41784181

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP102521\
Data File : BP007736.D
Acq On : 28 Oct 2021 00:35
Operator : CG/JU
Sample : M4215-14
Misc :
ALS Vial : 93 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
JDGE8

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SFAM-EPA-BP102521.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

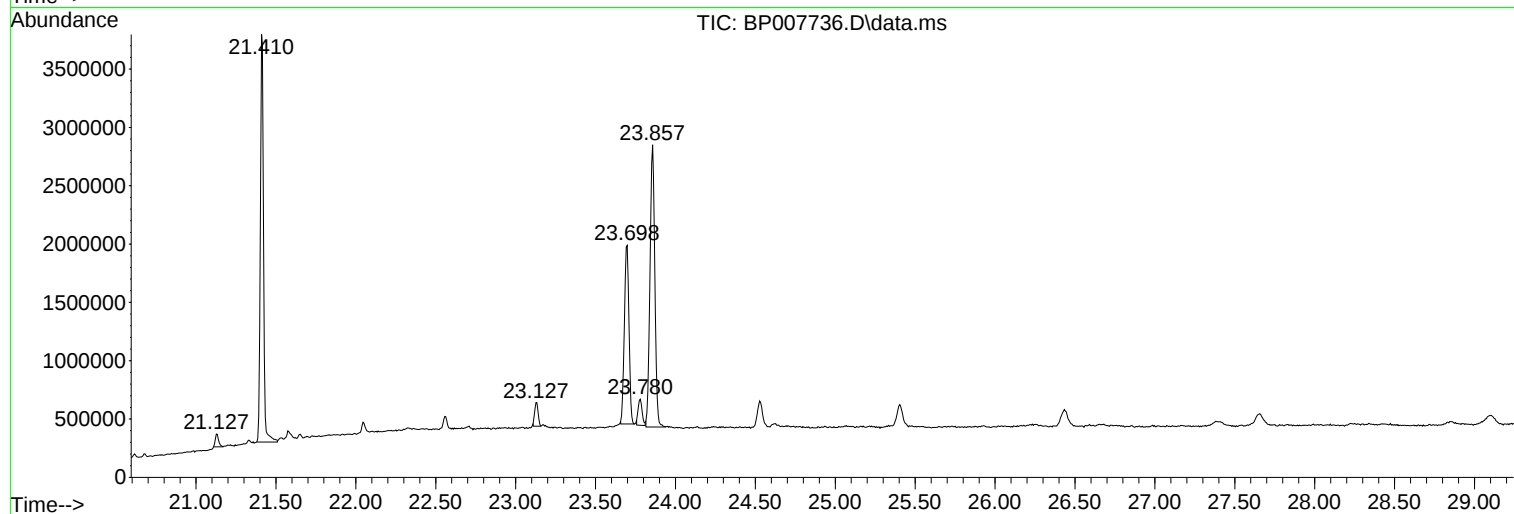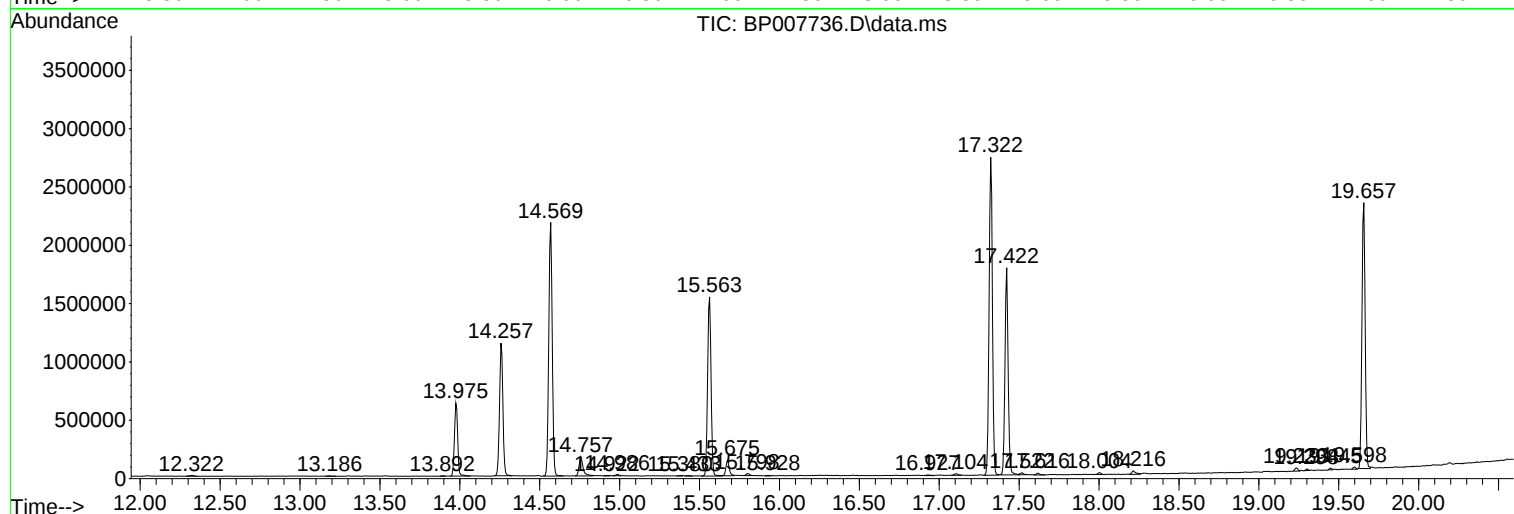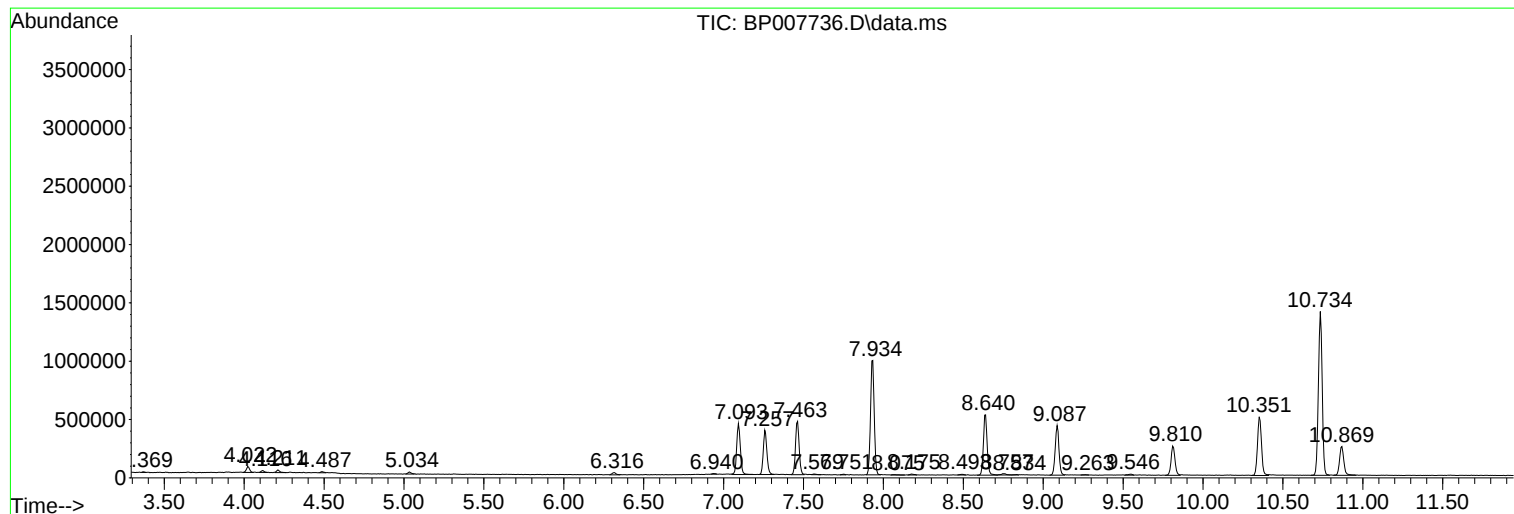

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP102521\
Data File : BP007736.D
Acq On : 28 Oct 2021 00:35
Operator : CG/JU
Sample : M4215-14
Misc :
ALS Vial : 93 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
JDGE8

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SFAM-EPA-BP102521.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP102521\
Data File : BP007736.D
Acq On : 28 Oct 2021 00:35
Operator : CG/JU
Sample : M4215-14
Misc :
ALS Vial : 93 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
JDGE8

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SFAM-EPA-BP102521.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
