

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP102521\
 Data File : BP007739.D
 Acq On : 28 Oct 2021 02:53
 Operator : CG/JU
 Sample : PB140099BL
 Misc :
 ALS Vial : 96 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SBLK099

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SFAM-EPA-BP102521.M
 Title : SVOA CALIBRATION

Signal : TIC: BP007739.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.369	9	14	22	rVB	49465	71002	1.19%	0.115%
2	3.781	80	84	102	rBV	675626	1036518	17.32%	1.681%
3	4.116	137	141	145	rVB2	13542	19104	0.32%	0.031%
4	7.093	640	647	659	rVB	823950	1304238	21.79%	2.115%
5	7.257	669	675	689	rVB	654565	1042563	17.42%	1.691%
6	7.463	702	710	722	rBV	850351	1341984	22.42%	2.176%
7	7.934	782	790	798	rBV	867395	1413824	23.62%	2.293%
8	8.640	902	910	921	rBV	1036290	1679383	28.06%	2.723%
9	9.087	978	986	998	rBV	762920	1283040	21.44%	2.081%
10	9.810	1099	1109	1121	rBV	610858	1046315	17.48%	1.697%
11	10.351	1192	1201	1217	rBV	1044328	1725265	28.83%	2.798%
12	10.734	1258	1266	1276	rVB	1275979	2094374	34.99%	3.396%
13	10.869	1281	1289	1298	rBV	1023296	1762723	29.45%	2.859%
14	11.540	1400	1403	1410	rVB9	2871	6433	0.11%	0.010%
15	12.322	1531	1536	1543	rVB2	19265	32568	0.54%	0.053%
16	12.534	1569	1572	1580	rVB9	4396	8599	0.14%	0.014%
17	13.545	1737	1744	1747	rBV7	5857	10984	0.18%	0.018%
18	13.981	1811	1818	1835	rBV	2078845	2944709	49.20%	4.775%
19	14.257	1858	1865	1880	rBV	2119910	3218491	53.77%	5.219%
20	14.569	1908	1918	1931	rBV	2124897	3027573	50.58%	4.910%
21	14.757	1943	1950	1964	rBV	958928	1412892	23.61%	2.291%
22	14.851	1964	1966	1975	rVV9	7985	19409	0.32%	0.031%
23	14.934	1975	1980	1982	rVV6	4973	8992	0.15%	0.015%
24	14.986	1986	1989	1993	rVB5	4983	7139	0.12%	0.012%
25	15.563	2079	2087	2096	rBV	2977224	4259310	71.16%	6.907%
26	15.681	2100	2107	2122	rVV	803679	1165516	19.47%	1.890%
27	15.804	2122	2128	2136	rVB	38466	64304	1.07%	0.104%
28	16.239	2197	2202	2210	rBV	4759	9379	0.16%	0.015%
29	16.998	2328	2331	2338	rVB9	4611	8290	0.14%	0.013%
30	17.110	2344	2350	2355	rBV3	11720	19786	0.33%	0.032%
31	17.322	2379	2386	2396	rBV	2537769	3738251	62.46%	6.062%
32	17.422	2396	2403	2416	rBV2	3387267	4870418	81.37%	7.898%
33	17.698	2445	2450	2454	rBV4	4844	9176	0.15%	0.015%
34	17.998	2498	2501	2506	rBV7	7564	8620	0.14%	0.014%
35	18.216	2535	2538	2540	rBV4	5552	6256	0.10%	0.010%
36	19.233	2707	2711	2717	rBV4	45029	70436	1.18%	0.114%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP102521\
Data File : BP007739.D
Acq On : 28 Oct 2021 02:53
Operator : CG/JU
Sample : PB140099BL
Misc :
ALS Vial : 96 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK099

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SFAM-EPA-BP102521.M
Title : SVOA CALIBRATION

37	19.304	2718	2723	2727	rBV	49197	67084	1.12%	0.109%
38	19.598	2770	2773	2777	rBV5	10629	12641	0.21%	0.020%
39	19.657	2777	2783	2791	rBV	4431016	5880894	98.26%	9.537%
40	21.416	3076	3082	3093	rBV	3264524	4415107	73.77%	7.160%
41	23.698	3463	3470	3479	rVB2	2937447	5985257	100.00%	9.706%
42	23.857	3490	3497	3512	rVB2	2150435	4555479	76.11%	7.388%




Sum of corrected areas: 61664326

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP102521\
Data File : BP007739.D
Acq On : 28 Oct 2021 02:53
Operator : CG/JU
Sample : PB140099BL
Misc :
ALS Vial : 96 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK099

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SFAM-EPA-BP102521.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

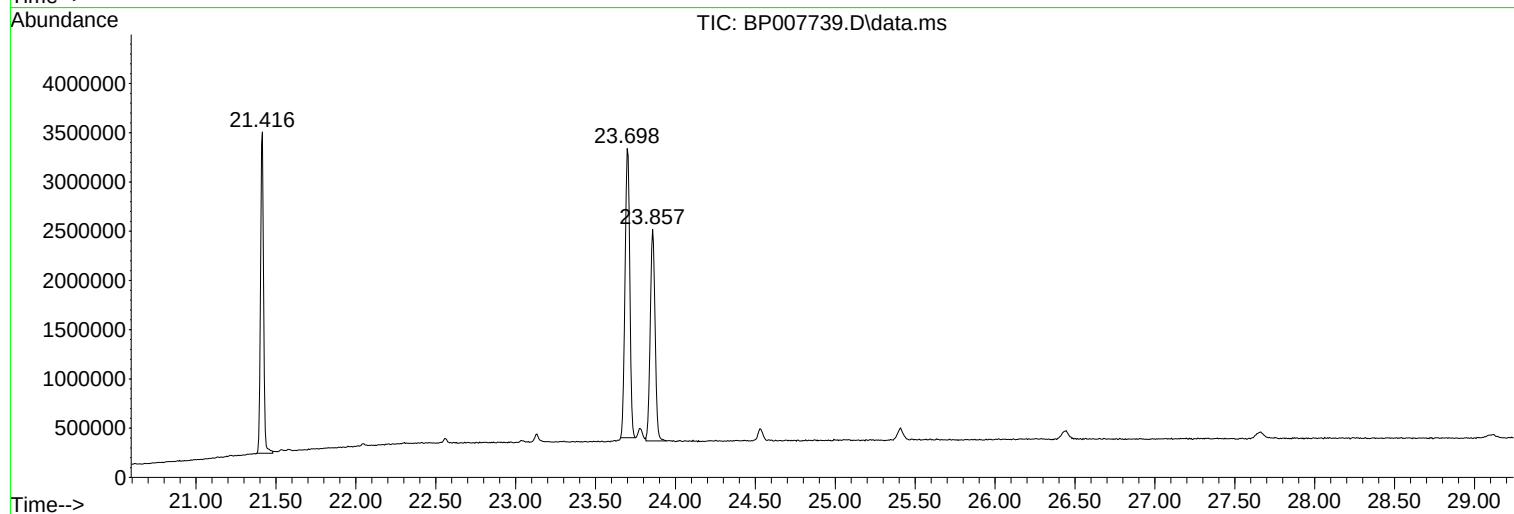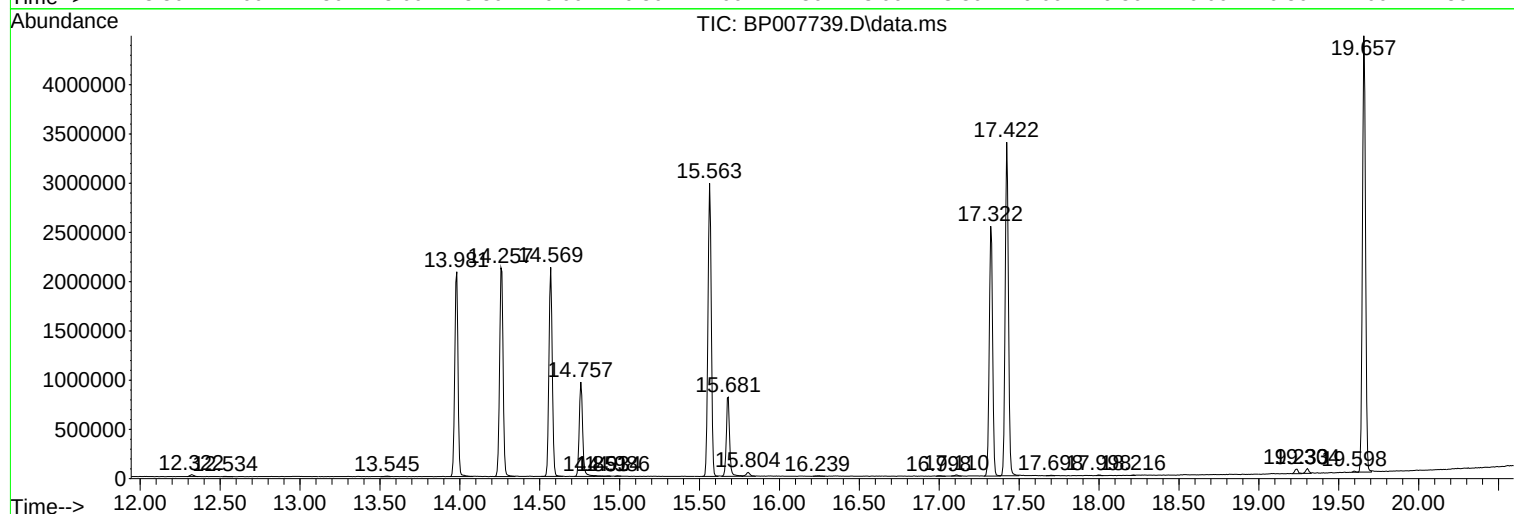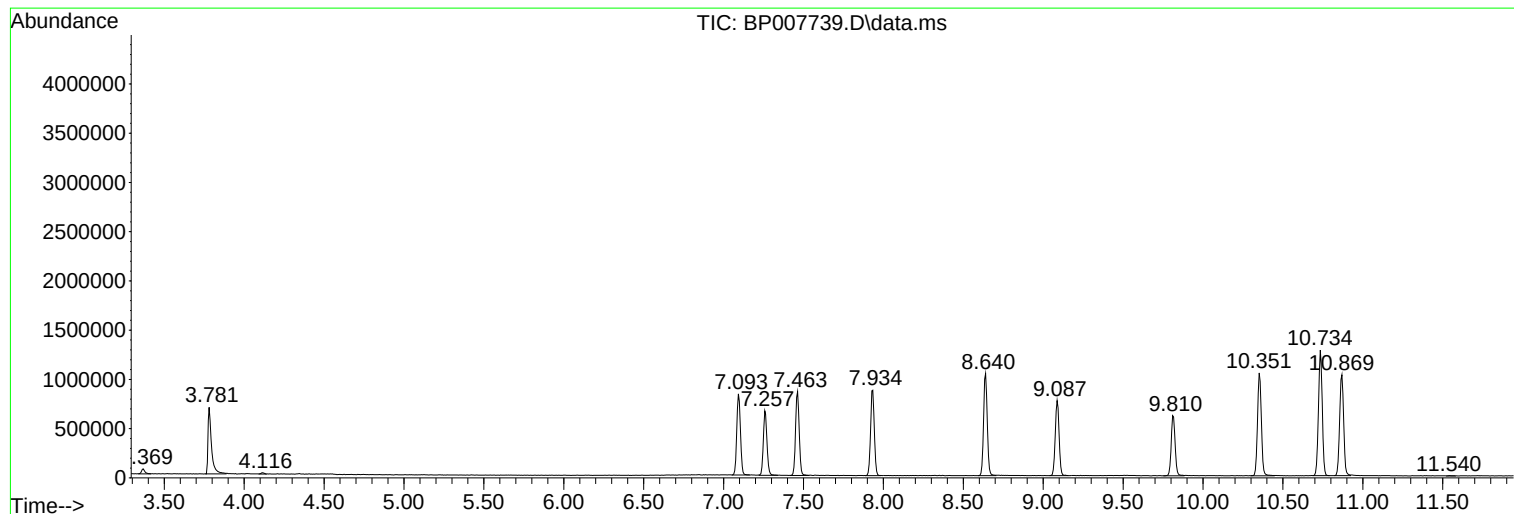

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP102521\
Data File : BP007739.D
Acq On : 28 Oct 2021 02:53
Operator : CG/JU
Sample : PB140099BL
Misc :
ALS Vial : 96 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK099

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SFAM-EPA-BP102521.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP102521\
Data File : BP007739.D
Acq On : 28 Oct 2021 02:53
Operator : CG/JU
Sample : PB140099BL
Misc :
ALS Vial : 96 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK099

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SFAM-EPA-BP102521.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
