

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP102521\
 Data File : BP007741.D
 Acq On : 28 Oct 2021 04:01
 Operator : CG/JU
 Sample : M4215-19
 Misc :
 ALS Vial : 98 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 JDGF6

Integration Parameters: LSCINT.P

Integrator: RTE

Soothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SFAM-EPA-BP102521.M
 Title : SVOA CALIBRATION

Signal : TIC: BP007741.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.370	10	14	23	rVB	56267	74980	0.85%	0.090%
2	3.787	82	85	99	rBV	289319	439497	5.00%	0.525%
3	4.117	138	141	147	rVB2	20681	26934	0.31%	0.032%
4	6.317	511	515	521	rVB8	5604	11010	0.13%	0.013%
5	7.099	640	648	659	rBV	1381854	2182414	24.83%	2.606%
6	7.264	669	676	686	rVB	1046793	1672901	19.03%	1.998%
7	7.464	703	710	725	rVB	1409216	2254751	25.65%	2.693%
8	7.934	783	790	798	rBV	1088968	1680462	19.12%	2.007%
9	8.011	798	803	809	rVB5	8015	12735	0.14%	0.015%
10	8.640	903	910	920	rBV	1699803	2800105	31.85%	3.344%
11	9.093	978	987	998	rBV	1320915	2164125	24.62%	2.584%
12	9.540	1061	1063	1070	rVB5	7777	14311	0.16%	0.017%
13	9.816	1102	1110	1118	rBV	1105816	1835638	20.88%	2.192%
14	10.357	1194	1202	1218	rBV	1732622	2966762	33.75%	3.543%
15	10.516	1222	1229	1241	rVB	84899	151102	1.72%	0.180%
16	10.740	1259	1267	1275	rBV	1460116	2456068	27.94%	2.933%
17	10.869	1280	1289	1303	rBV	1410708	2445954	27.82%	2.921%
18	12.322	1530	1536	1544	rVB2	29998	57240	0.65%	0.068%
19	12.534	1566	1572	1579	rBV2	4600	9933	0.11%	0.012%
20	12.940	1636	1641	1646	rBV9	8603	13792	0.16%	0.016%
21	13.181	1679	1682	1689	rBV9	10659	18050	0.21%	0.022%
22	13.475	1730	1732	1739	rBV8	8468	14035	0.16%	0.017%
23	13.546	1740	1744	1750	rVB4	13924	22725	0.26%	0.027%
24	13.981	1811	1818	1824	rBV	3174224	4394677	49.99%	5.248%
25	14.263	1859	1866	1876	rBV	3821653	5621643	63.95%	6.713%
26	14.445	1895	1897	1899	rVB3	12594	10124	0.12%	0.012%
27	14.575	1912	1919	1927	rBV	2374212	3579551	40.72%	4.275%
28	14.763	1945	1951	1960	rBV	1414838	2040598	23.21%	2.437%
29	14.987	1986	1989	1996	rBV5	18984	28515	0.32%	0.034%
30	15.569	2081	2088	2095	rBV	4913398	7010992	79.76%	8.372%
31	15.681	2101	2107	2116	rBV	1312362	1876186	21.34%	2.240%
32	15.810	2126	2129	2134	rVB	53888	75883	0.86%	0.091%
33	17.328	2382	2387	2393	rVB	2993700	4253270	48.38%	5.079%
34	17.428	2398	2404	2414	rVB2	5061759	7595705	86.41%	9.071%
35	18.710	2620	2622	2624	rBV2	316512	307433	3.50%	0.367%
36	19.663	2779	2784	2790	rBV	6331592	8575248	97.55%	10.240%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP102521\
Data File : BP007741.D
Acq On : 28 Oct 2021 04:01
Operator : CG/JU
Sample : M4215-19
Misc :
ALS Vial : 98 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
JDGF6

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SFAM-EPA-BP102521.M
Title : SVOA CALIBRATION

37	21.416	3079	3082	3089	rVB	4042897	6254069	71.15%	7.468%
38	23.710	3466	3472	3480	rVB2	4314374	8790550	100.00%	10.497%




Sum of corrected areas: 83739968

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP102521\
Data File : BP007741.D
Acq On : 28 Oct 2021 04:01
Operator : CG/JU
Sample : M4215-19
Misc :
ALS Vial : 98 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
JDGF6

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SFAM-EPA-BP102521.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

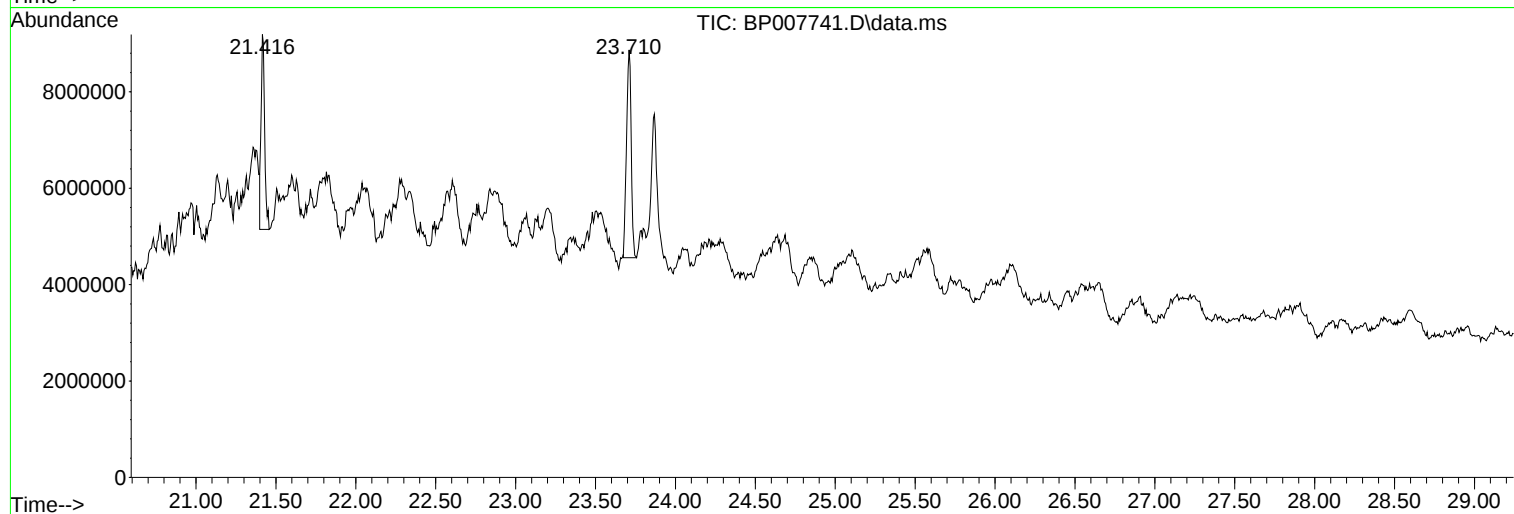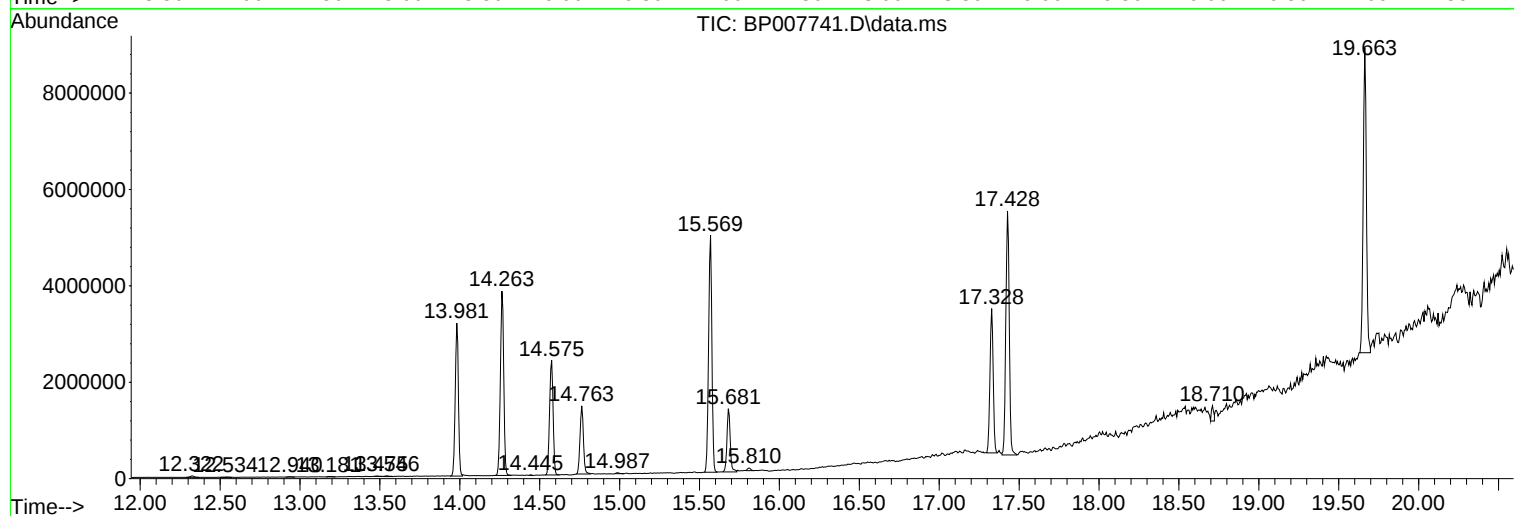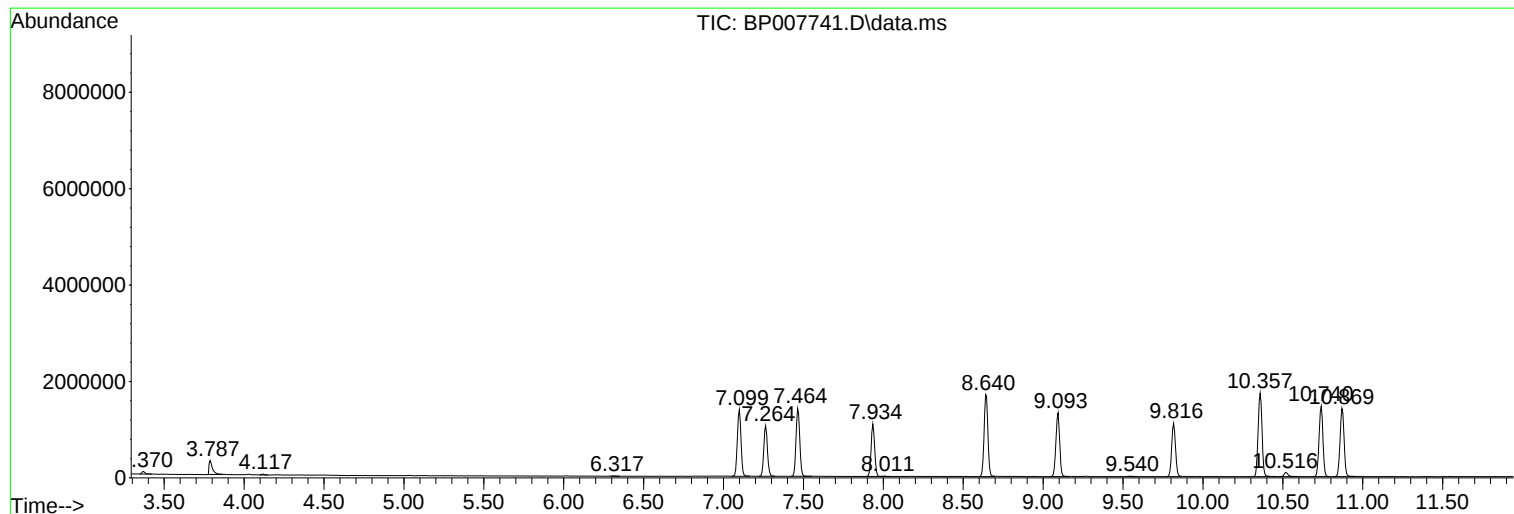

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP102521\
Data File : BP007741.D
Acq On : 28 Oct 2021 04:01
Operator : CG/JU
Sample : M4215-19
Misc :
ALS Vial : 98 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
JDGF6

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SFAM-EPA-BP102521.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP102521\
Data File : BP007741.D
Acq On : 28 Oct 2021 04:01
Operator : CG/JU
Sample : M4215-19
Misc :
ALS Vial : 98 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
JDGF6

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SFAM-EPA-BP102521.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
