
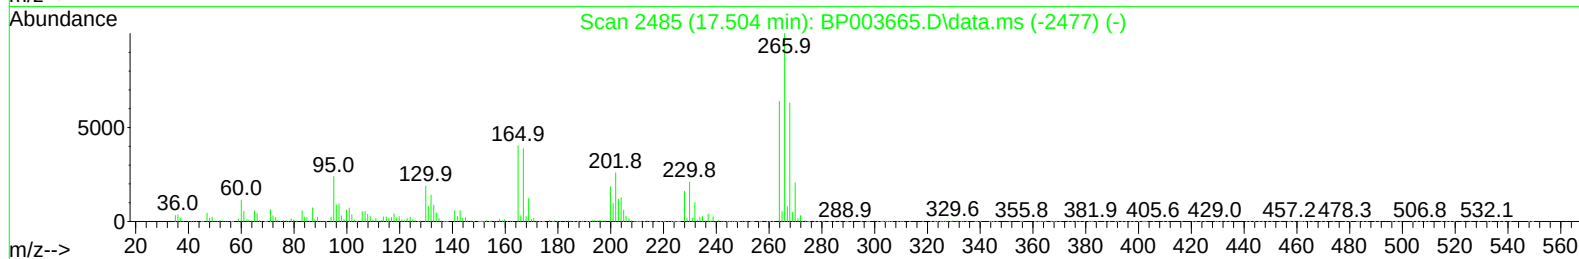
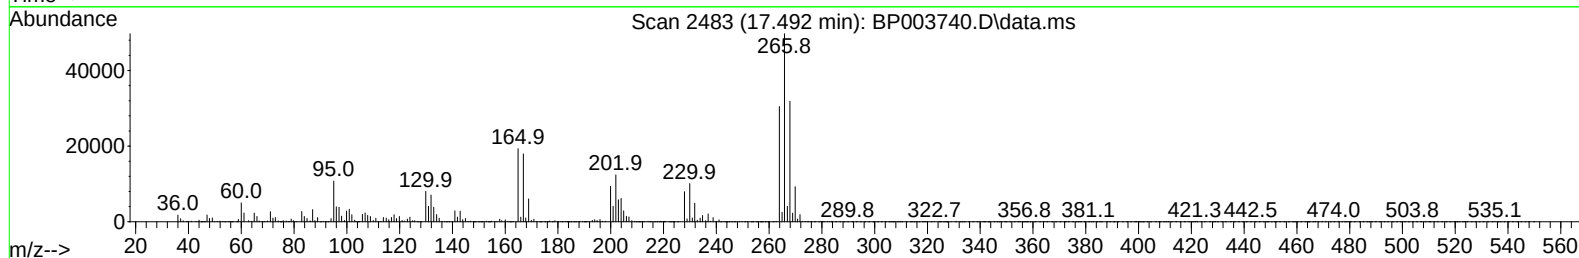


Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP102620\
Data File : BP003740.D
Acq On : 26 Oct 2020 14:45
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Oct 27 02:51:54 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\8270-BP101920.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Oct 26 16:22:21 2020
Response via : Initial Calibration

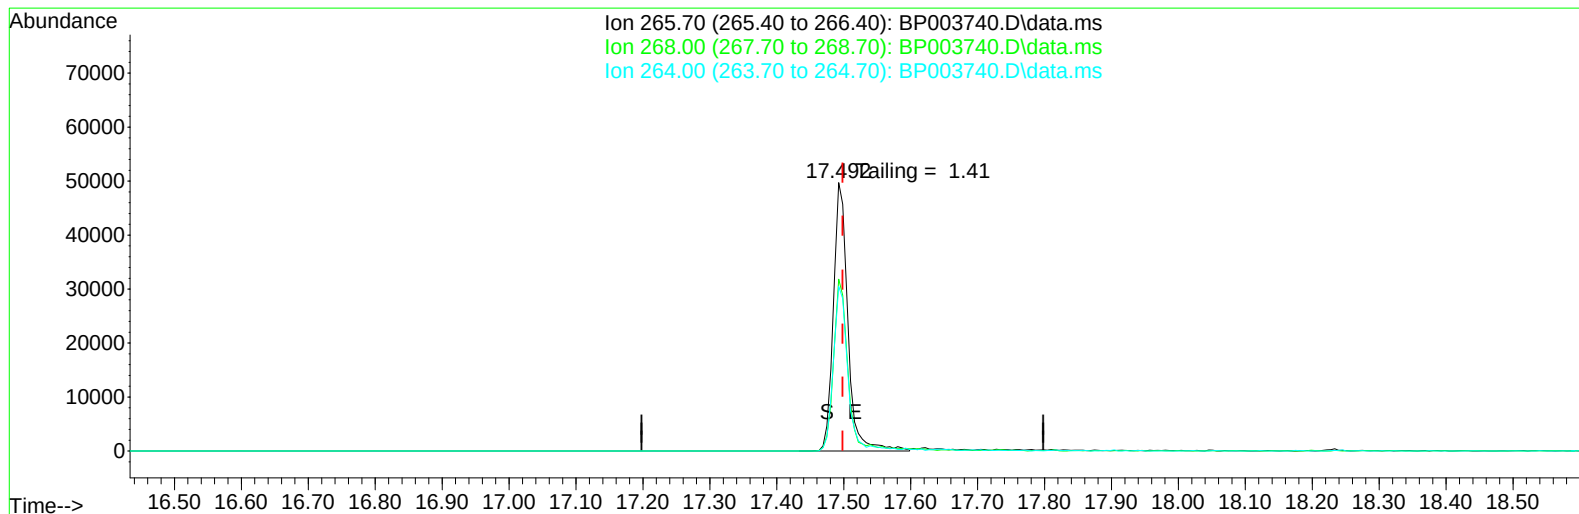

TIC: BP003740.D\data.ms

(70) Pentachlorophenol (C)




17.492min (-0.006) 50095.05 ng

response 75476

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	63.90	64.05
264.00	63.30	61.28
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP102620\
Data File : BP003740.D
Acq On : 26 Oct 2020 14:45
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Oct 27 02:51:54 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\8270-BP101920.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Oct 26 16:22:21 2020
Response via : Initial Calibration

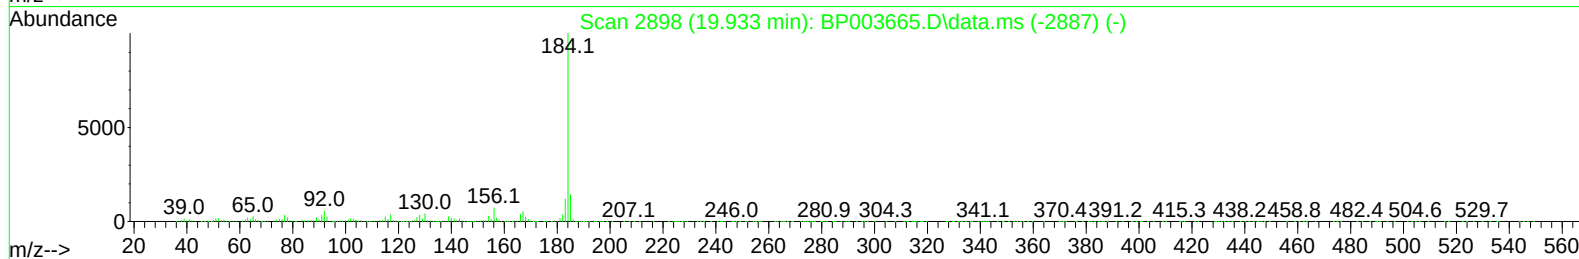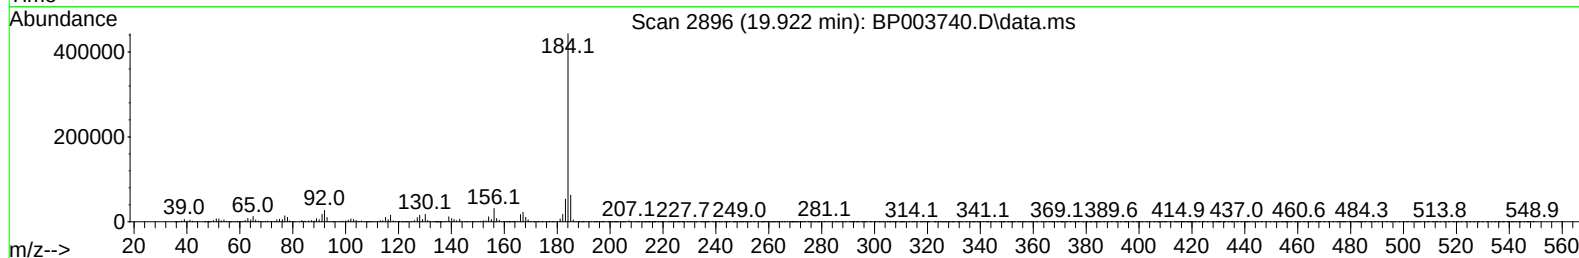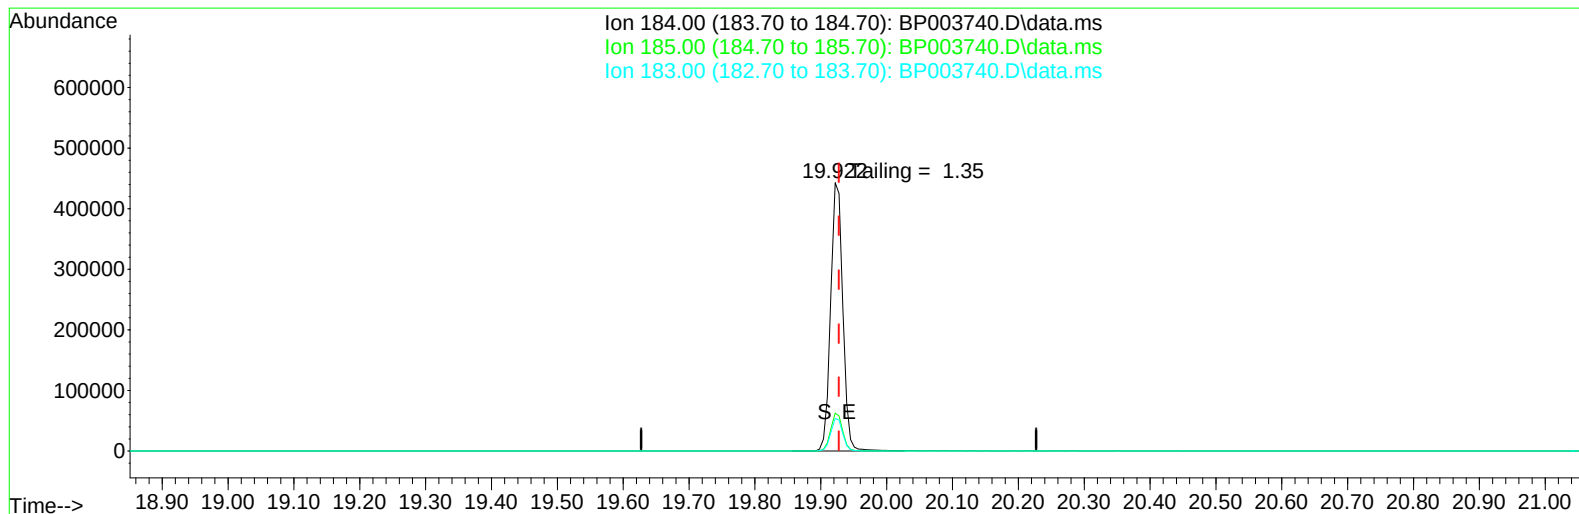

TIC: BP003740.D\data.ms

(77) Benzidine

19.922min (-0.006) 21183.01 ng

response 569977

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.40	14.16
183.00	12.00	12.13
0.00	0.00	0.00