

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP102620\
 Data File : BP003742.D
 Acq On : 26 Oct 2020 15:53
 Operator : CG/JU
 Sample : PB132578BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 PB132578BL

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON Filtering: 5
 Sampling : 1 Min Area: 3 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\8270-BP101920.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BP003742.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.087	29	34	54	rVB	9030800	11646965	100.00%	26.079%
2	6.011	523	531	543	rBV	2004406	3010402	25.85%	6.741%
3	7.658	803	811	821	rBV	1866834	3047251	26.16%	6.823%
4	8.510	948	956	967	rVB	400490	650212	5.58%	1.456%
5	9.675	1143	1154	1168	rBV	1278894	2094167	17.98%	4.689%
6	11.351	1431	1439	1449	rVB	501862	828663	7.11%	1.855%
7	13.734	1835	1844	1852	rBV	3355988	4970004	42.67%	11.129%
8	15.110	2070	2078	2087	rBV2	746110	1116044	9.58%	2.499%
9	16.581	2320	2328	2343	rBV	2569798	3680089	31.60%	8.240%
10	17.828	2532	2540	2552	rBV	1023776	1410506	12.11%	3.158%
11	20.298	2954	2960	2965	rBV	7488664	8807633	75.62%	19.722%
12	21.839	3217	3222	3233	rVB	1305110	1729378	14.85%	3.872%
13	24.410	3651	3659	3669	rVB	804203	1668742	14.33%	3.737%




Sum of corrected areas: 44660056

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP102620\
Data File : BP003742.D
Acq On : 26 Oct 2020 15:53
Operator : CG/JU
Sample : PB132578BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
PB132578BL

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\8270-BP101920.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

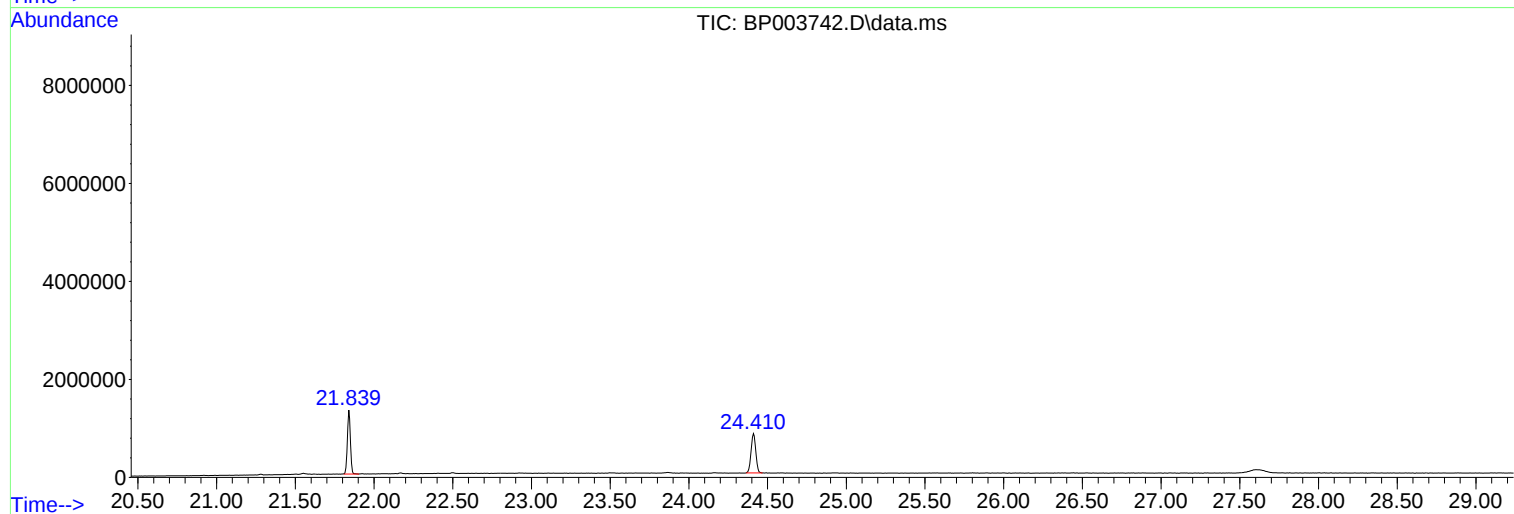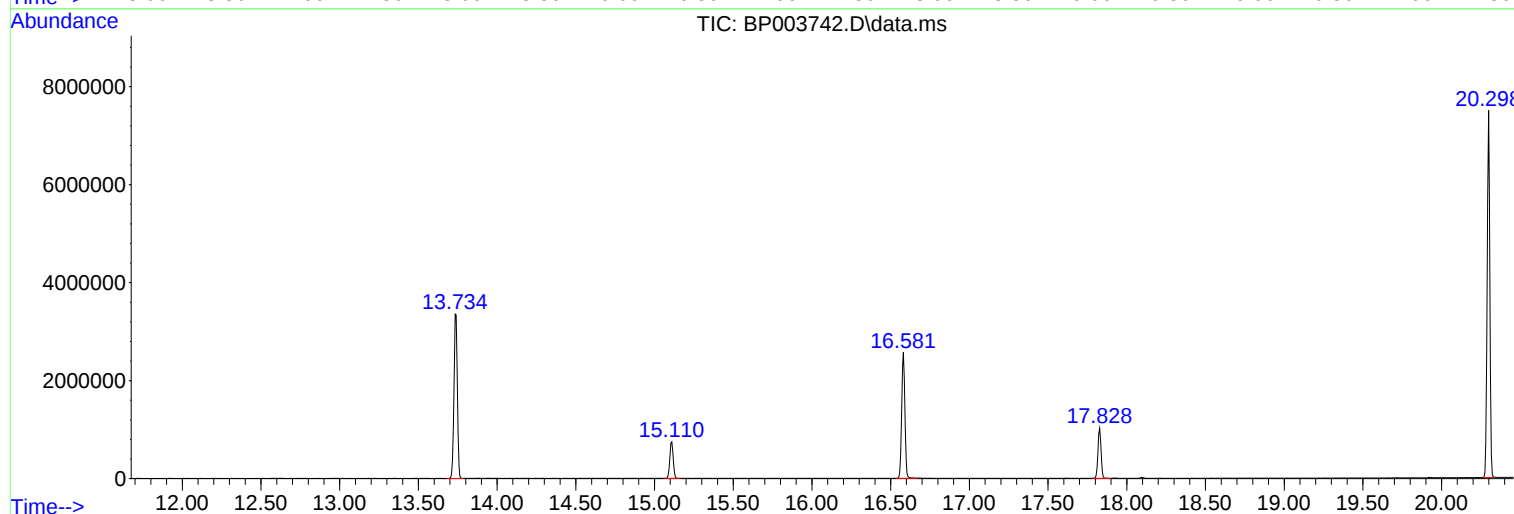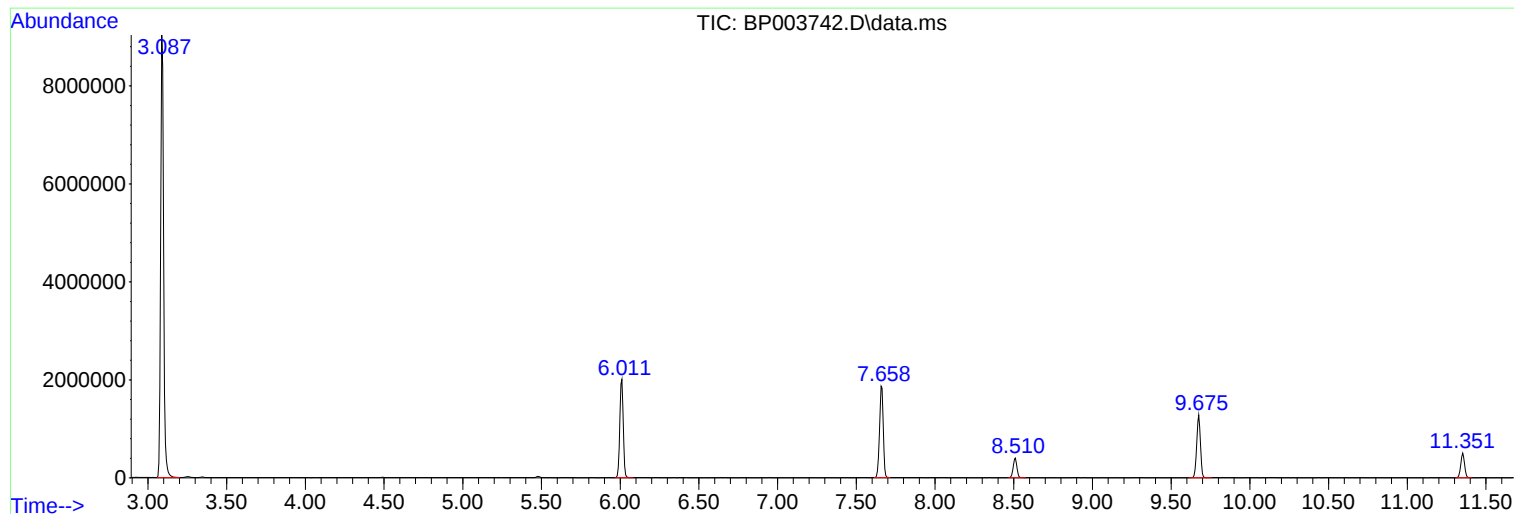

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP102620\
Data File : BP003742.D
Acq On : 26 Oct 2020 15:53
Operator : CG/JU
Sample : PB132578BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
PB132578BL










Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\8270-BP101920.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 Propane, 2,2-dimethoxy- Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
3.087	358.25 ng	11647000	1,4-Dichlorobenzene-d4	8.510

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			Propane, 2,2-dimethoxy-	104	C5H12O2	000077-76-9	50
2			Pentane, 3-methoxy-	102	C6H14O	036839-67-5	17
3			2-Hydroxy-2-methylbutyric acid	118	C5H10O3	003739-30-8	9
4			Propane, 2-methoxy-2-methyl-	88	C5H12O	001634-04-4	9
5			1-Hexen-4-ol, 1-chloro-3,5-dimet...	162	C8H15ClO	100244-09-5	9

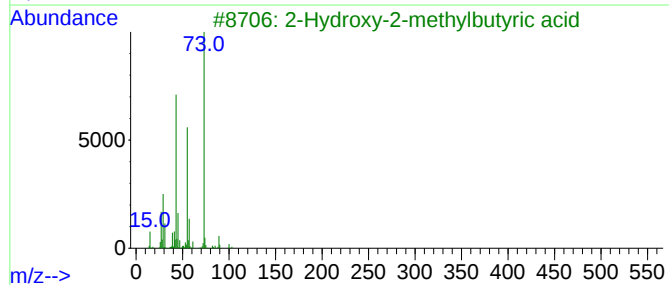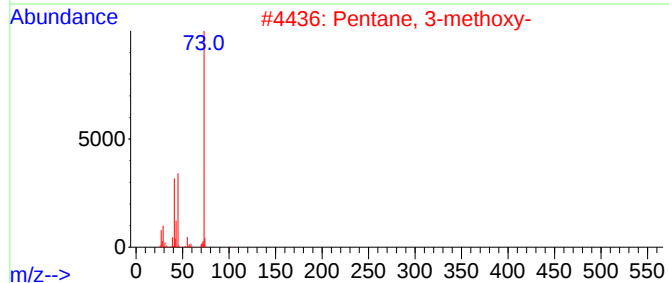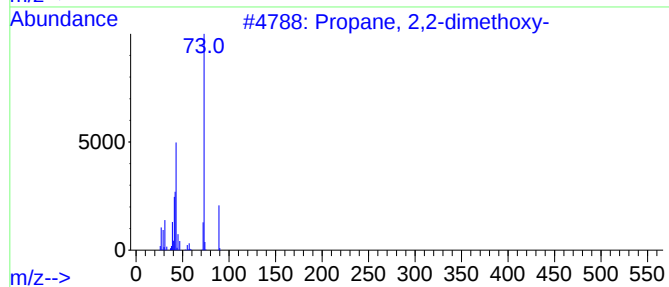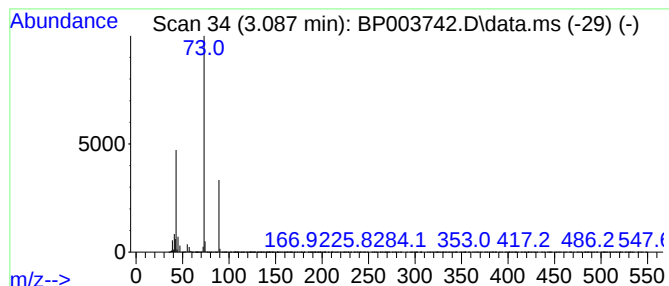

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP102620\
Data File : BP003742.D
Acq On : 26 Oct 2020 15:53
Operator : CG/JU
Sample : PB132578BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
PB132578BL

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\8270-BP101920.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
Propane, 2,2-di...	3.087	358.3	ng	11647000	1	8.510	650212	20.0