
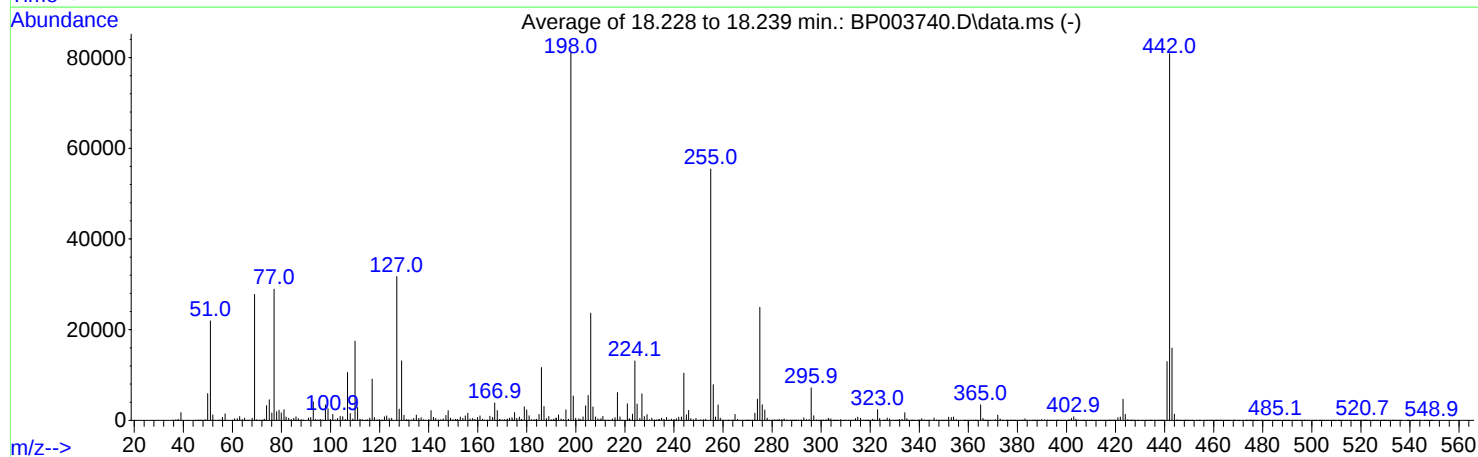


Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP102620\
 Data File : BP003740.D
 Acq On : 26 Oct 2020 14:45
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\8270-BP101920.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Mon Oct 26 16:22:21 2020

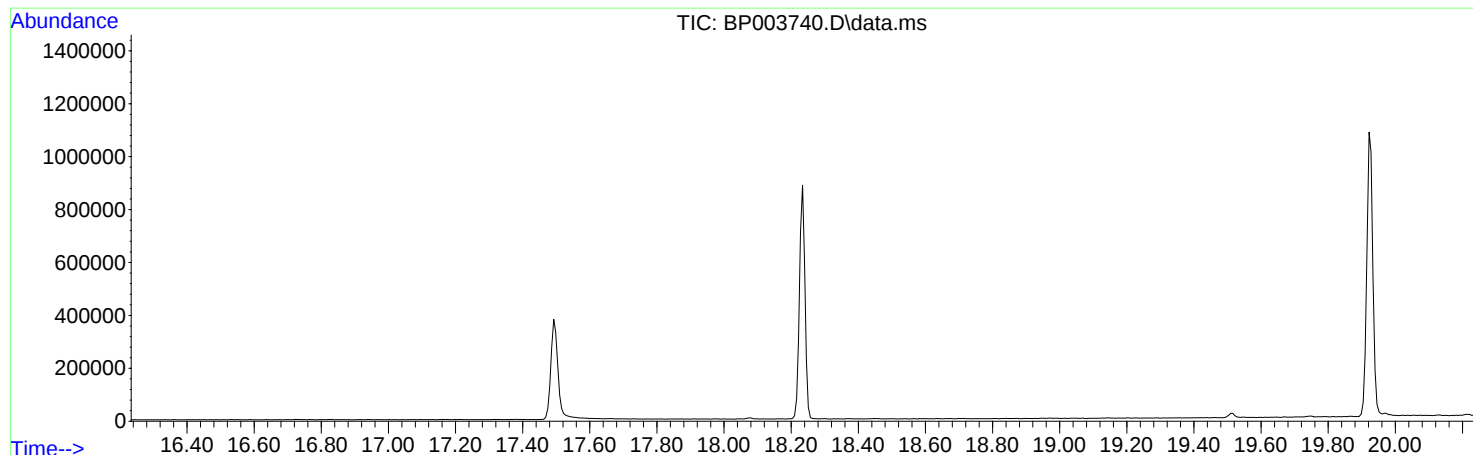

AutoFind: Scans 2608, 2609, 2610; Background Corrected with Scan 2599

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	27.0	21936	PASS
68	69	0.00	2	1.8	505	PASS
69	198	0.00	100	34.2	27768	PASS
70	69	0.00	2	0.5	128	PASS
127	198	10	80	39.1	31712	PASS
197	198	0.00	2	0.3	260	PASS
198	198	100	100	100.0	81123	PASS
199	198	5	9	6.6	5366	PASS
275	198	10	60	30.8	24949	PASS
365	198	1	100	4.2	3442	PASS
441	198	0.01	100	16.0	12944	PASS
442	198	50	100	99.7	80840	PASS
443	442	15	24	19.7	15945	PASS