

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP110222\
 Data File : BP012454.D
 Acq On : 02 Nov 2022 15:21
 Operator : CG/JU
 Sample : N5321-05
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DBXA4

Quant Time: Nov 02 23:14:43 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP102522.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue Nov 01 01:03:58 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.787	152	299683	20.000	ng/u1	0.00
20) Naphthalene-d8	10.587	136	1402720	20.000	ng/u1	-0.01
38) Acenaphthene-d10	14.440	164	955941	20.000	ng/u1	0.00
64) Phenanthrene-d10	17.204	188	2131220	20.000	ng/u1	0.00
79) Chrysene-d12	21.298	240	1956818	20.000	ng/u1	0.00
88) Perylene-d12	23.686	264	1693748	20.000	ng/u1	-0.01
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.199	96	553621	74.384	ng/uL	-0.04
4) Pyridine-d5	3.664	84	125999	5.893	ng/u1	0.00
7) Phenol-d5	6.963	99	212389	7.902	ng/u1	0.00
9) Bis-(2-Chloroethyl)eth...	7.128	67	533444	33.245	ng/u1	0.00
11) 2-Chlorophenol-d4	7.322	132	555121	28.281	ng/u1	0.00
15) 4-Methylphenol-d8	8.505	113	409992	19.286	ng/u1	0.00
21) Nitrobenzene-d5	8.957	128	372407	40.940	ng/u1	0.00
24) 2-Nitrophenol-d4	9.675	143	404003	42.791	ng/u1	-0.01
28) 2,4-Dichlorophenol-d3	10.216	165	693352	33.886	ng/u1	0.00
31) 4-Chloroaniline-d4	10.740	131	771519	25.324	ng/u1	0.00
46) Dimethylphthalate-d6	13.857	166	2495880	38.140	ng/u1	0.00
49) Acenaphthylene-d8	14.134	160	2728983	36.492	ng/u1	0.00
54) 4-Nitrophenol-d4	14.675	143	78647	6.350	ng/u1	0.00
60) Fluorene-d10	15.439	176	2143506	38.258	ng/u1	0.00
65) 4,6-Dinitro-2-methylph...	15.575	200	376716	33.951	ng/u1	0.00
73) Anthracene-d10	17.304	188	3480542	37.902	ng/u1	0.00
81) Pyrene-d10	19.545	212	4009754	40.814	ng/u1	0.00
92) Benzo(a)pyrene-d12	23.533	264	3194223	38.597	ng/u1	-0.01


Target Compounds					Qvalue
2) 1,4-Dioxane	3.270	88	11358	1.435 ng/uL#	93


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP110222\
Data File : BP012454.D
Acq On : 02 Nov 2022 15:21
Operator : CG/JU
Sample : N5321-05
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DBXA4

Quant Time: Nov 02 23:14:43 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP102522.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue Nov 01 01:03:58 2022
Response via : Initial Calibration

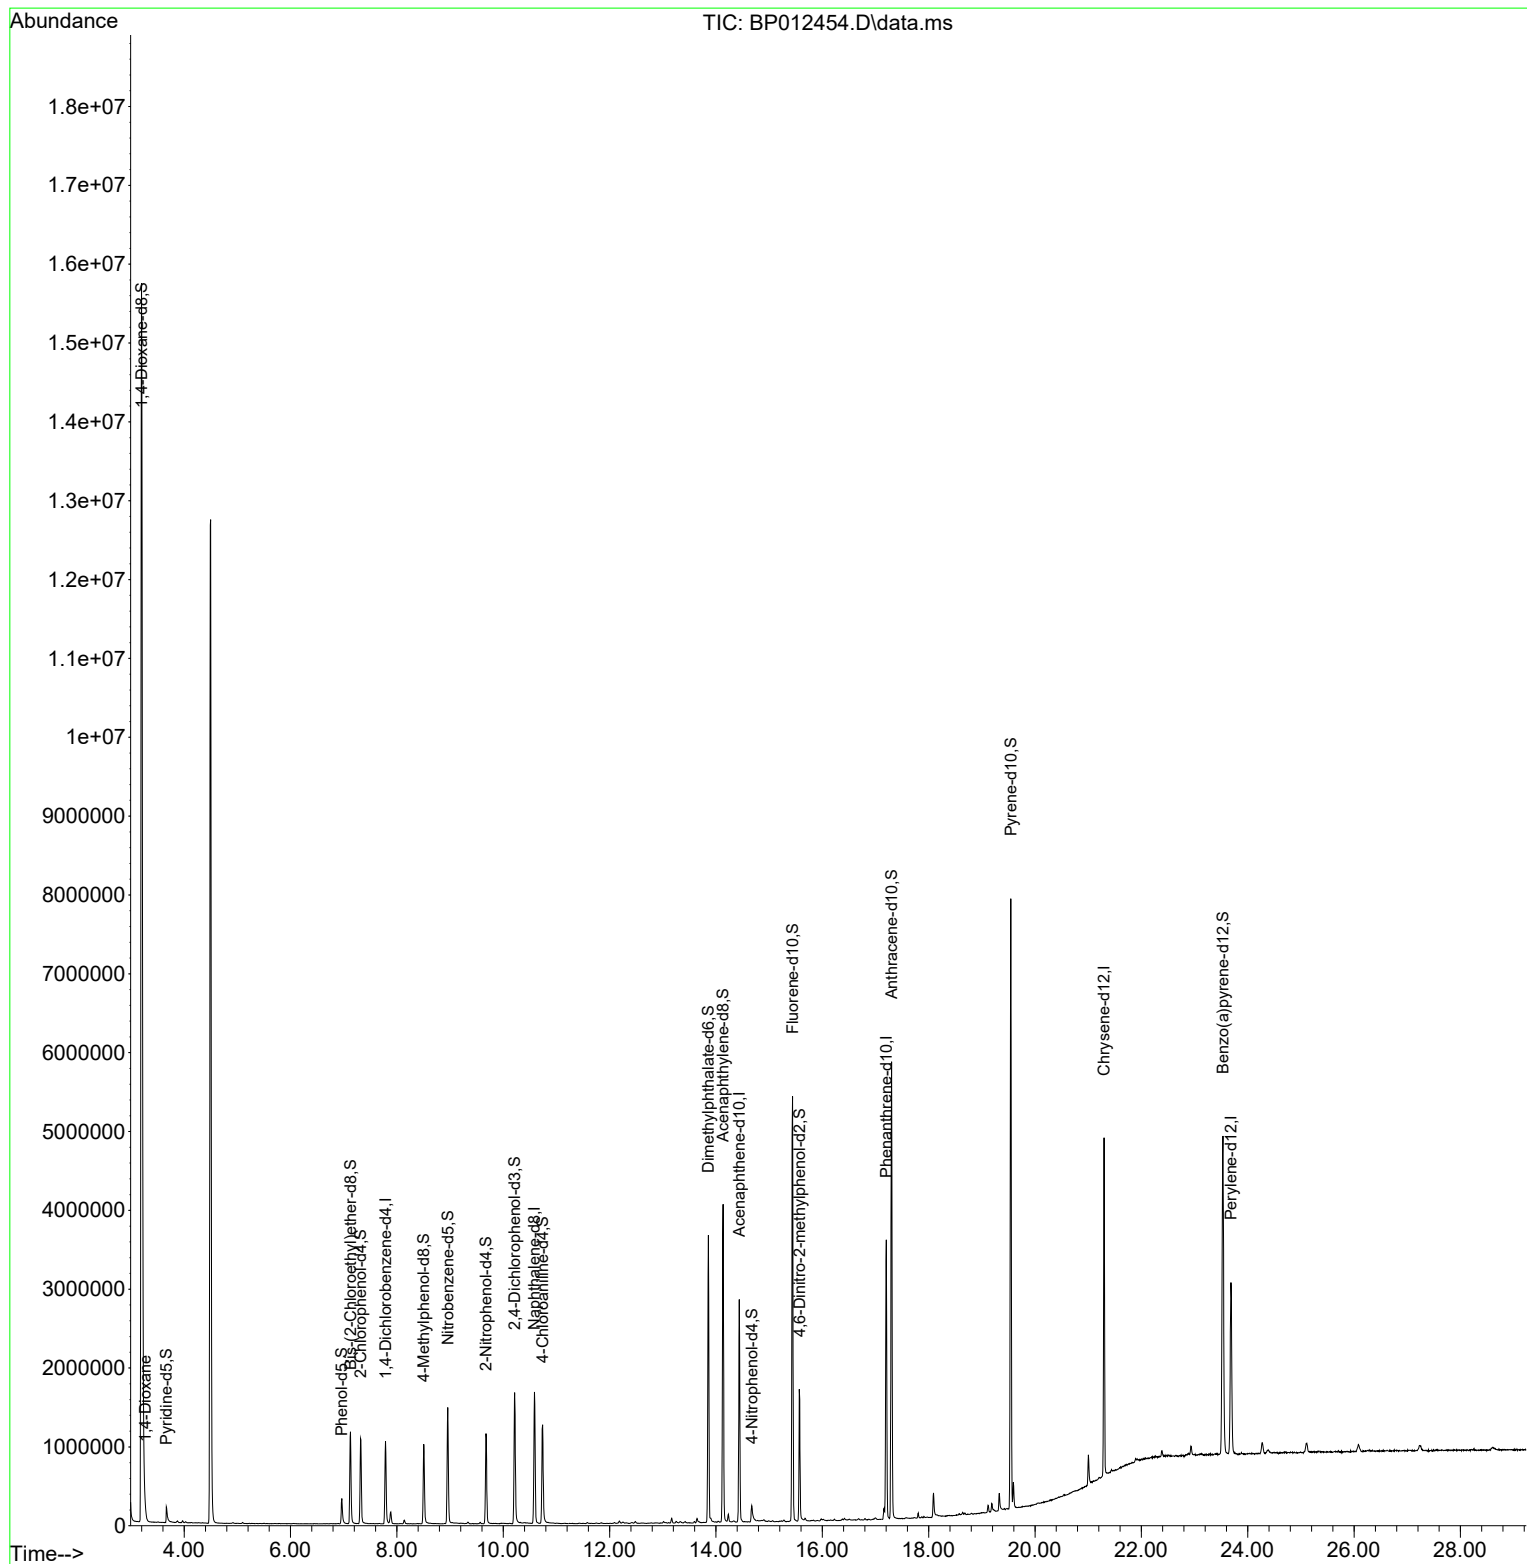

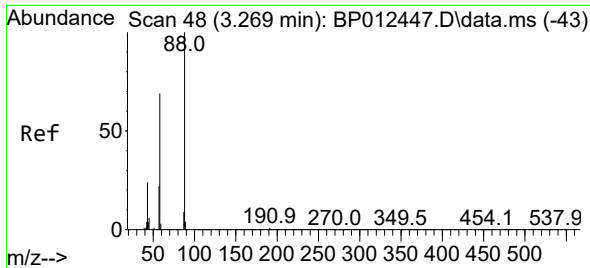

#2
 1,4-Dioxane
 Concen: 1.435 ng/uL
 RT: 3.270 min Scan# 41
 Delta R.T. -0.006 min
 Lab File: BP012454.D
 Acq: 02 Nov 2022 15:21

Instrument :
 BNA_P
 ClientSampleId :
 DBXA4

Tgt Ion: 88 Resp: 11358
 Ion Ratio Lower Upper
 88 100
 43 35.3 20.6 31.0#
 58 70.5 58.0 87.0

