




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP110222\
 Data File : BP012520.D
 Acq On : 04 Nov 2022 09:17
 Operator : CG/JU
 Sample : N5353-08
 Misc :
 ALS Vial : 77 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DBWR2

Manual IntegrationsAPPROVED

Reviewed By :Yogesh Patel 11/05/2022
 Supervised By :mohammad ahmed 11/06/2022

Quant Time: Nov 05 03:26:32 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP102522.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri Nov 04 02:53:36 2022
 Response via : Initial Calibration

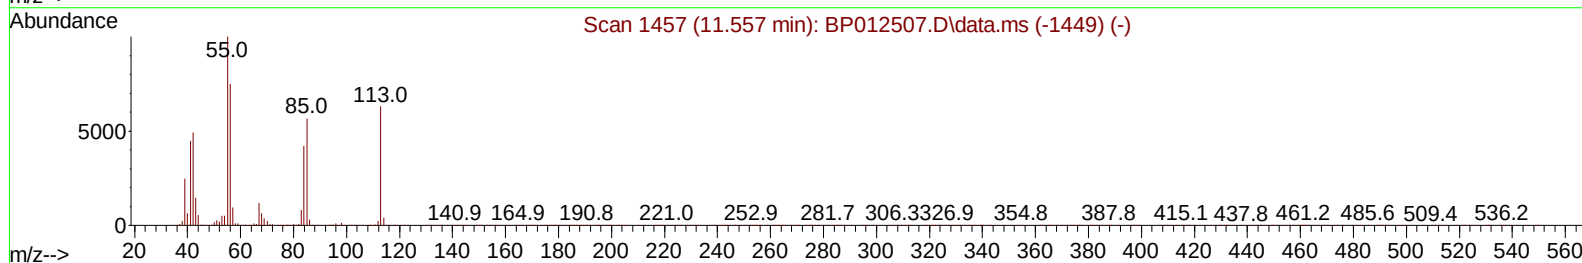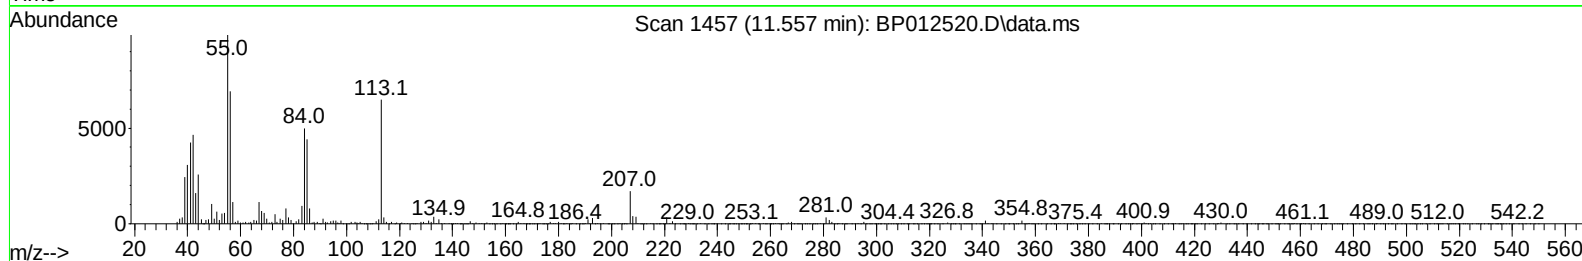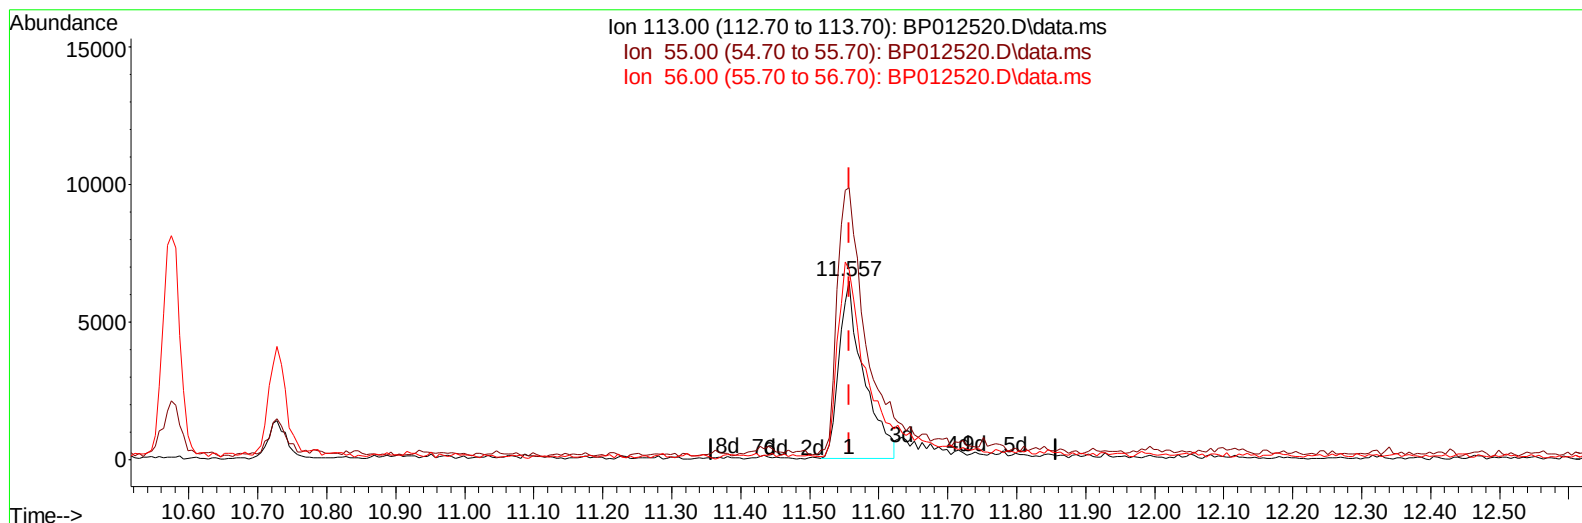

TIC: BP012520.D\data.ms

(34) Caprolactam

11.557min (0.000) 2.29 ng/ul

response 16035

Ion	Exp%	Act%
113.00	100.00	100.00
55.00	169.50	152.23
56.00	123.60	106.60
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP110222\
 Data File : BP012520.D
 Acq On : 04 Nov 2022 09:17
 Operator : CG/JU
 Sample : N5353-08
 Misc :
 ALS Vial : 77 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DBWR2

Manual IntegrationsAPPROVED

Quant Time: Nov 05 03:26:32 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP102522.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri Nov 04 02:53:36 2022
 Response via : Initial Calibration

Reviewed By :Yogesh Patel 11/05/2022
 Supervised By :mohammad ahmed 11/06/2022

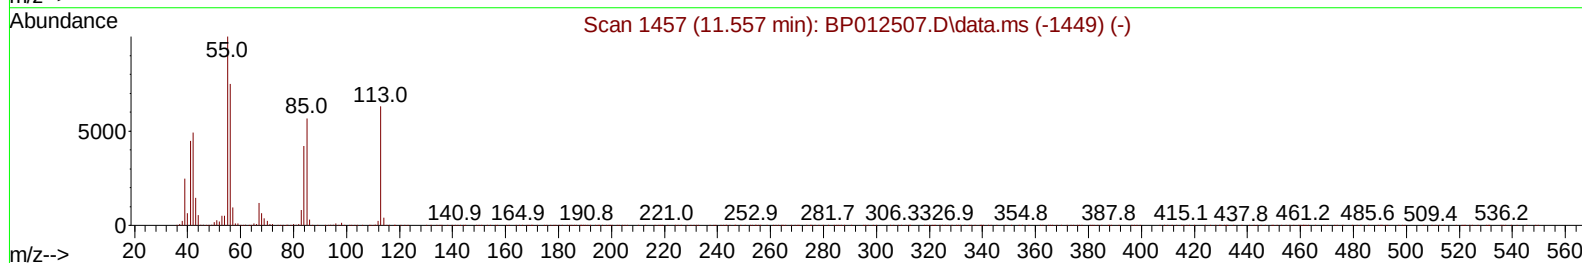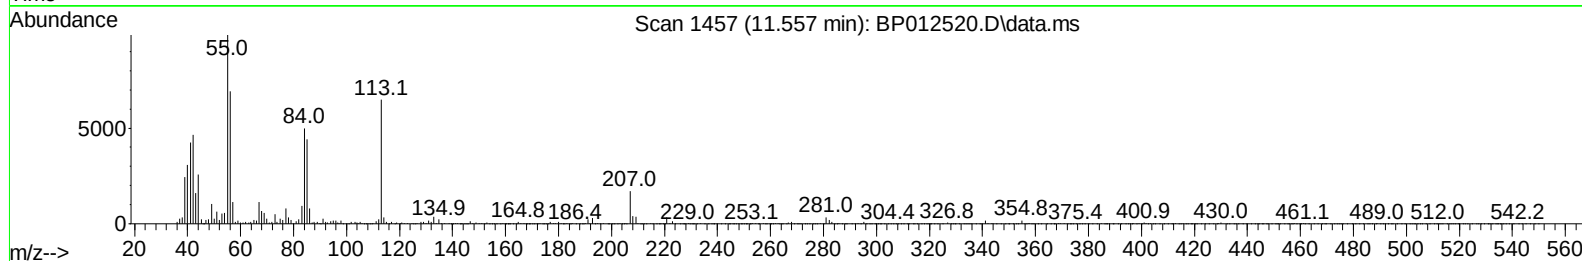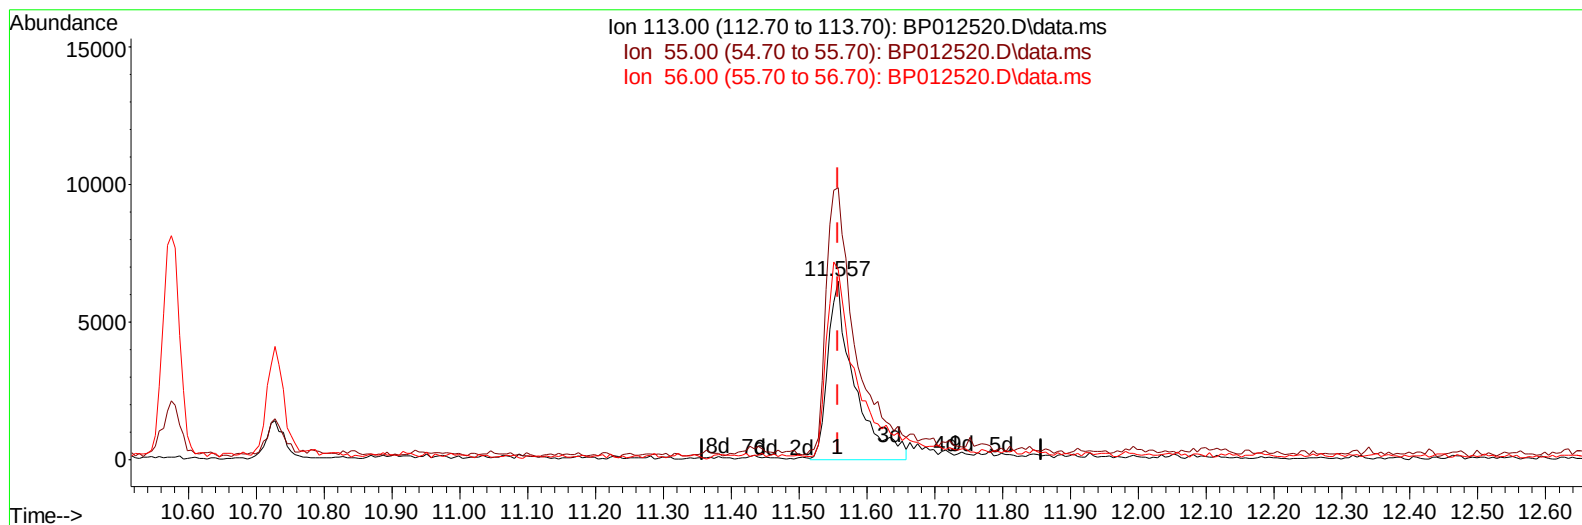

TIC: BP012520.D\data.ms

(34) Caprolactam

11.557min (0.000) 2.50 ng/ul m

response 17535

Ion	Exp%	Act%
113.00	100.00	100.00
55.00	169.50	152.23
56.00	123.60	106.60
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP110222\
 Data File : BP012520.D
 Acq On : 04 Nov 2022 09:17
 Operator : CG/JU
 Sample : N5353-08
 Misc :
 ALS Vial : 77 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DBWR2

Manual IntegrationsAPPROVED

Reviewed By :Yogesh Patel 11/05/2022
 Supervised By :mohammad ahmed 11/06/2022

Quant Time: Nov 05 03:26:32 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP102522.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri Nov 04 02:53:36 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.775	152	287530	20.000	ng/ul	0.00
20) Naphthalene-d8	10.575	136	1359124	20.000	ng/ul	0.00
38) Acenaphthene-d10	14.428	164	940624	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.192	188	2119122	20.000	ng/ul	0.00
79) Chrysene-d12	21.286	240	1865978	20.000	ng/ul	0.00
88) Perylene-d12	23.668	264	1644748	20.000	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.228	96	26622	3.728	ng/uL	0.00
4) Pyridine-d5	3.664	84	139211	6.786	ng/ul	0.01
7) Phenol-d5	6.958	99	149882	5.812	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	7.116	67	466069	30.273	ng/ul	0.00
11) 2-Chlorophenol-d4	7.310	132	457948	24.316	ng/ul	0.00
15) 4-Methylphenol-d8	8.499	113	316213	15.503	ng/ul	0.00
21) Nitrobenzene-d5	8.946	128	329452	37.380	ng/ul	0.00
24) 2-Nitrophenol-d4	9.669	143	347217	37.956	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.204	165	599858	30.257	ng/ul	0.00
31) 4-Chloroaniline-d4	10.728	131	776898	26.319	ng/ul	0.00
46) Dimethylphthalate-d6	13.845	166	2353202	36.546	ng/ul	0.00
49) Acenaphthylene-d8	14.122	160	2479552	33.697	ng/ul	0.00
54) 4-Nitrophenol-d4	14.681	143	46856	3.845	ng/ul	0.02
60) Fluorene-d10	15.428	176	2053097	37.241	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.563	200	317347	28.763	ng/ul	0.00
73) Anthracene-d10	17.292	188	3458926	37.882	ng/ul	0.00
81) Pyrene-d10	19.533	212	3896479	41.591	ng/ul	0.00
92) Benzo(a)pyrene-d12	23.510	264	3149351	39.188	ng/ul	0.00
Target Compounds						
34) Caprolactam	11.557	113	17535m	2.504	ng/ul	Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP110222\
Data File : BP012520.D
Acq On : 04 Nov 2022 09:17
Operator : CG/JU
Sample : N5353-08
Misc :
ALS Vial : 77 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DBWR2

Manual IntegrationsAPPROVED

Reviewed By :Yogesh Patel 11/05/2022
Supervised By :mohammad ahmed 11/06/2022

Quant Time: Nov 05 03:26:32 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP102522.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri Nov 04 02:53:36 2022
Response via : Initial Calibration

