

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP110222\
 Data File : BP012495.D
 Acq On : 03 Nov 2022 18:23
 Operator : CG/JU
 Sample : N5319-11
 Misc :
 ALS Vial : 51 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 BHAA6

Quant Time: Nov 03 23:05:36 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP102522.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu Nov 03 00:09:04 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc Units	Dev(Min)


Internal Standards					
1) 1,4-Dichlorobenzene-d4	7.781	152	228176	20.000 ng/u1	0.00
20) Naphthalene-d8	10.581	136	1089489	20.000 ng/u1	0.00
38) Acenaphthene-d10	14.434	164	759922	20.000 ng/u1	0.00
64) Phenanthrene-d10	17.198	188	1715406	20.000 ng/u1	0.00
79) Chrysene-d12	21.292	240	1620120	20.000 ng/u1	0.00
88) Perylene-d12	23.674	264	1440328	20.000 ng/u1	0.00
System Monitoring Compounds					
3) 1,4-Dioxane-d8	3.234	96	23165	4.088 ng/uL	0.00
4) Pyridine-d5	3.664	84	116935	7.183 ng/u1	0.00
7) Phenol-d5	6.963	99	138026	6.744 ng/u1	0.00
9) Bis-(2-Chloroethyl)eth...	7.122	67	379786	31.086 ng/u1	0.00
11) 2-Chlorophenol-d4	7.316	132	376922	25.220 ng/u1	0.00
15) 4-Methylphenol-d8	8.505	113	279932	17.294 ng/u1	0.00
21) Nitrobenzene-d5	8.952	128	271187	38.384 ng/u1	0.00
24) 2-Nitrophenol-d4	9.675	143	283613	38.676 ng/u1	0.00
28) 2,4-Dichlorophenol-d3	10.210	165	523261	32.926 ng/u1	0.00
31) 4-Chloroaniline-d4	10.734	131	577778	24.417 ng/u1	0.00
46) Dimethylphthalate-d6	13.851	166	2007322	38.587 ng/u1	0.00
49) Acenaphthylene-d8	14.128	160	2116197	35.597 ng/u1	0.00
54) 4-Nitrophenol-d4	14.681	143	49224	5.000 ng/u1	0.02
60) Fluorene-d10	15.434	176	1711002	38.416 ng/u1	0.00
65) 4,6-Dinitro-2-methylph...	15.569	200	268646	30.080 ng/u1	0.00
73) Anthracene-d10	17.298	188	2896066	39.182 ng/u1	0.00
81) Pyrene-d10	19.539	212	3363507	41.351 ng/u1	0.00
92) Benzo(a)pyrene-d12	23.521	264	2798484	39.765 ng/u1	0.00
Target Compounds					
8) Phenol	6.987	94	22719	1.068 ng/u1#	Qvalue 90


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP110222\
Data File : BP012495.D
Acq On : 03 Nov 2022 18:23
Operator : CG/JU
Sample : N5319-11
Misc :
ALS Vial : 51 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
BHAA6

Quant Time: Nov 03 23:05:36 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP102522.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu Nov 03 00:09:04 2022
Response via : Initial Calibration

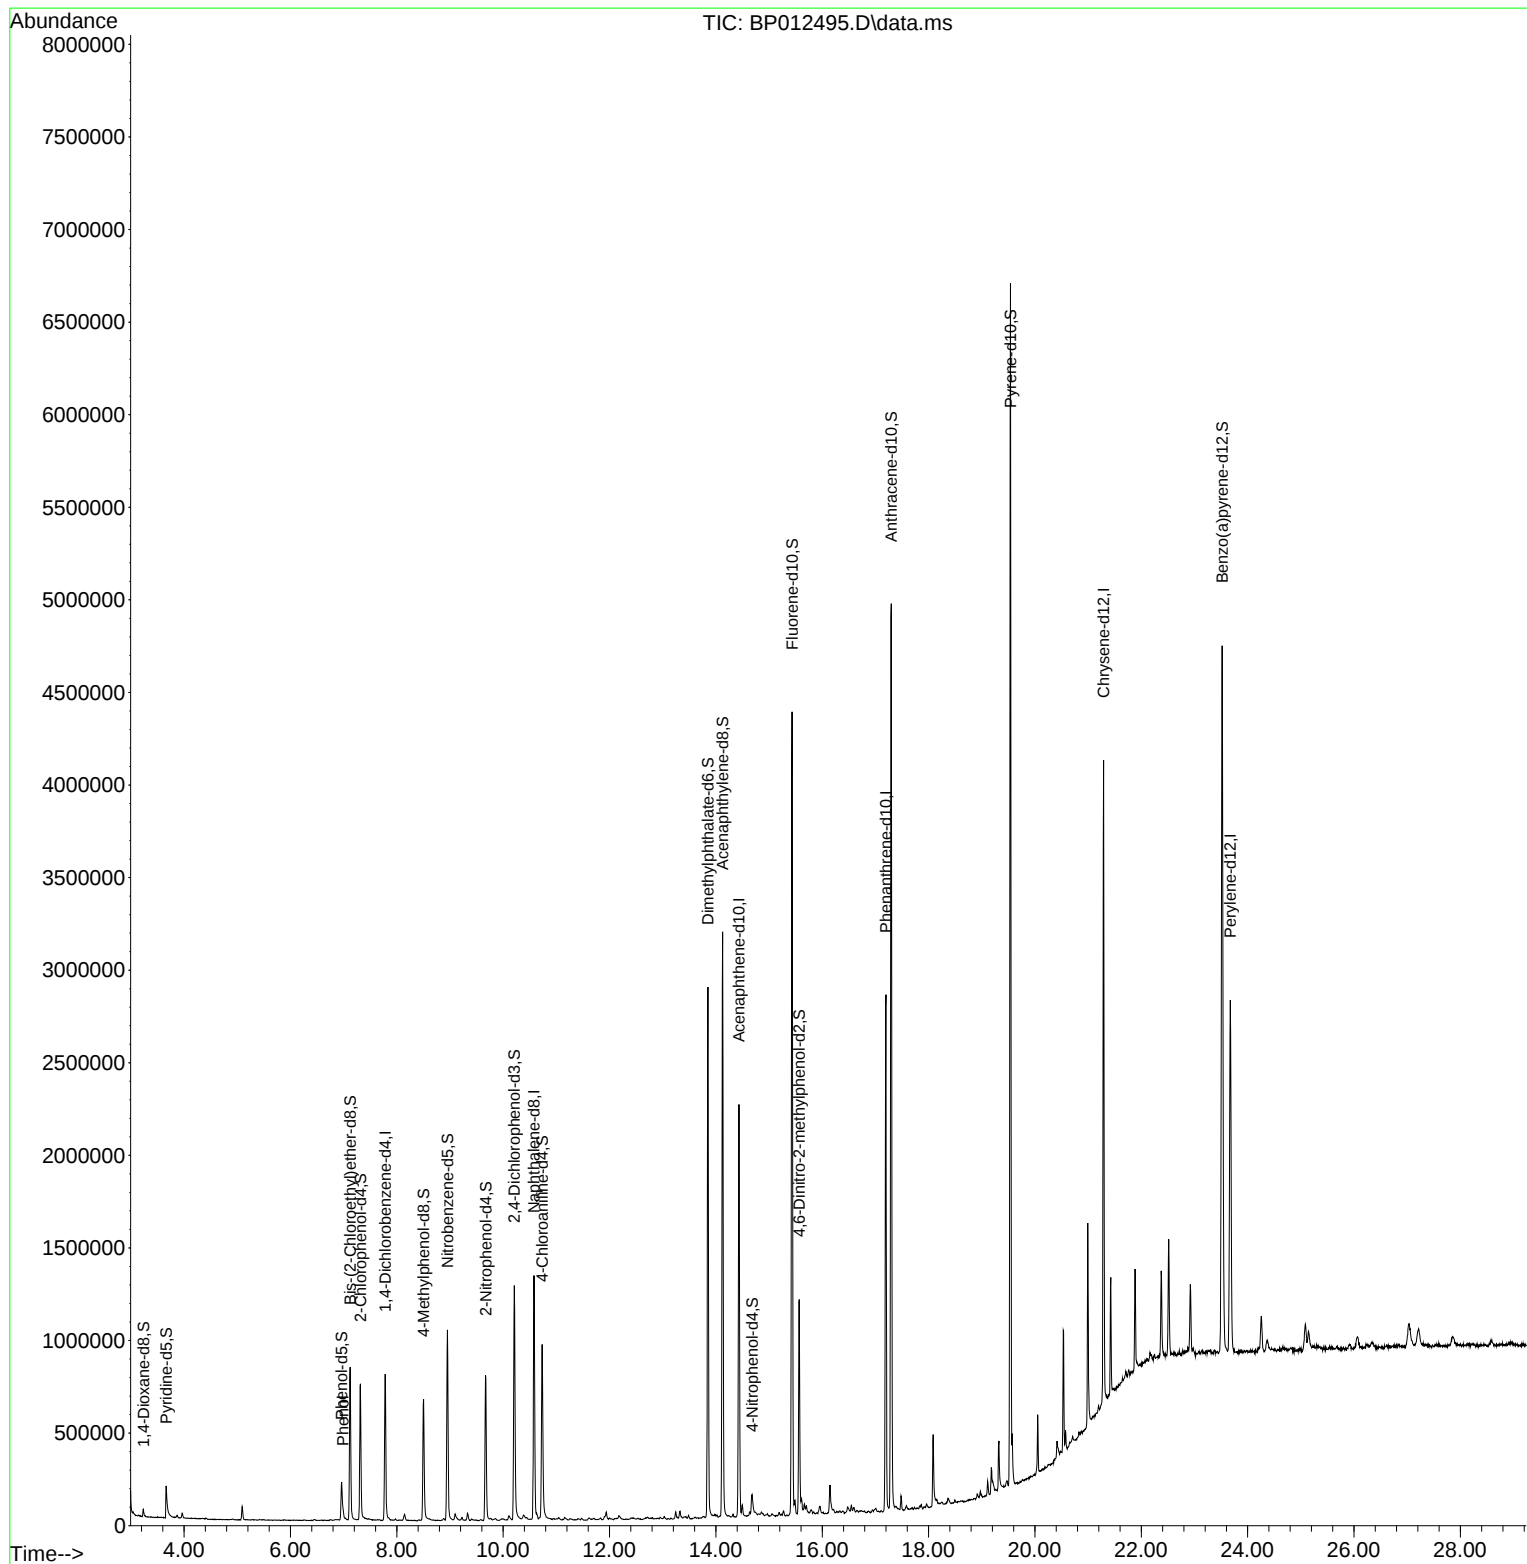

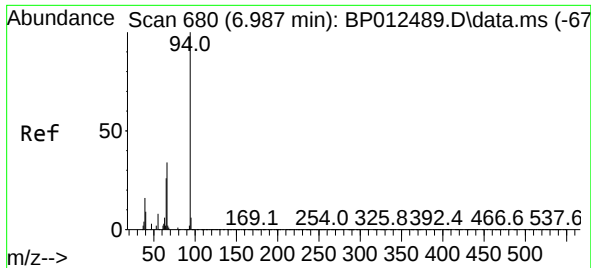

#8

Phenol

Concen: 1.068 ng/ul

RT: 6.987 min Scan# 68

Delta R.T. -0.006 min

Lab File: BP012495.D


Acq: 03 Nov 2022 18:23

Instrument :

BNA_P

ClientSampleId :

BHAA6

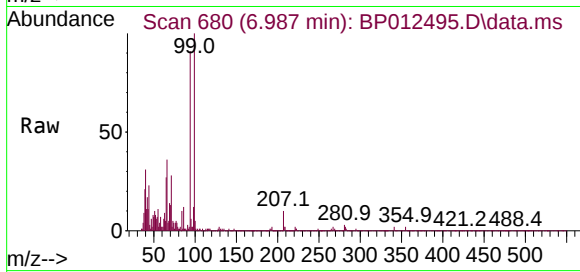

Tgt Ion: 94 Resp: 22719

Ion Ratio Lower Upper

94 100

65 29.9 20.8 31.2

66 39.6 26.2 39.2#

