

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP110222\
 Data File : BP012514.D
 Acq On : 04 Nov 2022 05:52
 Operator : CG/JU
 Sample : N5320-03
 Misc :
 ALS Vial : 71 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 BHAB5

Quant Time: Nov 04 06:33:23 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP102522.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri Nov 04 02:53:36 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.775	152	342673	20.000	ng/u1	0.00
20) Naphthalene-d8	10.575	136	1639003	20.000	ng/u1	0.00
38) Acenaphthene-d10	14.428	164	1127470	20.000	ng/u1	0.00
64) Phenanthrene-d10	17.192	188	2517944	20.000	ng/u1	0.00
79) Chrysene-d12	21.286	240	2237319	20.000	ng/u1	0.00
88) Perylene-d12	23.669	264	1995855	20.000	ng/u1	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.228	96	32664	3.838	ng/uL	0.00
4) Pyridine-d5	3.658	84	235473	9.632	ng/u1	0.00
7) Phenol-d5	6.958	99	196246	6.385	ng/u1	0.00
9) Bis-(2-Chloroethyl)eth...	7.116	67	508785	27.730	ng/u1	0.00
11) 2-Chlorophenol-d4	7.311	132	530228	23.624	ng/u1	0.00
15) 4-Methylphenol-d8	8.493	113	381902	15.711	ng/u1	0.00
21) Nitrobenzene-d5	8.946	128	351148	33.038	ng/u1	0.00
24) 2-Nitrophenol-d4	9.663	143	380279	34.471	ng/u1	0.00
28) 2,4-Dichlorophenol-d3	10.205	165	685336	28.666	ng/u1	0.00
31) 4-Chloroaniline-d4	10.728	131	904860	25.419	ng/u1	0.00
46) Dimethylphthalate-d6	13.845	166	2405703	31.169	ng/u1	0.00
49) Acenaphthylene-d8	14.122	160	2570213	29.140	ng/u1	0.00
54) 4-Nitrophenol-d4	14.675	143	63170	4.325	ng/u1	0.02
60) Fluorene-d10	15.428	176	2039317	30.861	ng/u1	0.00
65) 4,6-Dinitro-2-methylph...	15.563	200	339430	25.892	ng/u1	0.00
73) Anthracene-d10	17.292	188	3477333	32.051	ng/u1	0.00
81) Pyrene-d10	19.533	212	3995215	35.567	ng/u1	0.00
92) Benzo(a)pyrene-d12	23.516	264	3224488	33.065	ng/u1	0.00
Target Compounds						
67) N-Nitrosodiphenylamine	15.698	169	89661	1.264	ng/u1	Qvalue 97


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP110222\
Data File : BP012514.D
Acq On : 04 Nov 2022 05:52
Operator : CG/JU
Sample : N5320-03
Misc :
ALS Vial : 71 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
BHAB5

Quant Time: Nov 04 06:33:23 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP102522.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri Nov 04 02:53:36 2022
Response via : Initial Calibration

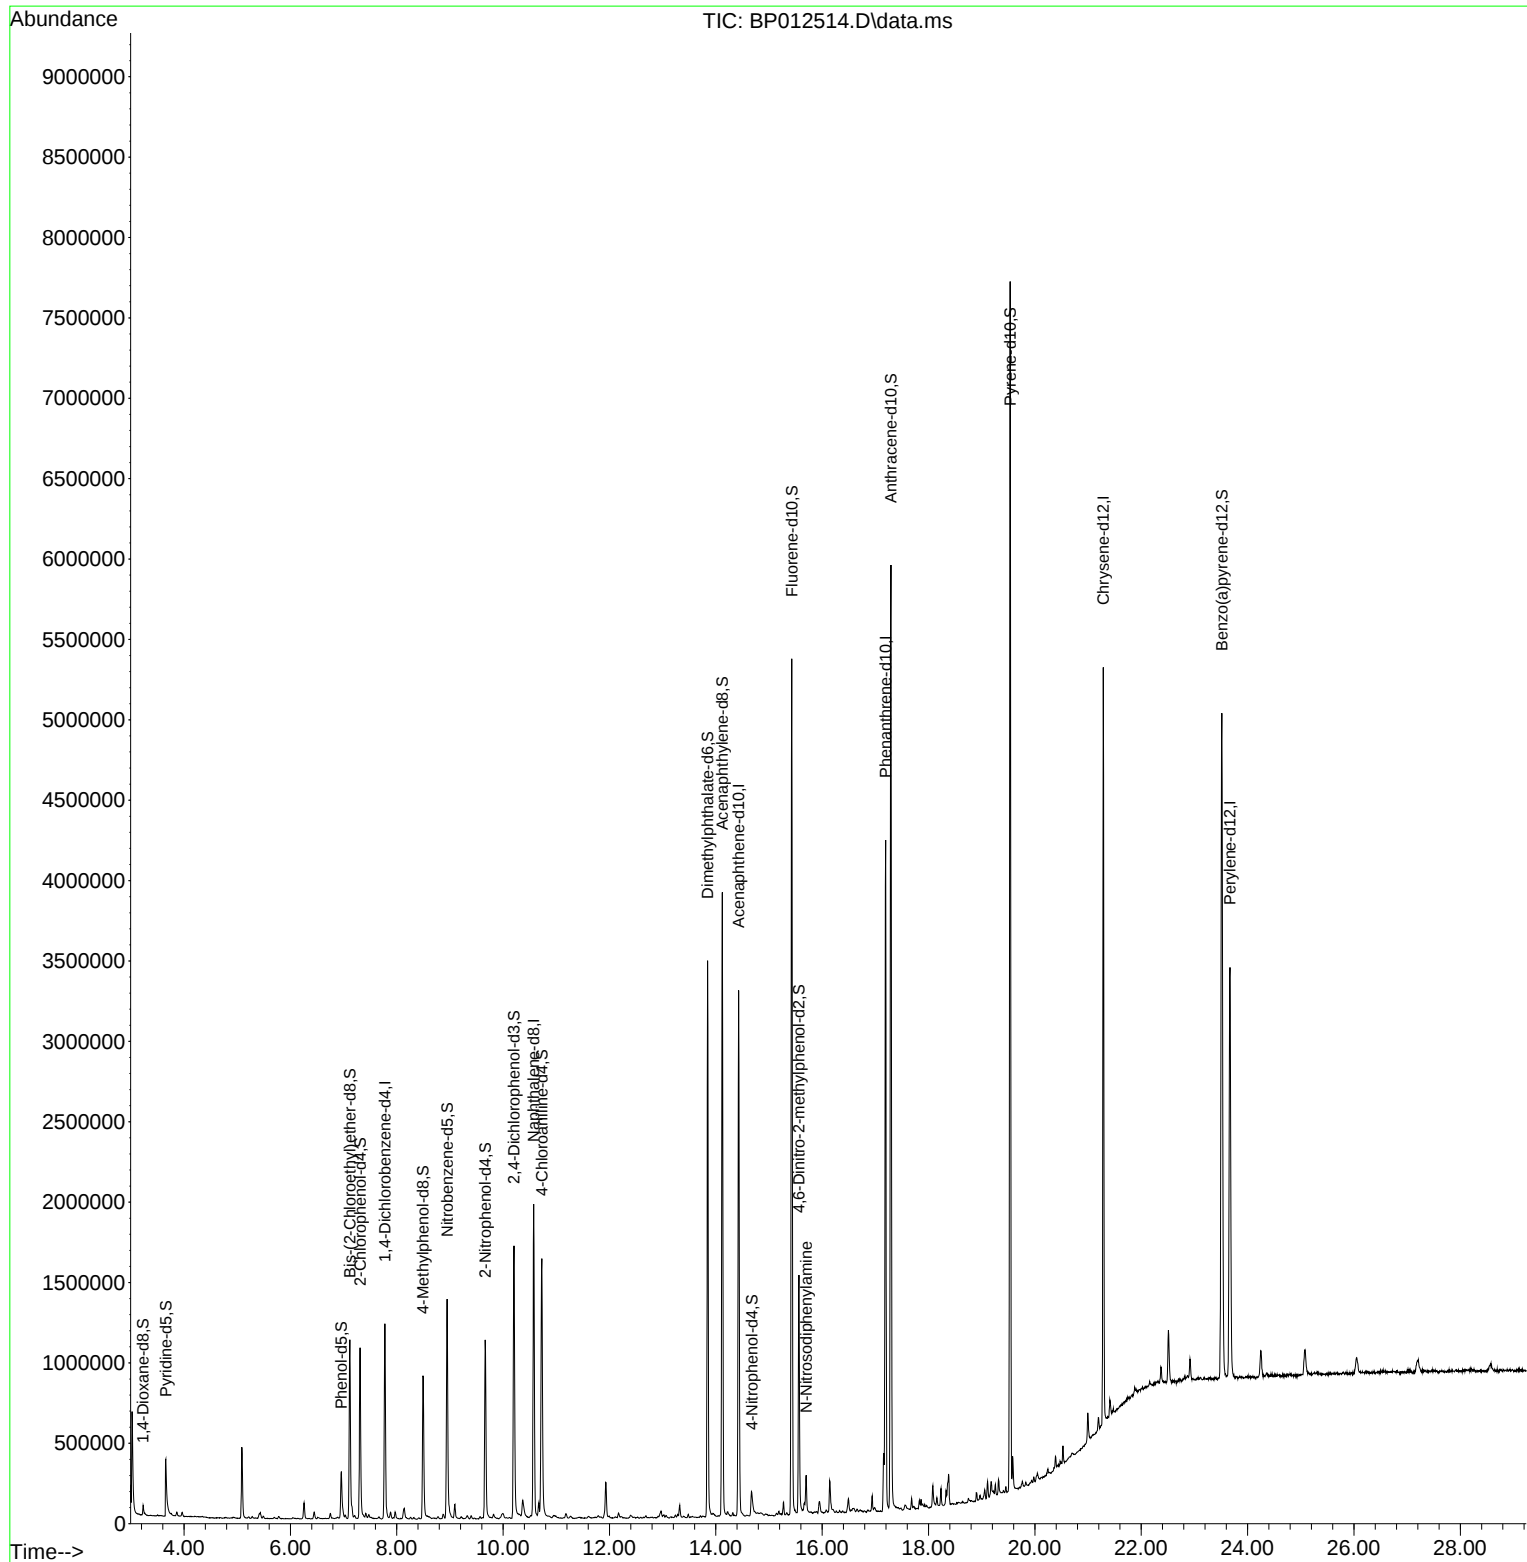

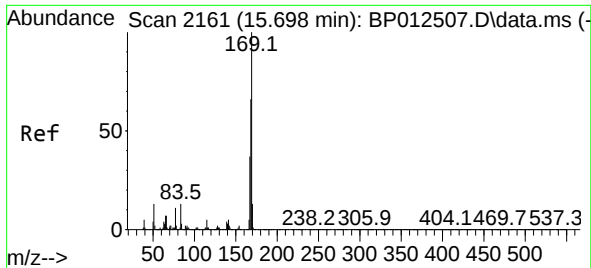

#67
 N-Nitrosodiphenylamine
 Concen: 1.264 ng/ul
 RT: 15.698 min Scan# 2161
 Delta R.T. 0.000 min
 Lab File: BP012514.D
 Acq: 04 Nov 2022 05:52

Instrument :
 BNA_P
 ClientSampleId :
 BHAB5

Tgt Ion:169 Resp: 89661
 Ion Ratio Lower Upper
 169 100
 168 67.9 52.9 79.3
 167 39.1 29.1 43.7

