

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP110222\
 Data File : BP012448.D
 Acq On : 02 Nov 2022 11:53
 Operator : CG/JU
 Sample : PB148675BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SBLK675

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP102522.M
 Title : SVOA CALIBRATION

Signal : TIC: BP012448.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.234	39	42	50	rVB	79374	109756	1.33%	0.142%
2	3.670	115	116	137	rBV	102654	221286	2.67%	0.286%
3	3.970	163	167	174	rVB	20624	31764	0.38%	0.041%
4	6.963	669	676	691	rBV	1167056	1946477	23.50%	2.518%
5	7.128	698	704	719	rBV	1028908	1622786	19.60%	2.100%
6	7.322	730	737	750	rBV	1200701	1954797	23.61%	2.529%
7	7.787	809	816	828	rBV	943612	1571970	18.98%	2.034%
8	8.505	929	938	957	rBV	1435850	2570441	31.04%	3.326%
9	8.957	1008	1015	1030	rBV	1162279	1987107	24.00%	2.571%
10	9.681	1129	1138	1152	rBV	1004754	1711427	20.67%	2.214%
11	10.216	1221	1229	1254	rBV	1393789	2664084	32.17%	3.447%
12	10.593	1284	1293	1308	rBV	1460017	2498072	30.17%	3.232%
13	12.198	1560	1566	1574	rBV2	18143	42521	0.51%	0.055%
14	13.416	1767	1773	1780	rBV7	5634	10613	0.13%	0.014%
15	13.857	1838	1848	1859	rBV	2961255	4261786	51.46%	5.514%
16	14.134	1887	1895	1911	rBV2	3368266	5086336	61.42%	6.581%
17	14.440	1940	1947	1965	rBV	2347975	3678322	44.42%	4.759%
18	14.663	1979	1985	2015	rBV	926090	1943433	23.47%	2.514%
19	14.851	2015	2017	2021	rVB5	7640	9935	0.12%	0.013%
20	15.439	2110	2117	2134	rBV	4593055	6586542	79.54%	8.521%
21	15.575	2134	2140	2154	rVV	894942	1325567	16.01%	1.715%
22	15.681	2154	2158	2166	rVB2	26875	47284	0.57%	0.061%
23	15.951	2199	2204	2209	rBV7	7684	10911	0.13%	0.014%
24	16.228	2249	2251	2257	rVB7	7356	8472	0.10%	0.011%
25	16.881	2359	2362	2366	rVB5	6495	8581	0.10%	0.011%
26	17.204	2410	2417	2427	rBV	3155485	4605124	55.61%	5.958%
27	17.304	2427	2434	2452	rVV	5012306	7287134	88.00%	9.428%
28	19.122	2739	2743	2750	rBV3	66940	96951	1.17%	0.125%
29	19.192	2751	2755	2761	rVV	58143	88279	1.07%	0.114%
30	19.545	2809	2815	2825	rBV	6197104	8281179	100.00%	10.714%
31	21.298	3108	3113	3122	rBV	3400460	4490379	54.22%	5.810%
32	23.533	3486	3493	3506	rVB2	3301763	6656239	80.38%	8.612%
33	23.686	3513	3519	3531	rVB2	1954281	3878005	46.83%	5.017%




Sum of corrected areas: 77293560

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP110222\
Data File : BP012448.D
Acq On : 02 Nov 2022 11:53
Operator : CG/JU
Sample : PB148675BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK675

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP102522.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

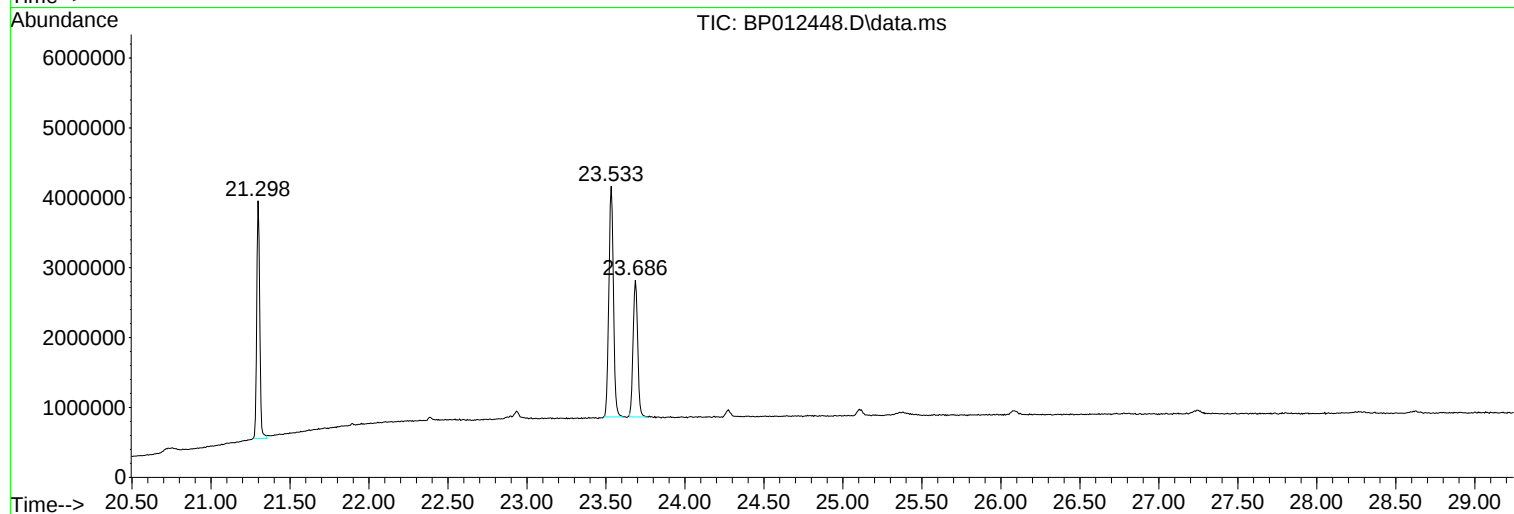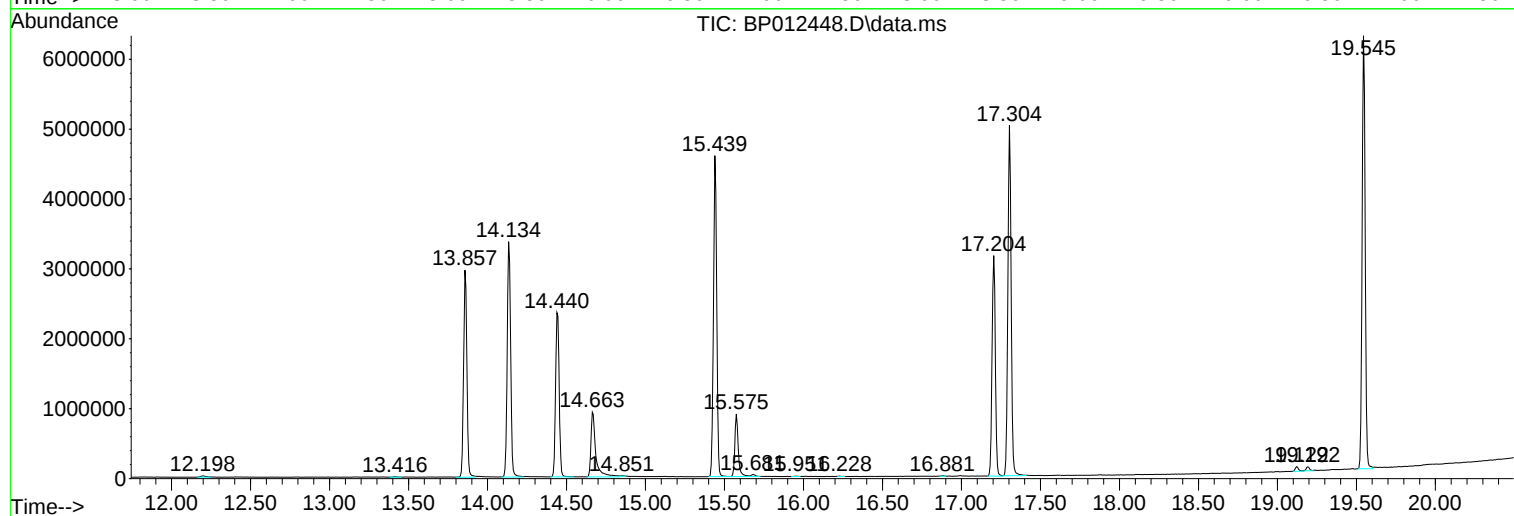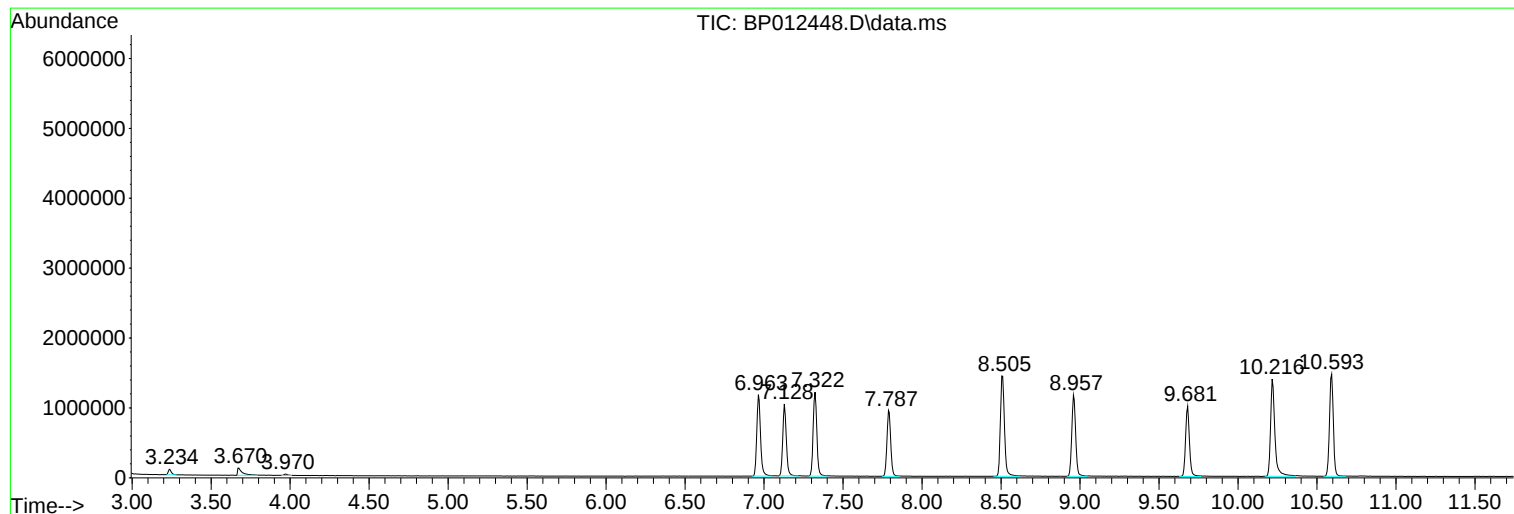

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP110222\
Data File : BP012448.D
Acq On : 02 Nov 2022 11:53
Operator : CG/JU
Sample : PB148675BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK675

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP102522.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP110222\
Data File : BP012448.D
Acq On : 02 Nov 2022 11:53
Operator : CG/JU
Sample : PB148675BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK675

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP102522.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST0.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc