

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP110222\
 Data File : BP012450.D
 Acq On : 02 Nov 2022 13:01
 Operator : CG/JU
 Sample : N5180-02
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 C0KX2

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP102522.M
 Title : SVOA CALIBRATION

Signal : TIC: BP012450.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.234	39	42	53	rVB	43849	63293	0.63%	0.081%
2	3.664	112	115	137	rBV	198762	395012	3.90%	0.505%
3	3.875	146	151	158	rVB	29849	49768	0.49%	0.064%
4	3.970	163	167	175	rVB	19400	30388	0.30%	0.039%
5	4.887	317	323	329	rBV7	6784	11855	0.12%	0.015%
6	5.099	354	359	368	rVB	18958	31095	0.31%	0.040%
7	6.964	669	676	691	rBV	218808	419909	4.15%	0.537%
8	7.128	697	704	718	rBV	979159	1632638	16.13%	2.087%
9	7.322	730	737	747	rBV	354717	599090	5.92%	0.766%
10	7.787	809	816	827	rBV	974508	1612872	15.94%	2.062%
11	8.140	871	876	880	rVB4	9685	14691	0.15%	0.019%
12	8.505	932	938	953	rBV	469952	873145	8.63%	1.116%
13	8.958	1007	1015	1029	rBV	1187804	2031713	20.08%	2.598%
14	9.340	1074	1080	1086	rVB	29459	45182	0.45%	0.058%
15	9.681	1131	1138	1148	rBV	192033	348474	3.44%	0.446%
16	10.216	1220	1229	1249	rBV	476869	948435	9.37%	1.213%
17	10.446	1262	1268	1275	rVB	6268	12301	0.12%	0.016%
18	10.587	1284	1292	1308	rBV	1481008	2530828	25.01%	3.236%
19	10.740	1310	1318	1338	rBV	1061697	1964911	19.42%	2.512%
20	11.422	1428	1434	1436	rBV6	6934	10593	0.10%	0.014%
21	11.834	1498	1504	1512	rVB2	22513	38239	0.38%	0.049%
22	12.016	1529	1535	1542	rBV2	12316	29093	0.29%	0.037%
23	12.193	1559	1565	1574	rBV	18291	35349	0.35%	0.045%
24	13.251	1738	1745	1749	rBV5	10847	17464	0.17%	0.022%
25	13.404	1767	1771	1778	rVB6	6612	12575	0.12%	0.016%
26	13.769	1827	1833	1839	rBV2	32181	55612	0.55%	0.071%
27	13.857	1839	1848	1861	rBV	3285832	4696445	46.41%	6.004%
28	14.134	1887	1895	1914	rBV	3536346	5452402	53.88%	6.971%
29	14.328	1923	1928	1934	rVB7	9098	16001	0.16%	0.020%
30	14.440	1940	1947	1965	rVB	2504040	3758470	37.14%	4.805%
31	14.693	1982	1990	2001	rBV5	35482	122481	1.21%	0.157%
32	15.193	2071	2075	2079	rBV	24063	34304	0.34%	0.044%
33	15.234	2079	2082	2086	rVV	36589	48417	0.48%	0.062%
34	15.281	2086	2090	2095	rVB4	12182	18911	0.19%	0.024%
35	15.440	2107	2117	2123	rBV	4894975	7293728	72.08%	9.325%
36	15.498	2123	2127	2139	rVV	98329	200999	1.99%	0.257%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP110222\
 Data File : BP012450.D
 Acq On : 02 Nov 2022 13:01
 Operator : CG/JU
 Sample : N5180-02
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 C0KX2

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF Filtering: 5
 Sampling : 1 Min Area: 0.1 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP102522.M
 Title : SVOA CALIBRATION

37	15.593	2139	2143	2153	rVV	10558	26999	0.27%	0.035%
38	15.681	2153	2158	2164	rVB3	26235	44403	0.44%	0.057%
39	16.151	2234	2238	2245	rVB3	11567	21326	0.21%	0.027%
40	16.222	2247	2250	2254	rBV6	8075	11340	0.11%	0.014%
41	16.875	2359	2361	2366	rVB5	8683	11320	0.11%	0.014%
42	16.951	2370	2374	2377	rBV4	11530	15262	0.15%	0.020%
43	17.198	2410	2416	2427	rVV	3230114	4730569	46.75%	6.048%
44	17.304	2427	2434	2453	rVV2	5669234	8766181	86.63%	11.207%
45	17.869	2528	2530	2535	rVB5	9267	11739	0.12%	0.015%
46	19.116	2739	2742	2748	rBV2	80436	109708	1.08%	0.140%
47	19.186	2751	2754	2760	rVV	56697	81590	0.81%	0.104%
48	19.545	2809	2815	2828	rBV	7598858	10118979	100.00%	12.937%
49	19.804	2855	2859	2866	rBV2	44615	105951	1.05%	0.135%
50	20.998	3059	3062	3071	rBV3	184143	322249	3.18%	0.412%
51	21.298	3108	3113	3120	rBV	3830786	4996299	49.38%	6.388%
52	23.533	3486	3493	3504	rVB2	4442924	8910939	88.06%	11.393%
53	23.686	3512	3519	3529	rVB2	2201420	4475587	44.23%	5.722%




Sum of corrected areas: 78217124

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP110222\
Data File : BP012450.D
Acq On : 02 Nov 2022 13:01
Operator : CG/JU
Sample : N5180-02
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0KX2

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP102522.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

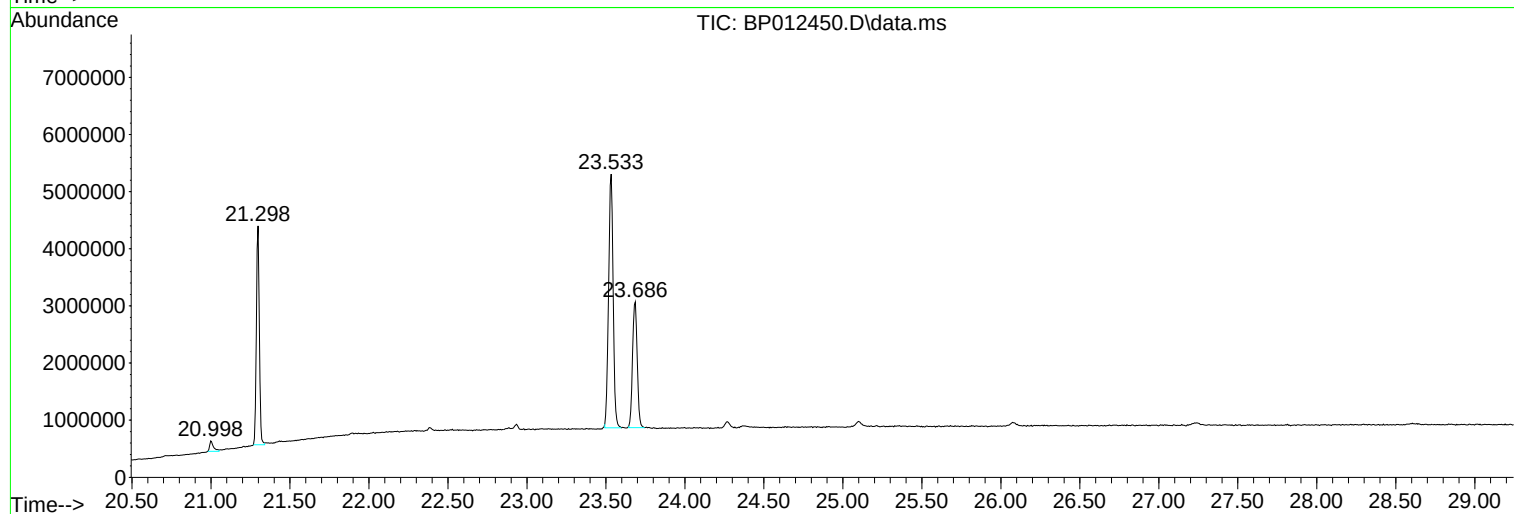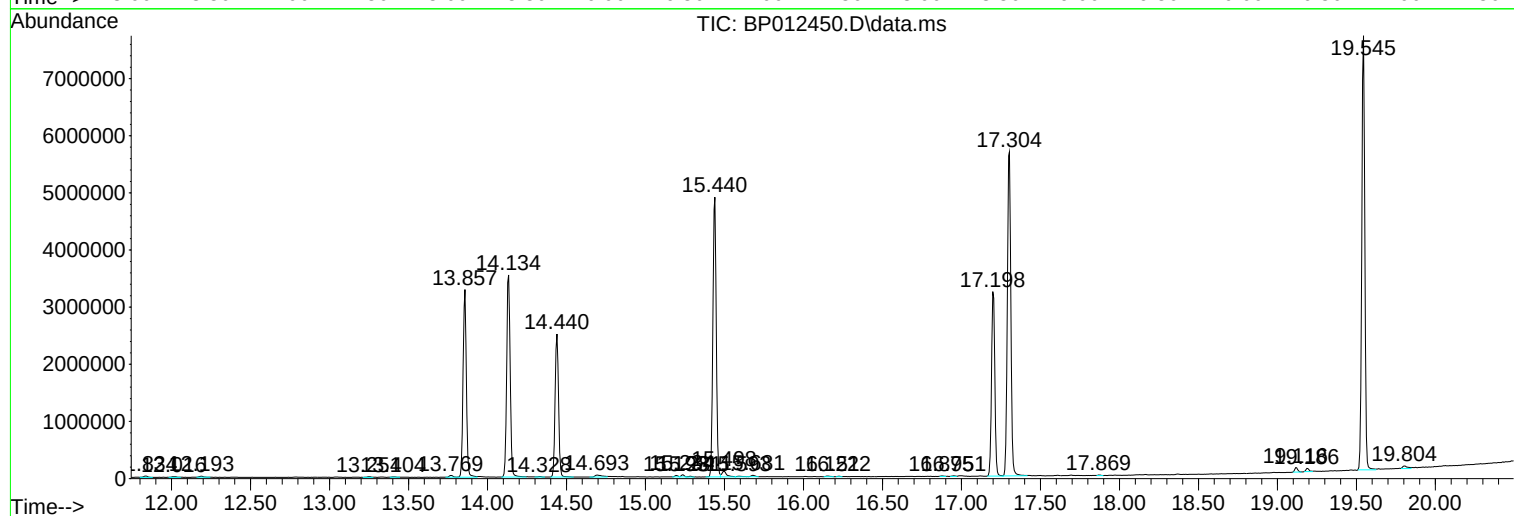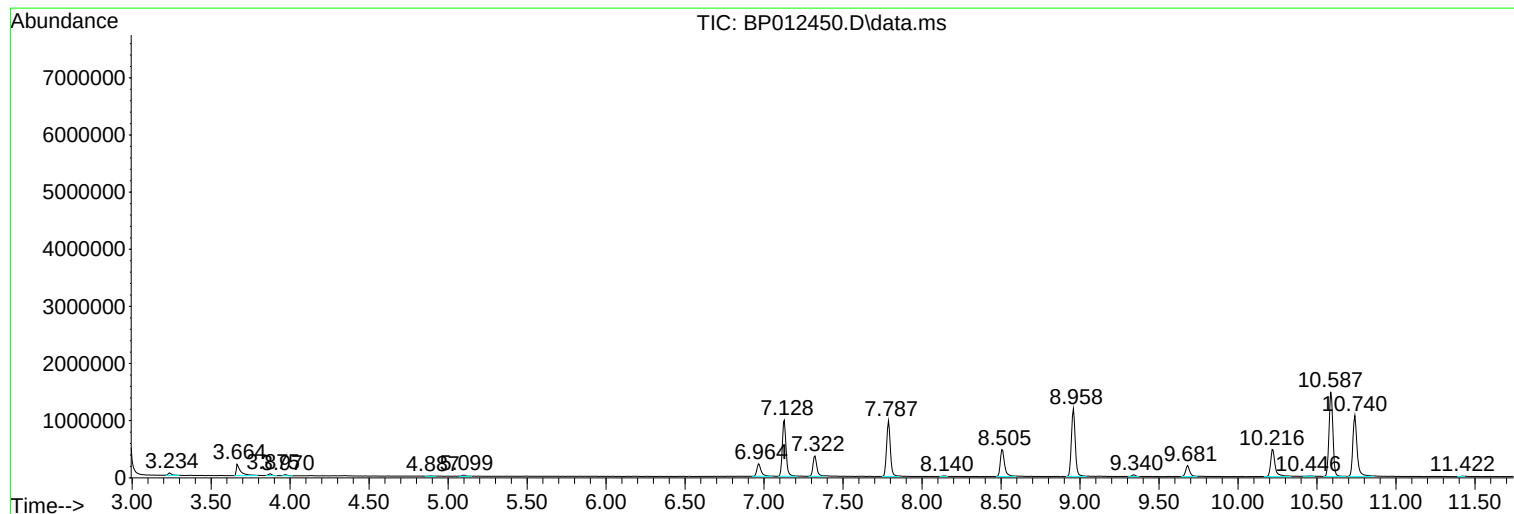

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP110222\
Data File : BP012450.D
Acq On : 02 Nov 2022 13:01
Operator : CG/JU
Sample : N5180-02
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0KX2

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP102522.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP110222\
Data File : BP012450.D
Acq On : 02 Nov 2022 13:01
Operator : CG/JU
Sample : N5180-02
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0KX2

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP102522.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc