

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP110222\
 Data File : BP012451.D
 Acq On : 02 Nov 2022 13:37
 Operator : CG/JU
 Sample : N5180-03
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 C0KX3

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP102522.M
 Title : SVOA CALIBRATION

Signal : TIC: BP012451.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.234	39	42	53	rVB	57614	83417	0.80%	0.105%
2	3.664	113	115	132	rBV	221258	414704	4.00%	0.522%
3	3.875	145	151	158	rVB	37435	62006	0.60%	0.078%
4	3.969	163	167	174	rVB	18499	27843	0.27%	0.035%
5	4.346	228	231	236	rVB6	7217	11134	0.11%	0.014%
6	4.887	320	323	331	rVB2	7670	13843	0.13%	0.017%
7	6.963	670	676	688	rBV	338743	598297	5.77%	0.753%
8	7.128	697	704	718	rBV	1070547	1739685	16.78%	2.188%
9	7.322	730	737	746	rBV	665833	1118694	10.79%	1.407%
10	7.787	809	816	827	rBV	916075	1485640	14.33%	1.869%
11	8.504	931	938	953	rBV	782669	1381132	13.33%	1.737%
12	8.957	1007	1015	1030	rBV	1267381	2147340	20.72%	2.701%
13	9.122	1038	1043	1054	rVB5	16571	35940	0.35%	0.045%
14	9.340	1074	1080	1089	rVB	35253	57041	0.55%	0.072%
15	9.681	1130	1138	1148	rBV	161380	299109	2.89%	0.376%
16	9.763	1150	1152	1159	rVB8	6795	12572	0.12%	0.016%
17	10.216	1221	1229	1250	rBV	837873	1545273	14.91%	1.944%
18	10.587	1284	1292	1305	rBV	1356138	2370150	22.87%	2.981%
19	10.740	1310	1318	1340	rBV	1264952	2355384	22.72%	2.963%
20	11.422	1428	1434	1441	rBV7	13405	29999	0.29%	0.038%
21	11.840	1497	1505	1513	rBV	35187	57780	0.56%	0.073%
22	12.016	1530	1535	1541	rBV9	5591	11226	0.11%	0.014%
23	12.193	1558	1565	1574	rBV2	19547	41717	0.40%	0.052%
24	12.792	1661	1667	1673	rBV6	7878	14392	0.14%	0.018%
25	13.045	1705	1710	1715	rBV2	9915	16606	0.16%	0.021%
26	13.334	1755	1759	1764	rVB8	5998	10658	0.10%	0.013%
27	13.410	1767	1772	1782	rVB7	8699	16875	0.16%	0.021%
28	13.857	1840	1848	1854	rBV	3355511	4581159	44.20%	5.762%
29	13.898	1854	1855	1864	rVB	75735	99309	0.96%	0.125%
30	14.134	1884	1895	1914	rBV2	3649302	5604978	54.08%	7.050%
31	14.439	1940	1947	1964	rBV	2362370	3515482	33.92%	4.422%
32	14.686	1983	1989	2007	rBV	60310	220665	2.13%	0.278%
33	14.857	2014	2018	2023	rVB5	7050	10491	0.10%	0.013%
34	15.198	2072	2076	2079	rBV	7815	12513	0.12%	0.016%
35	15.239	2079	2083	2086	rVV	29500	39370	0.38%	0.050%
36	15.275	2086	2089	2097	rVB3	10630	20137	0.19%	0.025%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP110222\
 Data File : BP012451.D
 Acq On : 02 Nov 2022 13:37
 Operator : CG/JU
 Sample : N5180-03
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 C0KX3

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP102522.M
 Title : SVOA CALIBRATION

37	15.439	2110	2117	2125	rBV	4965526	7428875	71.67%	9.344%
38	15.498	2125	2127	2136	rVV4	36283	57398	0.55%	0.072%
39	15.586	2139	2142	2150	rVB8	9469	15103	0.15%	0.019%
40	15.681	2154	2158	2163	rBV4	21962	36597	0.35%	0.046%
41	16.157	2234	2239	2244	rBV8	9105	19408	0.19%	0.024%
42	16.228	2247	2251	2257	rVB9	9075	15694	0.15%	0.020%
43	16.345	2264	2271	2276	rBV10	7450	17603	0.17%	0.022%
44	16.663	2321	2325	2333	rBV10	5978	13225	0.13%	0.017%
45	17.204	2410	2417	2427	rBV	3096331	4419229	42.64%	5.558%
46	17.304	2427	2434	2446	rBV	6243861	8981537	86.65%	11.297%
47	17.428	2453	2455	2460	rVB	11155	15428	0.15%	0.019%
48	17.498	2462	2467	2470	rBV7	9680	15113	0.15%	0.019%
49	17.875	2527	2531	2535	rBV	43597	55305	0.53%	0.070%
50	19.010	2721	2724	2728	rVB6	24284	28805	0.28%	0.036%
51	19.122	2739	2743	2750	rBV3	81408	128112	1.24%	0.161%
52	19.192	2751	2755	2758	rBV	57366	78491	0.76%	0.099%
53	19.545	2809	2815	2828	rBV	7849257	10364839	100.00%	13.037%
54	21.004	3059	3063	3074	rBV4	204161	402825	3.89%	0.507%
55	21.298	3108	3113	3123	rBV	3653791	4612369	44.50%	5.801%
56	23.533	3486	3493	3505	rVB2	4409673	8788214	84.79%	11.054%
57	23.686	3513	3519	3528	rVB2	2015462	3947543	38.09%	4.965%




Sum of corrected areas: 79504274

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP110222\
Data File : BP012451.D
Acq On : 02 Nov 2022 13:37
Operator : CG/JU
Sample : N5180-03
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0KX3

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP102522.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

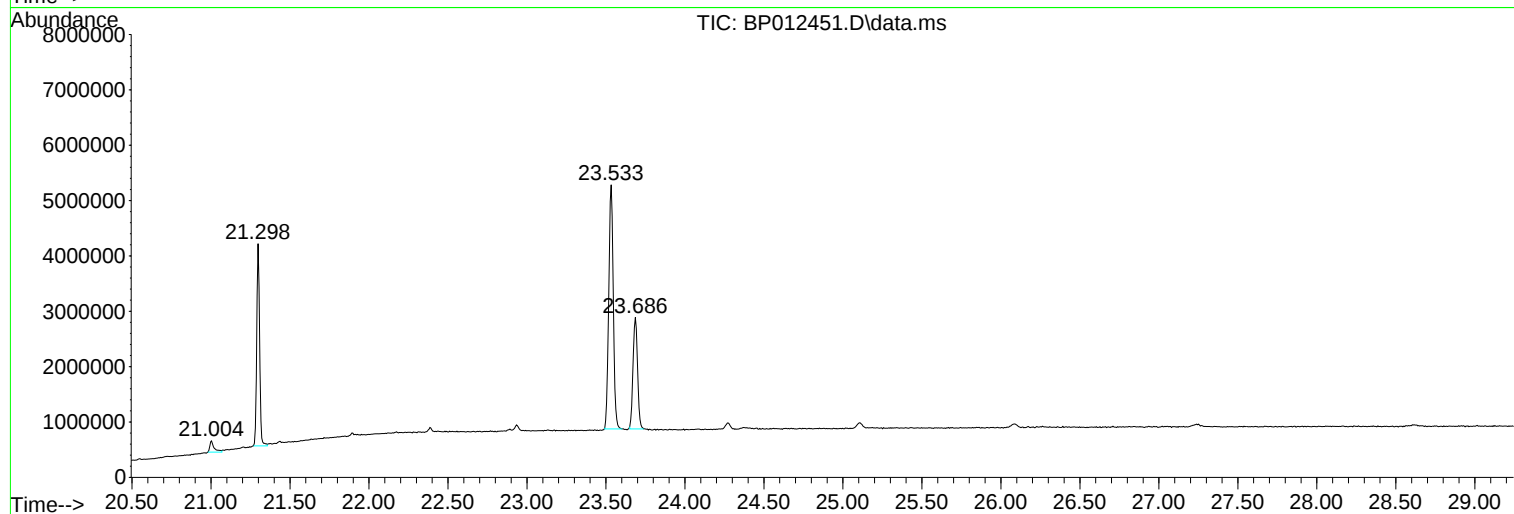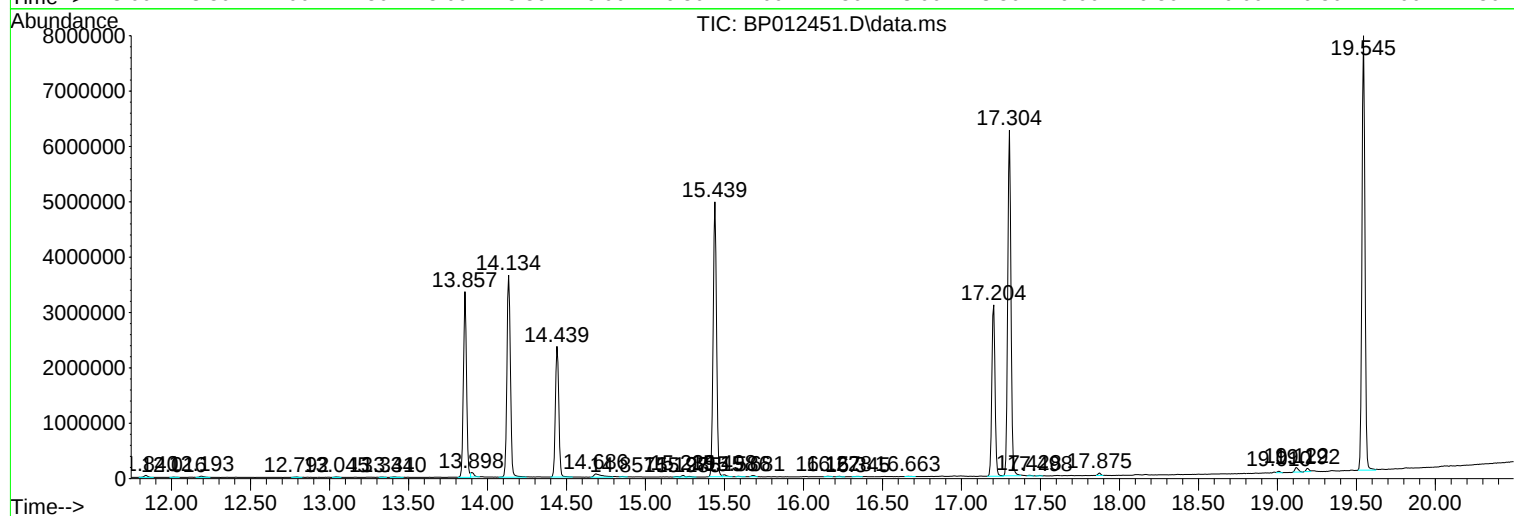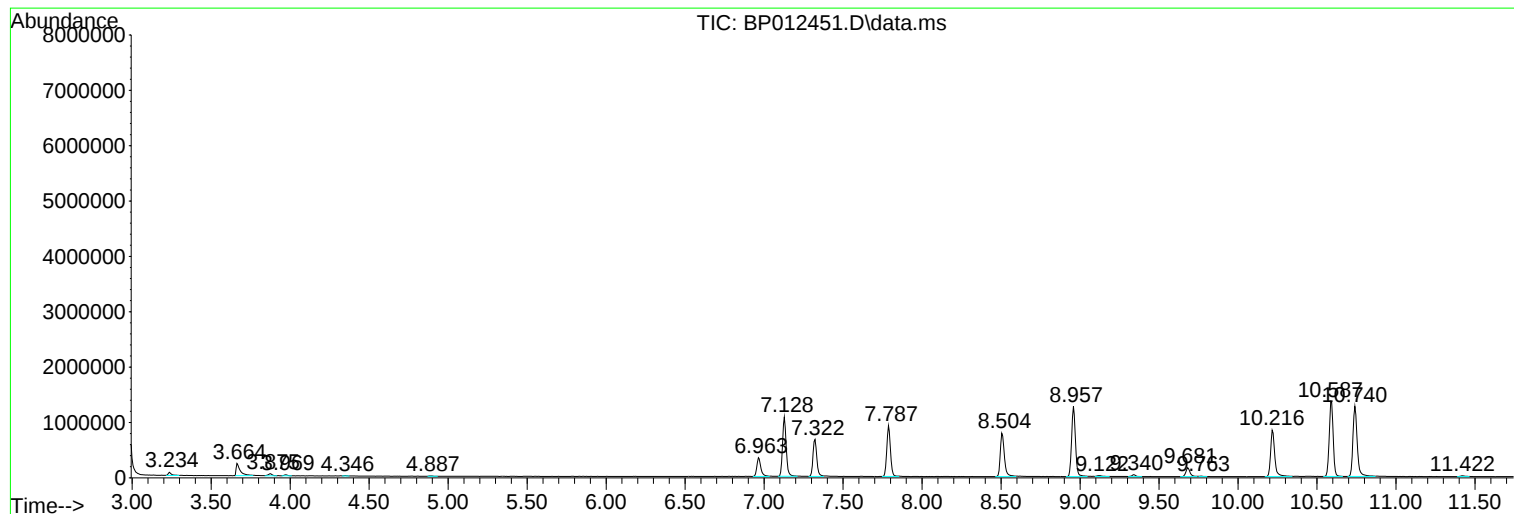

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP110222\
Data File : BP012451.D
Acq On : 02 Nov 2022 13:37
Operator : CG/JU
Sample : N5180-03
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0KX3

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP102522.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP110222\
Data File : BP012451.D
Acq On : 02 Nov 2022 13:37
Operator : CG/JU
Sample : N5180-03
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0KX3

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP102522.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc