

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP110222\
 Data File : BP012455.D
 Acq On : 02 Nov 2022 15:56
 Operator : CG/JU
 Sample : N5321-09
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DBWR5

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP102522.M
 Title : SVOA CALIBRATION

Signal : TIC: BP012455.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.199	31	36	40	rBV	164805	245532	1.87%	0.224%
2	3.234	40	42	47	rVB	65771	79607	0.61%	0.073%
3	3.664	112	115	138	rBV	349510	614382	4.67%	0.560%
4	3.869	146	150	156	rVB2	18464	30782	0.23%	0.028%
5	3.975	163	168	172	rVB	19963	28508	0.22%	0.026%
6	4.916	324	328	333	rVB3	9569	13361	0.10%	0.012%
7	6.963	670	676	690	rBV	358426	628441	4.78%	0.573%
8	7.128	697	704	728	rBV	1204802	1969138	14.97%	1.795%
9	7.316	730	736	753	rBV	1154449	1907579	14.50%	1.739%
10	7.787	808	816	825	rBV	1171766	1855290	14.10%	1.691%
11	7.887	827	833	842	rVB2	94852	169143	1.29%	0.154%
12	8.504	931	938	952	rBV	1105426	1868512	14.20%	1.703%
13	8.716	969	974	980	rVB5	6882	15426	0.12%	0.014%
14	8.957	1007	1015	1028	rBV	1461713	2444610	18.58%	2.228%
15	9.334	1075	1079	1085	rBV2	18535	28525	0.22%	0.026%
16	9.563	1114	1118	1125	rBV4	15575	29211	0.22%	0.027%
17	9.675	1130	1137	1154	rBV	1141520	1976479	15.02%	1.801%
18	10.122	1208	1213	1221	rBV	12922	27518	0.21%	0.025%
19	10.216	1221	1229	1252	rBV	1844575	3307331	25.14%	3.014%
20	10.587	1284	1292	1306	rBV	1793066	3025567	23.00%	2.757%
21	10.740	1308	1318	1334	rBV	1400118	2620401	19.92%	2.388%
22	11.151	1382	1388	1396	rVB9	10945	21122	0.16%	0.019%
23	11.581	1456	1461	1470	rBV	14650	27117	0.21%	0.025%
24	11.840	1500	1505	1510	rBV8	8381	17213	0.13%	0.016%
25	12.093	1542	1548	1559	rBV3	41582	89428	0.68%	0.082%
26	12.181	1559	1563	1569	rVB2	24625	42126	0.32%	0.038%
27	12.316	1580	1586	1595	rVB10	12382	29145	0.22%	0.027%
28	12.416	1595	1603	1610	rBV10	10121	28280	0.21%	0.026%
29	12.487	1610	1615	1619	rBV2	15432	23154	0.18%	0.021%
30	12.787	1659	1666	1671	rBV2	8393	17946	0.14%	0.016%
31	13.016	1700	1705	1708	rBV3	14041	22415	0.17%	0.020%
32	13.116	1717	1722	1726	rBV3	12618	21466	0.16%	0.020%
33	13.169	1726	1731	1736	rVB2	44719	68606	0.52%	0.063%
34	13.251	1741	1745	1754	rVV4	17903	34834	0.26%	0.032%
35	13.334	1754	1759	1767	rVB7	16275	30166	0.23%	0.027%
36	13.422	1767	1774	1778	rBV8	13863	30355	0.23%	0.028%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP110222\
 Data File : BP012455.D
 Acq On : 02 Nov 2022 15:56
 Operator : CG/JU
 Sample : N5321-09
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DBWR5

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP102522.M
 Title : SVOA CALIBRATION

37	13.592	1798	1803	1807	rBV2	18653	26130	0.20%	0.024%
38	13.645	1807	1812	1822	rVV2	39667	79492	0.60%	0.072%
39	13.857	1841	1848	1854	rBV	4037305	5610876	42.65%	5.114%
40	13.992	1869	1871	1875	rVB2	12069	14262	0.11%	0.013%
41	14.045	1875	1880	1884	rBV4	16506	28165	0.21%	0.026%
42	14.134	1888	1895	1907	rVV	4421364	6615322	50.28%	6.029%
43	14.234	1907	1912	1921	rVB3	71056	119989	0.91%	0.109%
44	14.339	1928	1930	1939	rVB7	17178	28489	0.22%	0.026%
45	14.439	1940	1947	1960	rVB	2972238	4386538	33.34%	3.998%
46	14.675	1981	1987	1998	rBV	227436	547558	4.16%	0.499%
47	14.786	2002	2006	2008	rBV5	12452	19688	0.15%	0.018%
48	14.828	2010	2013	2015	rVV2	13610	17656	0.13%	0.016%
49	15.063	2051	2053	2063	rVB7	17240	26050	0.20%	0.024%
50	15.234	2079	2082	2086	rBV4	16267	27585	0.21%	0.025%
51	15.281	2086	2090	2095	rVB3	29185	51757	0.39%	0.047%
52	15.439	2110	2117	2133	rBV	6784999	10024514	76.20%	9.136%
53	15.569	2133	2139	2154	rBV	1964832	2861271	21.75%	2.608%
54	15.681	2154	2158	2164	rVB	31994	53115	0.40%	0.048%
55	15.975	2205	2208	2212	rBV2	21954	31301	0.24%	0.029%
56	16.433	2282	2286	2289	rBV4	26555	36417	0.28%	0.033%
57	16.686	2324	2329	2337	rBV6	46254	87136	0.66%	0.079%
58	16.992	2378	2381	2390	rVB6	43779	87227	0.66%	0.079%
59	17.163	2405	2410	2411	rBV	113465	135530	1.03%	0.124%
60	17.198	2411	2416	2427	rVV	4179612	6231168	47.36%	5.679%
61	17.304	2427	2434	2445	rVV	7500667	11069250	84.14%	10.088%
62	17.869	2527	2530	2534	rBV5	22743	34477	0.26%	0.031%
63	18.092	2563	2568	2574	rBV	362860	564293	4.29%	0.514%
64	19.116	2739	2742	2750	rBV	116098	176496	1.34%	0.161%
65	19.186	2750	2754	2765	rBV	155498	301358	2.29%	0.275%
66	19.327	2774	2778	2786	rBV	322718	512286	3.89%	0.467%
67	19.545	2809	2815	2828	rBV	9414713	13155782	100.00%	11.990%
68	21.004	3059	3063	3071	rBV	514397	752829	5.72%	0.686%
69	21.298	3108	3113	3119	rBV	4991216	6314680	48.00%	5.755%
70	23.533	3486	3493	3510	rVB2	5350836	10843583	82.42%	9.883%
71	23.686	3512	3519	3529	rVB2	2640792	5461466	41.51%	4.978%




Sum of corrected areas: 109722452

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP110222\
Data File : BP012455.D
Acq On : 02 Nov 2022 15:56
Operator : CG/JU
Sample : N5321-09
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DBWR5

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP102522.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

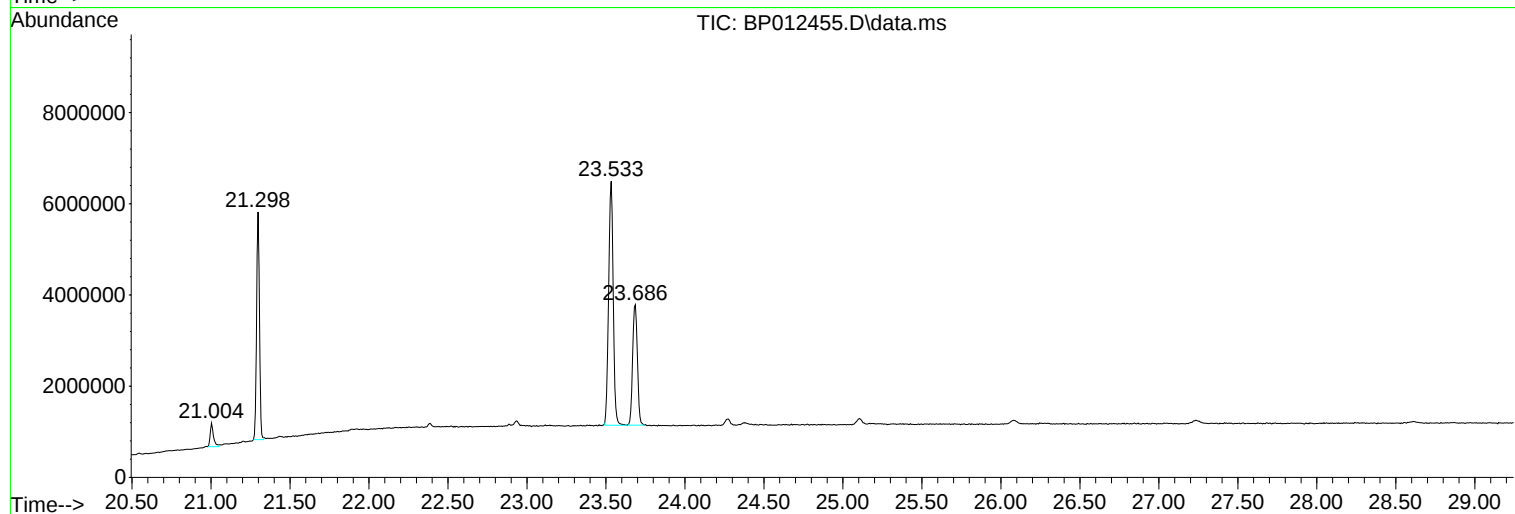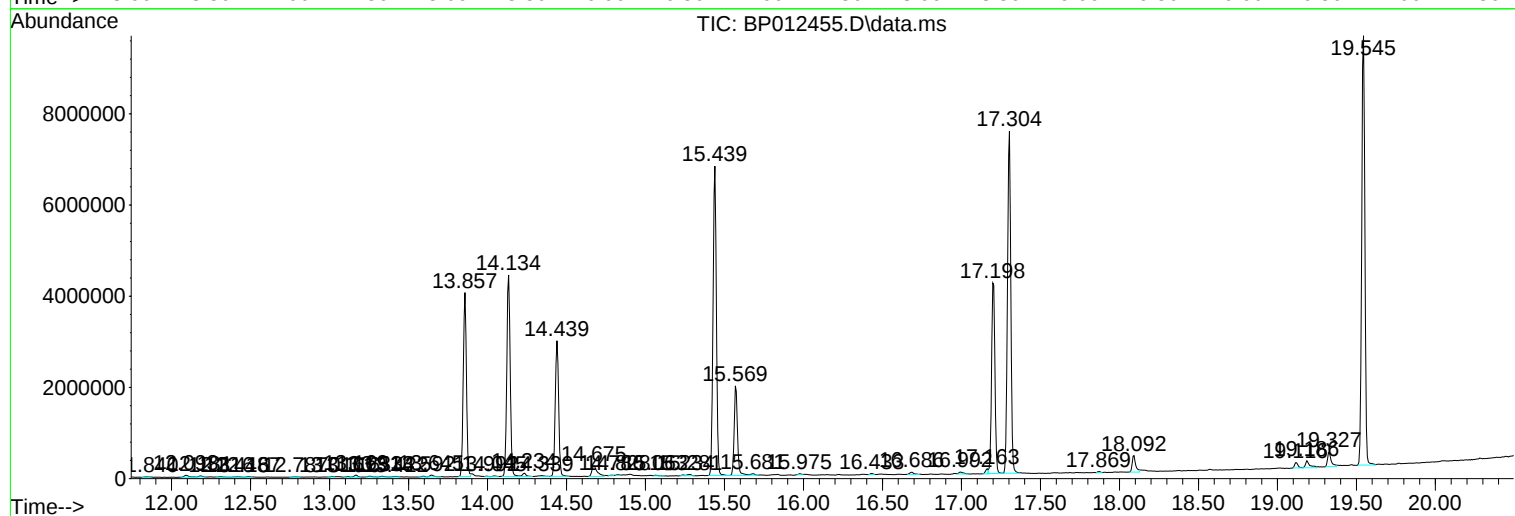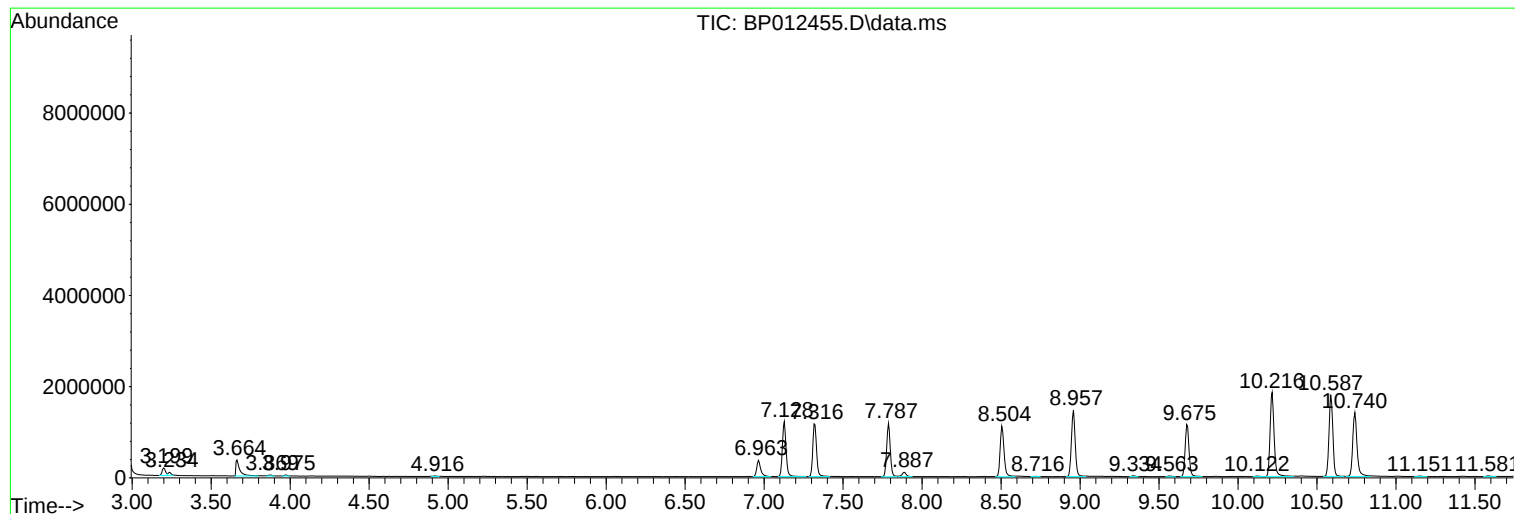

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP110222\
Data File : BP012455.D
Acq On : 02 Nov 2022 15:56
Operator : CG/JU
Sample : N5321-09
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DBWR5










Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP102522.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 (DEL) Alkane: Cyclic21.004 Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
21.004	2.38 ng/ul	752829	Chrysene-d12	21.298

Hit#	of 5	Tentative ID	MW	MolForm	CAS#	Qual
1		Cyclotetracosane	336	C24H48	000297-03-0	98
2		Cyclopentadecane	210	C15H30	000295-48-7	94
3		1-Heneicosyl formate	340	C22H44O2	077899-03-7	94
4		1-Heptacosanol	396	C27H56O	002004-39-9	94
5		Pentacos-1-ene	350	C25H50	016980-85-1	93

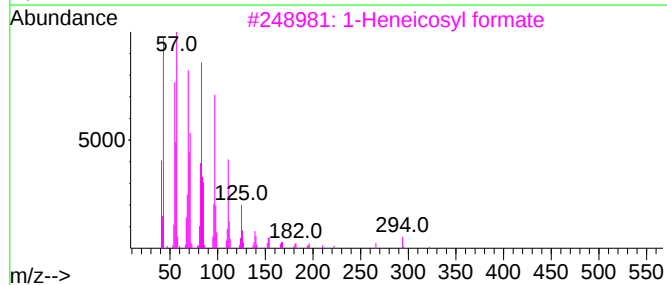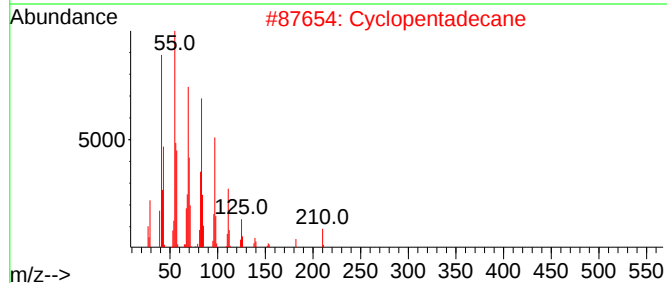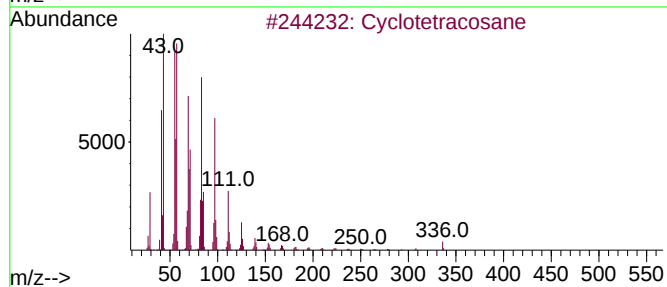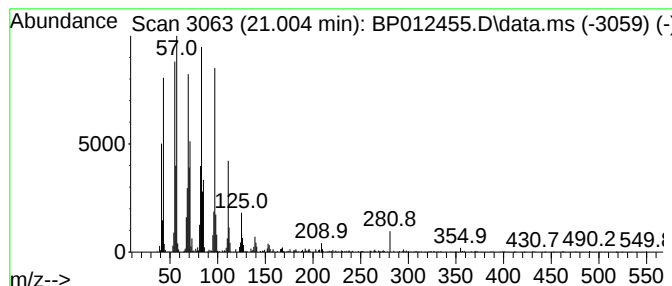

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP110222\
Data File : BP012455.D
Acq On : 02 Nov 2022 15:56
Operator : CG/JU
Sample : N5321-09
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DBWR5

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP102522.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
(DEL) Alkane: C...	21.004	2.4	ng/u1	752829	5	21.298	6314680	20.0