

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP110222\
 Data File : BP012458.D
 Acq On : 02 Nov 2022 19:25
 Operator : CG/JU
 Sample : PB148617BL
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SBLK617

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP102522.M
 Title : SVOA CALIBRATION

Signal : TIC: BP012458.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.234	38	42	49	rBV	82076	112852	1.20%	0.120%
2	3.658	111	114	140	rBV	994257	1618153	17.18%	1.714%
3	3.969	163	167	174	rVB	35576	54034	0.57%	0.057%
4	6.963	669	676	693	rBV	1314165	2172743	23.06%	2.301%
5	7.128	697	704	718	rVV	1122155	1811056	19.22%	1.918%
6	7.316	729	736	747	rBV	1317906	2162959	22.96%	2.291%
7	7.787	807	816	829	rBV	1163140	1902628	20.20%	2.015%
8	8.504	931	938	960	rBV	1673802	2885803	30.63%	3.056%
9	8.957	1007	1015	1032	rBV	1294775	2229308	23.66%	2.361%
10	9.675	1129	1137	1155	rBV	1104852	1896863	20.14%	2.009%
11	10.216	1221	1229	1250	rBV	1616705	2953906	31.36%	3.129%
12	10.587	1284	1292	1304	rBV	1819949	3032571	32.19%	3.212%
13	10.734	1310	1317	1348	rBV	1564928	3025993	32.12%	3.205%
14	12.193	1557	1565	1577	rBV2	21599	58460	0.62%	0.062%
15	13.410	1768	1772	1779	rVB4	5852	10220	0.11%	0.011%
16	13.857	1840	1848	1859	rBV	3366759	4697602	49.87%	4.975%
17	14.128	1884	1894	1911	rBV	3610402	5693232	60.43%	6.030%
18	14.439	1939	1947	1957	rBV	3089563	4448400	47.22%	4.711%
19	14.663	1978	1985	2008	rBV	1159298	2222818	23.60%	2.354%
20	15.434	2109	2116	2132	rBV	4706786	7188317	76.31%	7.613%
21	15.569	2133	2139	2154	rVV	1248467	1932406	20.51%	2.047%
22	15.675	2154	2157	2166	rVB	24866	49642	0.53%	0.053%
23	16.875	2357	2361	2365	rBV7	8051	11991	0.13%	0.013%
24	16.986	2375	2380	2386	rBV4	10178	24317	0.26%	0.026%
25	17.198	2410	2416	2426	rBV	3796257	5526086	58.66%	5.853%
26	17.298	2427	2433	2456	rVB2	5334291	8012372	85.05%	8.486%
27	19.116	2738	2742	2749	rBV2	72419	110853	1.18%	0.117%
28	19.186	2750	2754	2759	rBV	74100	111426	1.18%	0.118%
29	19.539	2808	2814	2824	rBV	6682337	9420480	100.00%	9.977%
30	21.298	3108	3113	3121	rBV	4211228	5673650	60.23%	6.009%
31	23.527	3485	3492	3504	rVB2	4021587	8268850	87.78%	8.758%
32	23.680	3512	3518	3528	rVB2	2532726	5099107	54.13%	5.401%




Sum of corrected areas: 94419098

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP110222\
Data File : BP012458.D
Acq On : 02 Nov 2022 19:25
Operator : CG/JU
Sample : PB148617BL
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK617

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP102522.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

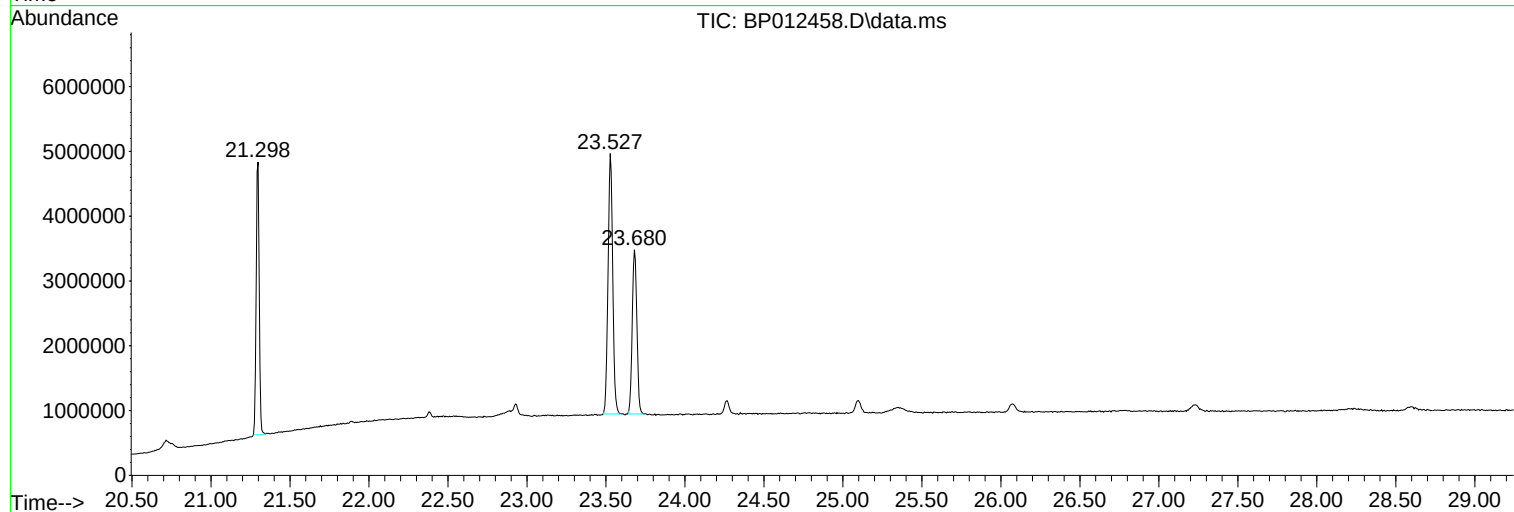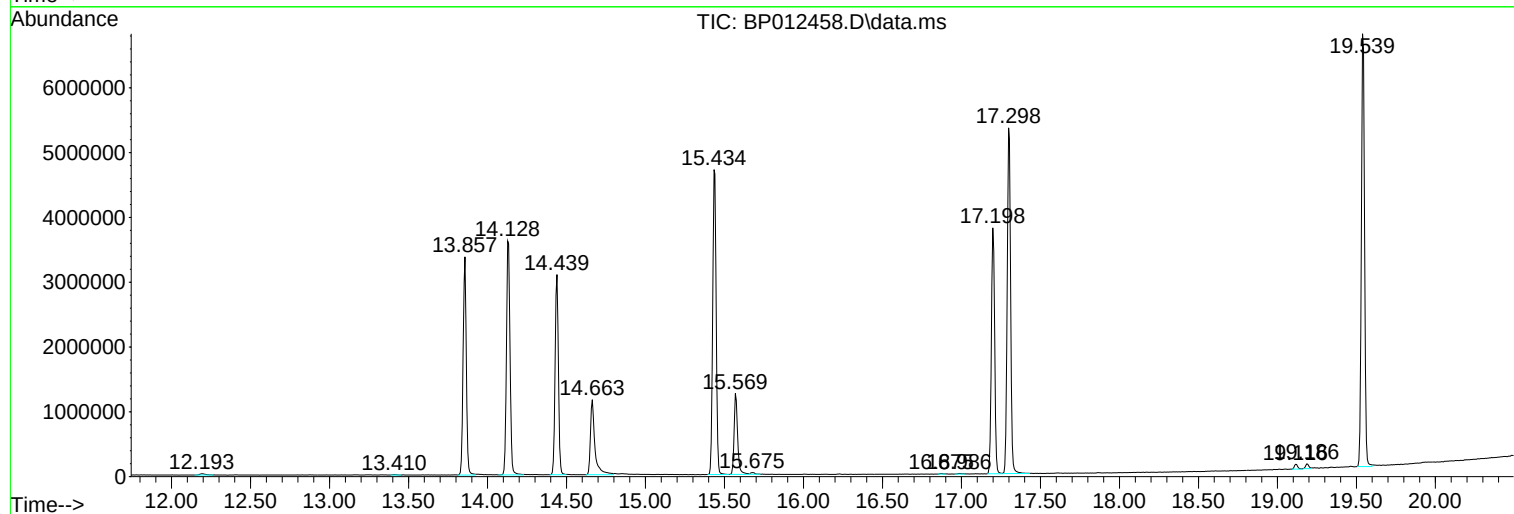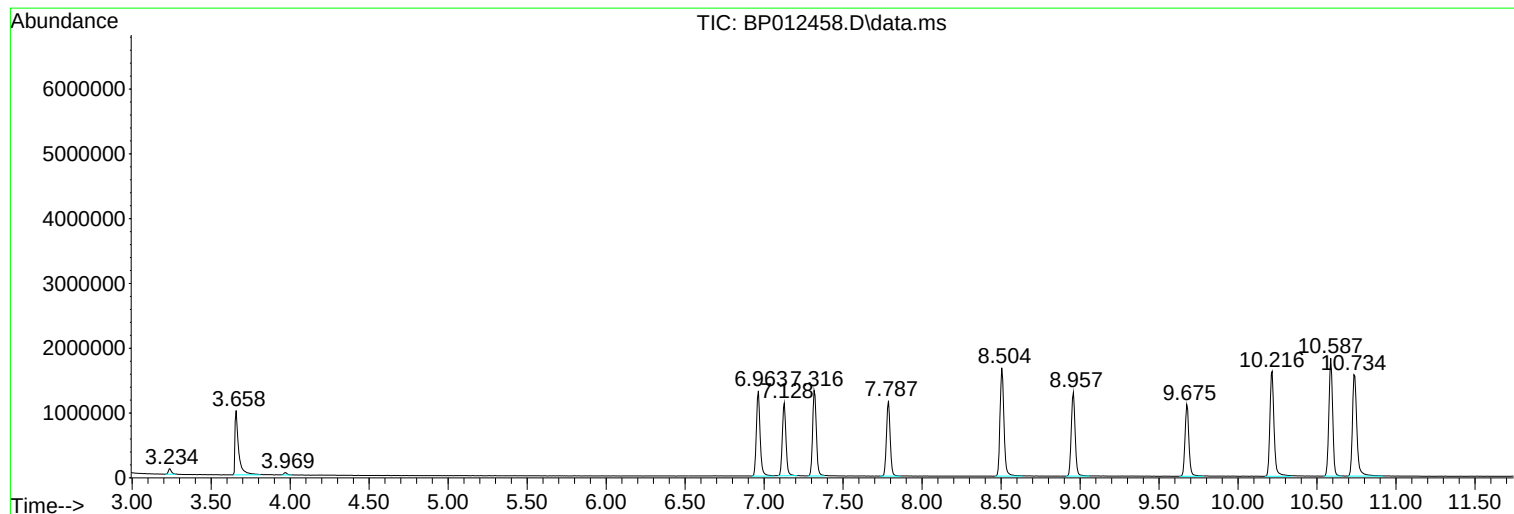

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP110222\
Data File : BP012458.D
Acq On : 02 Nov 2022 19:25
Operator : CG/JU
Sample : PB148617BL
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK617

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP102522.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP110222\
Data File : BP012458.D
Acq On : 02 Nov 2022 19:25
Operator : CG/JU
Sample : PB148617BL
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK617

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP102522.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------