

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP110222\
 Data File : BP012460.D
 Acq On : 02 Nov 2022 20:35
 Operator : CG/JU
 Sample : N5321-12
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DBWN6

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP102522.M
 Title : SVOA CALIBRATION

Signal : TIC: BP012460.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.199	31	36	53	rVB2	561420	968881	9.66%	1.054%
2	3.664	113	115	137	rBV	261894	513450	5.12%	0.558%
3	3.869	146	150	156	rVB	20582	33364	0.33%	0.036%
4	3.969	162	167	173	rVB	32056	51216	0.51%	0.056%
5	6.963	668	676	689	rBV	324613	561370	5.60%	0.611%
6	7.128	696	704	722	rBV	1056676	1778887	17.74%	1.935%
7	7.316	729	736	747	rBV	1060877	1747686	17.42%	1.901%
8	7.552	771	776	783	rBV3	11443	23305	0.23%	0.025%
9	7.787	809	816	825	rBV	1013771	1667611	16.63%	1.814%
10	7.887	826	833	845	rVB2	176340	324263	3.23%	0.353%
11	8.387	910	918	927	rBV2	10338	30792	0.31%	0.033%
12	8.505	930	938	951	rVV	988309	1689521	16.84%	1.837%
13	8.605	952	955	966	rVB6	15898	38108	0.38%	0.041%
14	8.957	1004	1015	1026	rBV	1304676	2215780	22.09%	2.410%
15	9.104	1036	1040	1049	rVB5	12569	29331	0.29%	0.032%
16	9.410	1088	1092	1099	rVB5	7800	12210	0.12%	0.013%
17	9.563	1111	1118	1127	rVB2	20793	39097	0.39%	0.043%
18	9.675	1130	1137	1154	rBV	1071175	1801104	17.96%	1.959%
19	10.122	1207	1213	1221	rVB5	6145	12408	0.12%	0.013%
20	10.216	1221	1229	1243	rBV	1643733	3001264	29.92%	3.264%
21	10.587	1284	1292	1307	rVB	1599255	2720263	27.12%	2.958%
22	10.740	1310	1318	1334	rBV	1229503	2284058	22.77%	2.484%
23	11.151	1382	1388	1391	rVB7	5421	10442	0.10%	0.011%
24	11.581	1455	1461	1465	rBV	12236	22991	0.23%	0.025%
25	12.122	1540	1553	1559	rBV	162252	304735	3.04%	0.331%
26	12.181	1560	1563	1570	rVB2	25907	43978	0.44%	0.048%
27	12.310	1578	1585	1595	rVB2	9594	29635	0.30%	0.032%
28	12.422	1595	1604	1610	rBV2	9832	24983	0.25%	0.027%
29	12.487	1610	1615	1624	rVB7	11389	22849	0.23%	0.025%
30	12.787	1659	1666	1669	rBV9	7906	15346	0.15%	0.017%
31	13.010	1700	1704	1709	rBV2	37740	70026	0.70%	0.076%
32	13.057	1709	1712	1718	rVV	42121	64946	0.65%	0.071%
33	13.116	1718	1722	1725	rVV3	9477	11488	0.11%	0.012%
34	13.163	1725	1730	1736	rVV2	68552	111661	1.11%	0.121%
35	13.251	1740	1745	1753	rBV2	8169	18010	0.18%	0.020%
36	13.328	1753	1758	1767	rBV10	14513	28421	0.28%	0.031%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP110222\
 Data File : BP012460.D
 Acq On : 02 Nov 2022 20:35
 Operator : CG/JU
 Sample : N5321-12
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DBWN6

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF Filtering: 5
 Sampling : 1 Min Area: 0.1 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP102522.M
 Title : SVOA CALIBRATION

37	13.422	1767	1774	1778	rBV5	15703	30852	0.31%	0.034%
38	13.592	1798	1803	1807	rBV3	21275	32725	0.33%	0.036%
39	13.645	1807	1812	1821	rVV	58222	106774	1.06%	0.116%
40	13.857	1841	1848	1855	rBV	3520564	4963357	49.49%	5.398%
41	13.992	1869	1871	1876	rVB4	9067	10412	0.10%	0.011%
42	14.045	1876	1880	1886	rBV2	22907	38034	0.38%	0.041%
43	14.134	1888	1895	1906	rVV	3872384	5939932	59.22%	6.460%
44	14.234	1908	1912	1921	rVB2	49896	81987	0.82%	0.089%
45	14.345	1928	1931	1937	rVB4	16593	25499	0.25%	0.028%
46	14.440	1940	1947	1959	rVV	2602194	3965739	39.54%	4.313%
47	14.675	1981	1987	2002	rBV2	201595	527504	5.26%	0.574%
48	14.828	2009	2013	2015	rBV4	11684	16670	0.17%	0.018%
49	14.898	2022	2025	2036	rVB	25636	50911	0.51%	0.055%
50	15.239	2079	2083	2085	rBV4	19606	31713	0.32%	0.034%
51	15.269	2086	2088	2096	rVB3	27241	43921	0.44%	0.048%
52	15.345	2098	2101	2106	rBV6	14740	26183	0.26%	0.028%
53	15.434	2110	2116	2133	rVB	5081174	7747767	77.25%	8.426%
54	15.569	2133	2139	2153	rBV	1597208	2350397	23.43%	2.556%
55	15.675	2155	2157	2164	rVB	29401	40963	0.41%	0.045%
56	15.975	2204	2208	2212	rBV3	36899	62297	0.62%	0.068%
57	16.222	2248	2250	2256	rVB5	10500	15900	0.16%	0.017%
58	16.369	2272	2275	2281	rBV5	30353	53918	0.54%	0.059%
59	16.428	2282	2285	2289	rBV4	28664	36713	0.37%	0.040%
60	16.686	2324	2329	2338	rVB3	48204	84138	0.84%	0.092%
61	16.992	2378	2381	2393	rVB8	46127	85693	0.85%	0.093%
62	17.157	2405	2409	2411	rBV	93613	124973	1.25%	0.136%
63	17.198	2411	2416	2426	rVV	3353543	4956952	49.42%	5.391%
64	17.298	2427	2433	2449	rVV	5606904	8449104	84.24%	9.189%
65	18.086	2563	2567	2574	rBV	131001	221261	2.21%	0.241%
66	19.116	2739	2742	2748	rVB	87216	108215	1.08%	0.118%
67	19.186	2751	2754	2759	rVV	84010	109364	1.09%	0.119%
68	19.322	2774	2777	2784	rBV	131774	205767	2.05%	0.224%
69	19.539	2808	2814	2821	rBV	7326673	10029820	100.00%	10.908%
70	21.292	3108	3112	3121	rBV	4050572	5251550	52.36%	5.711%
71	23.527	3485	3492	3504	rVB2	4311962	9011966	89.85%	9.801%
72	23.680	3512	3518	3527	rVB2	2412838	4786907	47.73%	5.206%




Sum of corrected areas: 91949358

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP110222\
Data File : BP012460.D
Acq On : 02 Nov 2022 20:35
Operator : CG/JU
Sample : N5321-12
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DBWN6

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP102522.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

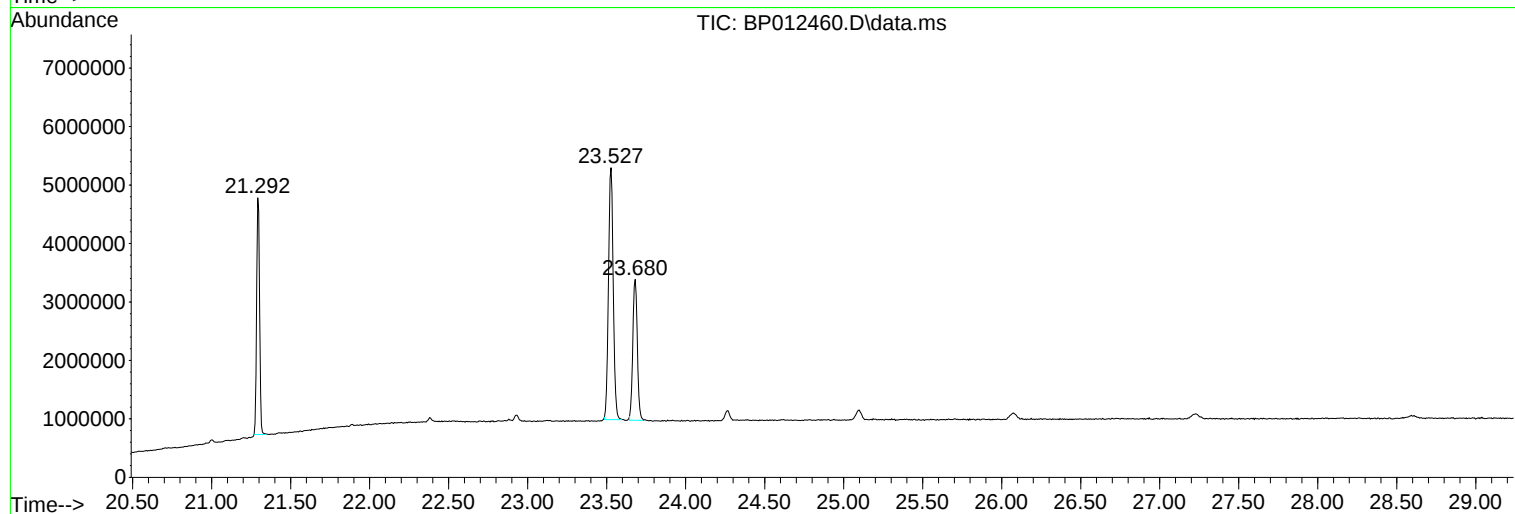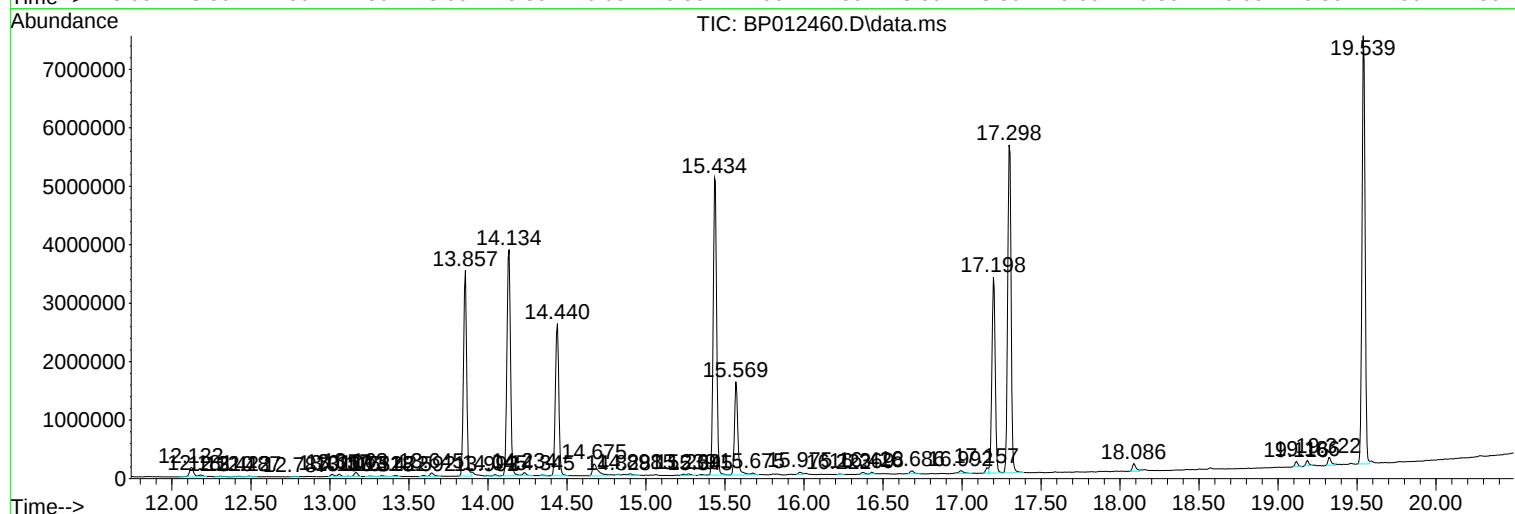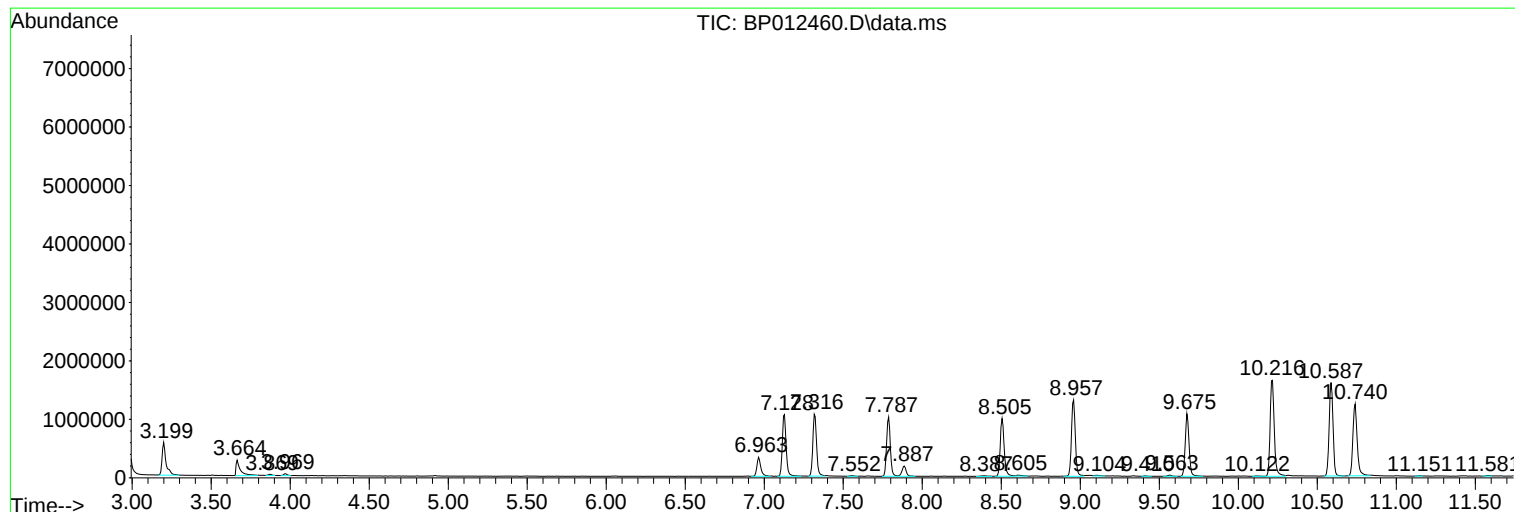

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP110222\
Data File : BP012460.D
Acq On : 02 Nov 2022 20:35
Operator : CG/JU
Sample : N5321-12
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DBWN6










Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP102522.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 unknown-01 Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
7.887	3.89 ng/ul	324263	1,4-Dichlorobenzene-d4	7.787

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			1-Methyl-1H-1,2,4-triazole	83	C3H5N3	006086-21-1	49
2			1H-Pyrazole, 4,5-dihydro-1,5-dim...	98	C5H10N2	005775-96-2	47
3			Propanenitrile, 2-(dimethylamino)-	98	C5H10N2	005350-67-4	47
4			1H-Pyrazole, 4,5-dihydro-1,5-dim...	98	C5H10N2	005775-96-2	40
5			3-Methyl-2-butenic acid, oct-3-...	210	C13H22O2	1000299-31-2	38

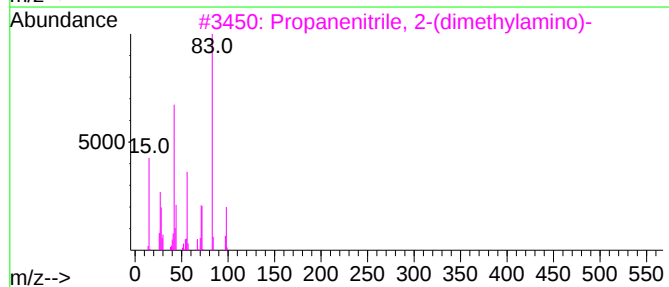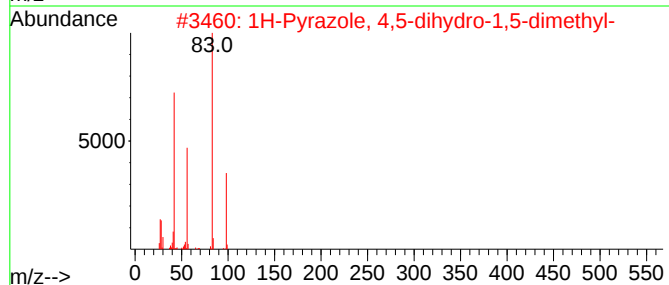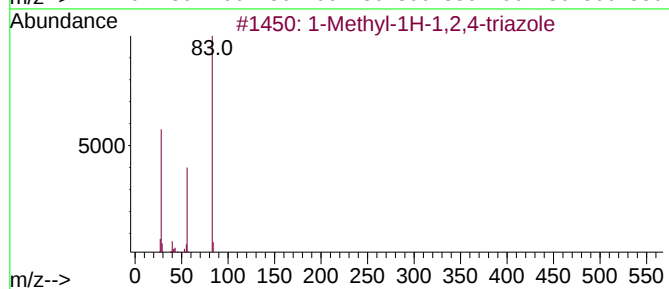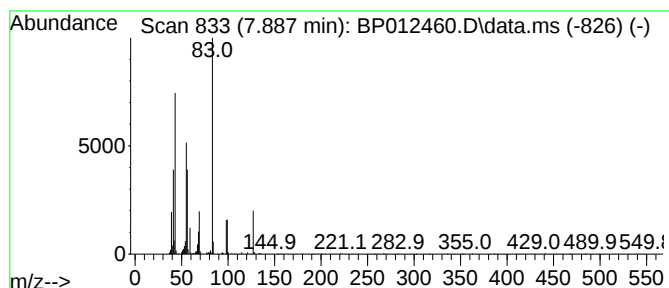

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP110222\
Data File : BP012460.D
Acq On : 02 Nov 2022 20:35
Operator : CG/JU
Sample : N5321-12
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DBWN6










Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP102522.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 2 unknown-02 Concentration Rank 2

R.T.	EstConc	Area	Relative to ISTD	R.T.
12.122	2.24 ng/ul	304735	Naphthalene-d8	10.587

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			1,2,3,4-Tetrahydropentalene, 1,1...	171	C12H13N	1000217-18-6	37
2			Bicyclo[3.2.0]hept-2-ene, 4-isop...	171	C12H13N	1000217-15-6	32
3			4-Chloro-3,5-dimethylphenol, O-i...	242	C12H15ClO3	1000487-39-3	32
4			Chloroxylenol	156	C8H9ClO	000088-04-0	32
5			Benzene, 2,5-cyclohexadien-1-yl-	156	C12H12	004794-05-2	28

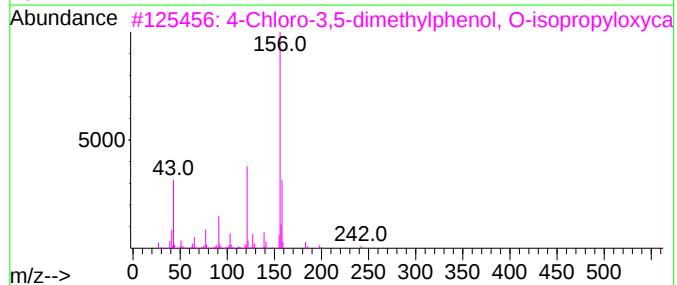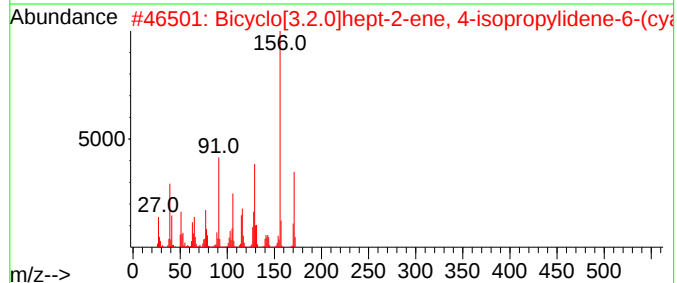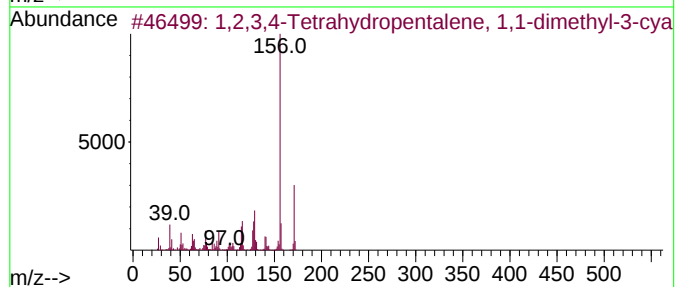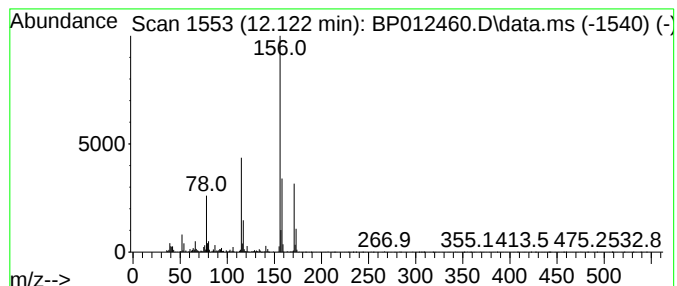

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP110222\
Data File : BP012460.D
Acq On : 02 Nov 2022 20:35
Operator : CG/JU
Sample : N5321-12
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DBWN6

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP102522.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST0.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
unknown-01	7.887	3.9	ng/u1	324263	1	7.787	1667610	20.0
unknown-02	12.122	2.2	ng/u1	304735	2	10.587	2720260	20.0