

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP110222\
 Data File : BP012462.D
 Acq On : 02 Nov 2022 21:44
 Operator : CG/JU
 Sample : N5300-08
 Misc :
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 BHAC4

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP102522.M
 Title : SVOA CALIBRATION

Signal : TIC: BP012462.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.028	4	7	26	rVB	417759	739138	5.90%	0.677%
2	3.240	38	43	56	rVB	63125	101944	0.81%	0.093%
3	3.664	113	115	140	rBV	304953	567078	4.52%	0.519%
4	3.875	146	151	156	rVB	20202	35781	0.29%	0.033%
5	3.969	163	167	173	rVB	32805	43854	0.35%	0.040%
6	4.911	324	327	336	rVB	24415	40883	0.33%	0.037%
7	6.963	670	676	692	rBV	320164	558676	4.46%	0.512%
8	7.122	697	703	716	rBV	1285756	2117303	16.89%	1.939%
9	7.316	730	736	747	rBV	1189955	1947098	15.53%	1.783%
10	7.787	807	816	824	rBV	1301122	2125694	16.96%	1.946%
11	7.857	824	828	836	rVB3	19722	46913	0.37%	0.043%
12	7.993	846	851	857	rBV5	7937	16084	0.13%	0.015%
13	8.187	877	884	893	rBV	27405	57458	0.46%	0.053%
14	8.504	931	938	957	rBV	1039965	1743370	13.91%	1.596%
15	8.957	1007	1015	1029	rBV	1578868	2639230	21.05%	2.416%
16	9.116	1037	1042	1052	rVB	7630	17574	0.14%	0.016%
17	9.340	1074	1080	1085	rBV4	9650	16365	0.13%	0.015%
18	9.675	1129	1137	1155	rBV	1264468	2159275	17.23%	1.977%
19	9.834	1159	1164	1170	rBV3	15859	29621	0.24%	0.027%
20	10.210	1220	1228	1249	rBV	1869167	3337102	26.62%	3.055%
21	10.587	1282	1292	1305	rBV	2011706	3467639	27.66%	3.175%
22	10.740	1311	1318	1341	rVB	1431000	2674197	21.33%	2.448%
23	12.187	1558	1564	1571	rBV2	28091	55603	0.44%	0.051%
24	12.257	1571	1576	1582	rBV3	16777	37731	0.30%	0.035%
25	12.969	1691	1697	1704	rBV2	20377	44642	0.36%	0.041%
26	13.063	1707	1713	1719	rVV	25716	44753	0.36%	0.041%
27	13.292	1747	1752	1757	rBV	58552	97922	0.78%	0.090%
28	13.404	1767	1771	1776	rBV3	8230	13564	0.11%	0.012%
29	13.781	1829	1835	1839	rBV8	9165	22327	0.18%	0.020%
30	13.857	1841	1848	1860	rVV	4264197	6105431	48.71%	5.590%
31	14.134	1887	1895	1919	rBV	4467863	6865959	54.77%	6.286%
32	14.439	1934	1947	1957	rBV	3436607	5024040	40.08%	4.600%
33	14.675	1980	1987	2000	rBV	207883	527831	4.21%	0.483%
34	15.434	2109	2116	2131	rBV	6265525	9421349	75.16%	8.626%
35	15.569	2133	2139	2151	rVV	2174648	2990239	23.85%	2.738%
36	15.675	2153	2157	2165	rVB3	36304	65838	0.53%	0.060%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP110222\
 Data File : BP012462.D
 Acq On : 02 Nov 2022 21:44
 Operator : CG/JU
 Sample : N5300-08
 Misc :
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 BHAC4

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF Filtering: 5
 Sampling : 1 Min Area: 0.1 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP102522.M
 Title : SVOA CALIBRATION

37	16.086	2223	2227	2234	rVB5	11085	17595	0.14%	0.016%
38	16.710	2330	2333	2342	rBV3	19885	46073	0.37%	0.042%
39	16.875	2358	2361	2366	rVB5	9609	14320	0.11%	0.013%
40	17.198	2410	2416	2426	rBV	4266980	6178963	49.29%	5.657%
41	17.298	2427	2433	2447	rVV2	7218641	10897261	86.93%	9.978%
42	17.869	2526	2530	2534	rBV2	35632	46463	0.37%	0.043%
43	18.086	2563	2567	2576	rBV	188801	300414	2.40%	0.275%
44	19.116	2738	2742	2747	rBV	115860	147580	1.18%	0.135%
45	19.186	2750	2754	2760	rBV	120255	201261	1.61%	0.184%
46	19.322	2774	2777	2789	rBV2	207801	339981	2.71%	0.311%
47	19.539	2808	2814	2829	rBV	8971571	12535457	100.00%	11.477%
48	20.998	3059	3062	3068	rBV	245668	342583	2.73%	0.314%
49	21.292	3107	3112	3121	rBV	4670549	6269348	50.01%	5.740%
50	23.527	3485	3492	3505	rVB2	5314332	10615419	84.68%	9.719%
51	23.680	3511	3518	3527	rVB2	2664018	5465972	43.60%	5.005%




Sum of corrected areas: 109218196

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP110222\
Data File : BP012462.D
Acq On : 02 Nov 2022 21:44
Operator : CG/JU
Sample : N5300-08
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
BHAC4

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP102522.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

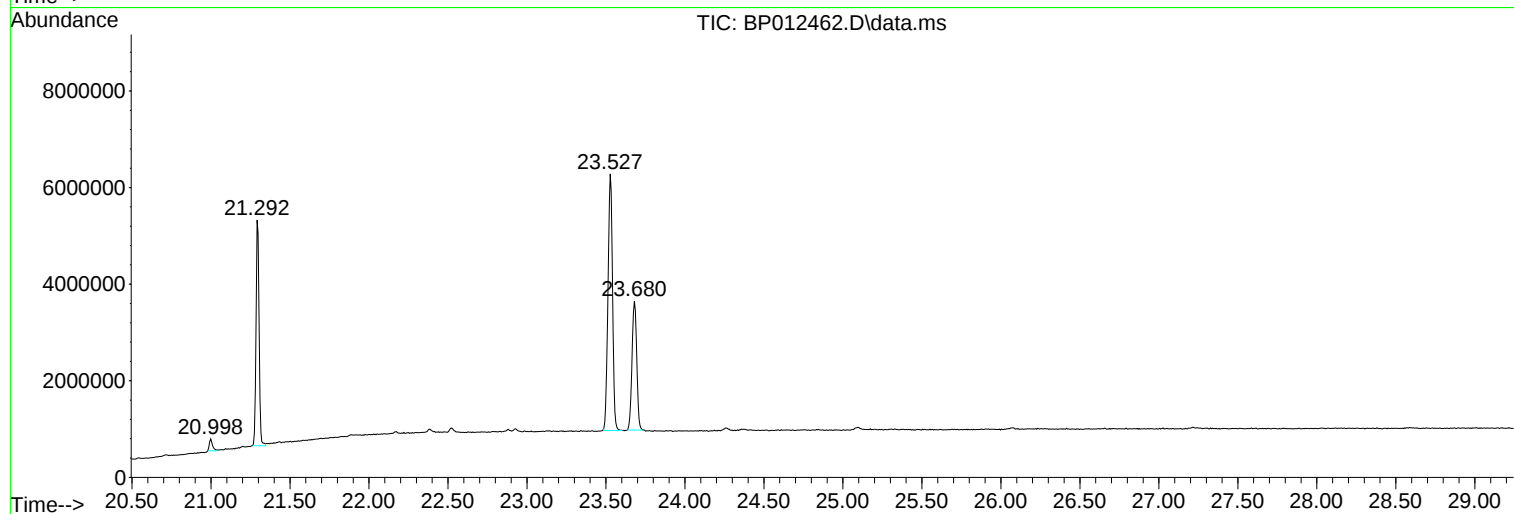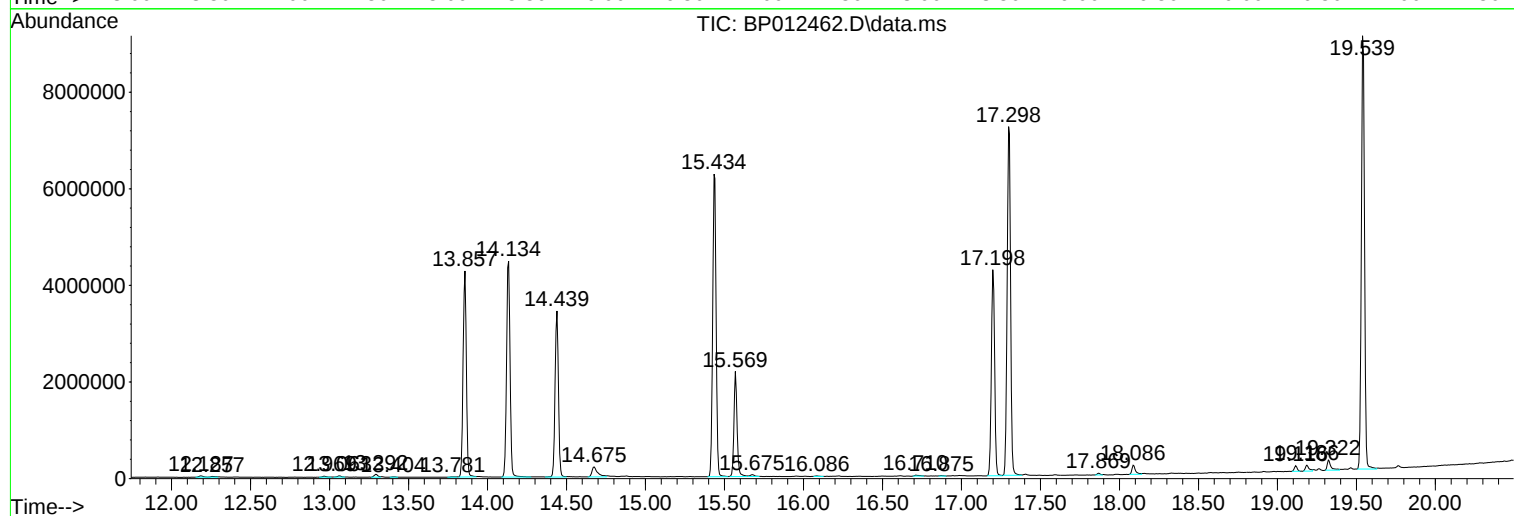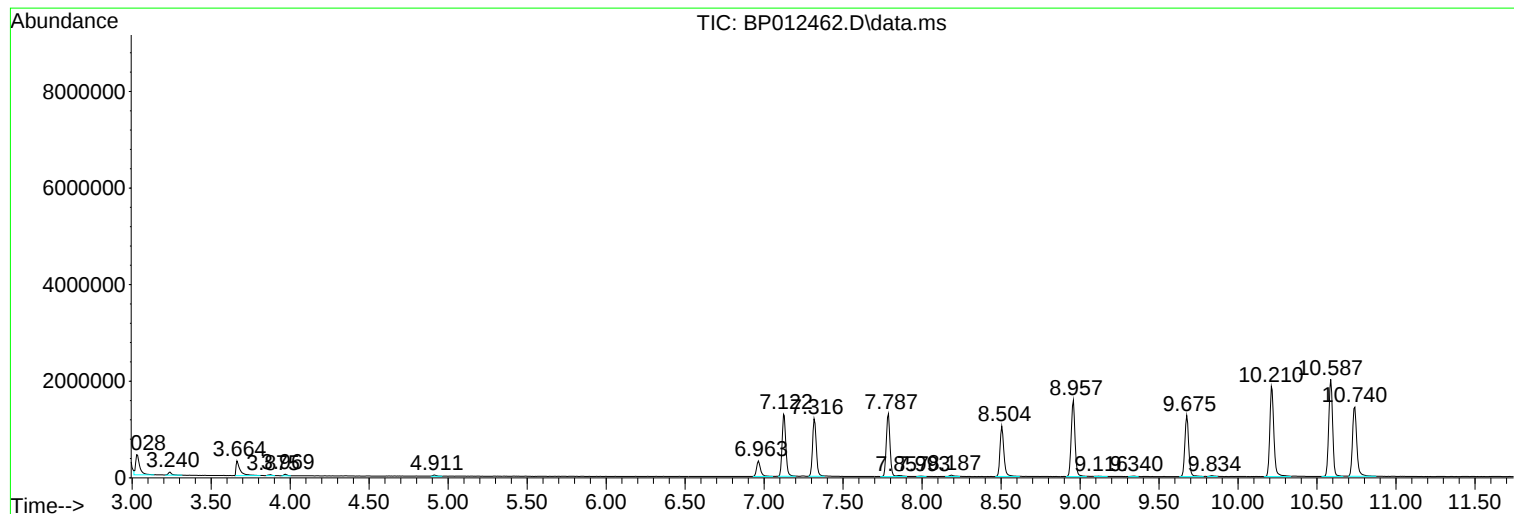

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP110222\
Data File : BP012462.D
Acq On : 02 Nov 2022 21:44
Operator : CG/JU
Sample : N5300-08
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
BHAC4










Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP102522.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 Triethylamine Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
3.028	6.95 ng/ul	739138	1,4-Dichlorobenzene-d4	7.787

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			Triethylamine	101	C6H15N	000121-44-8	91
2			Triethylamine	101	C6H15N	000121-44-8	91
3			Triethylamine	101	C6H15N	000121-44-8	90
4			Tetraethylammonium chloride	165	C8H20ClN	000056-34-8	78
5			Tetraethyl ammonium fluoride	149	C8H20FN	000665-46-3	78

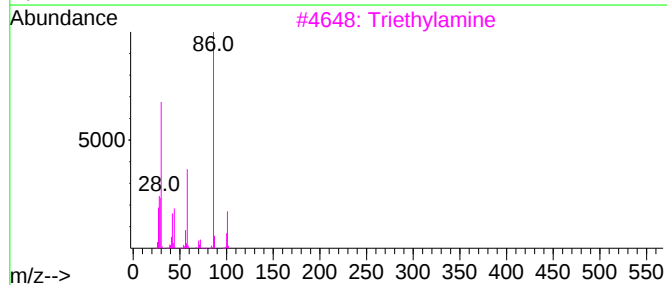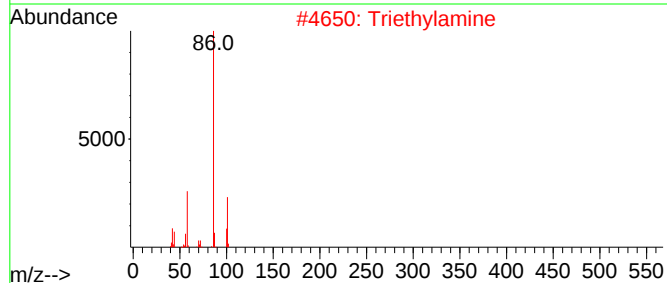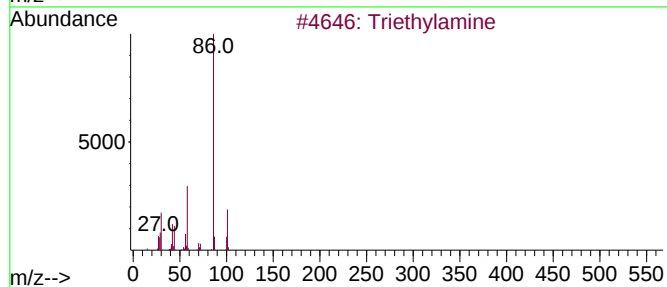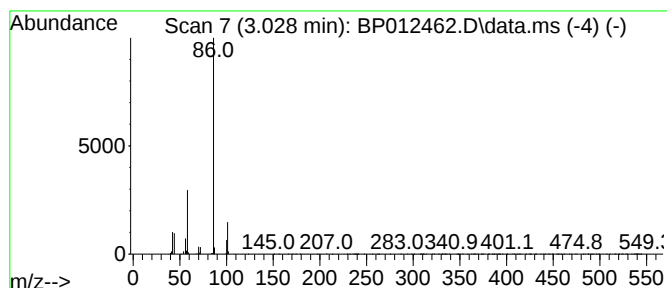

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP110222\
Data File : BP012462.D
Acq On : 02 Nov 2022 21:44
Operator : CG/JU
Sample : N5300-08
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
BHAC4

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP102522.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST0.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
Triethylamine	3.028	7.0	ng/u1	739138	1	7.787	2125690	20.0