

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP110222\
 Data File : BP012466.D
 Acq On : 03 Nov 2022 00:02
 Operator : CG/JU
 Sample : N5300-13
 Misc :
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 BHA91

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP102522.M
 Title : SVOA CALIBRATION

Signal : TIC: BP012466.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.234	38	42	47	rBV	44194	53977	0.50%	0.059%
2	3.664	113	115	134	rBV	164541	301803	2.81%	0.333%
3	3.869	146	150	156	rVB2	15157	23297	0.22%	0.026%
4	3.969	163	167	172	rVB	24252	31926	0.30%	0.035%
5	4.905	320	326	334	rBV	47675	77713	0.72%	0.086%
6	5.787	472	476	481	rVB5	6743	11445	0.11%	0.013%
7	6.769	638	643	647	rBV8	8076	12312	0.11%	0.014%
8	6.963	670	676	689	rVB	253645	425119	3.96%	0.468%
9	7.122	697	703	721	rBV	957087	1535636	14.31%	1.692%
10	7.316	728	736	746	rBV	918881	1470244	13.70%	1.620%
11	7.463	757	761	765	rVV6	7744	13301	0.12%	0.015%
12	7.528	768	772	781	rVB6	7546	17730	0.17%	0.020%
13	7.634	784	790	796	rBV9	6870	11143	0.10%	0.012%
14	7.781	808	815	824	rBV	938533	1535322	14.31%	1.692%
15	8.222	881	890	895	rBV3	8768	14876	0.14%	0.016%
16	8.504	927	938	955	rBV	805976	1385818	12.92%	1.527%
17	8.687	965	969	979	rVB	9792	17933	0.17%	0.020%
18	8.775	979	984	990	rBV8	9400	13835	0.13%	0.015%
19	8.952	1007	1014	1035	rVV	1157159	1998683	18.63%	2.202%
20	9.263	1061	1067	1071	rVB9	7057	13001	0.12%	0.014%
21	9.340	1075	1080	1085	rBV5	15613	29877	0.28%	0.033%
22	9.675	1129	1137	1152	rBV	954042	1636688	15.25%	1.804%
23	9.828	1158	1163	1169	rVB2	22000	33493	0.31%	0.037%
24	10.028	1188	1197	1203	rVB9	13597	27678	0.26%	0.030%
25	10.210	1219	1228	1249	rBV	1512561	2757191	25.70%	3.038%
26	10.440	1266	1267	1273	rVB6	8806	11845	0.11%	0.013%
27	10.587	1284	1292	1305	rBV	1481871	2586440	24.10%	2.850%
28	10.734	1310	1317	1336	rVV	1248947	2306559	21.50%	2.542%
29	10.963	1348	1356	1362	rBV7	11207	31808	0.30%	0.035%
30	11.187	1387	1394	1402	rVB10	9550	23236	0.22%	0.026%
31	11.428	1427	1435	1439	rBV6	13262	35940	0.33%	0.040%
32	11.551	1451	1456	1460	rBV8	8794	15439	0.14%	0.017%
33	11.616	1462	1467	1472	rVB7	8076	17152	0.16%	0.019%
34	11.745	1484	1489	1493	rBV2	16366	24718	0.23%	0.027%
35	11.793	1493	1497	1501	rVV5	9598	15293	0.14%	0.017%
36	11.845	1501	1506	1512	rVV7	15471	28571	0.27%	0.031%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP110222\
 Data File : BP012466.D
 Acq On : 03 Nov 2022 00:02
 Operator : CG/JU
 Sample : N5300-13
 Misc :
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 BHA91

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP102522.M
 Title : SVOA CALIBRATION

37	11.916	1512	1518	1528	rVB4	26018	49869	0.46%	0.055%
38	12.175	1557	1562	1567	rBV2	30438	54313	0.51%	0.060%
39	12.240	1568	1573	1578	rVV2	34777	59986	0.56%	0.066%
40	12.310	1583	1585	1594	rVB10	10815	18763	0.17%	0.021%
41	12.404	1596	1601	1612	rVB5	32354	77274	0.72%	0.085%
42	12.493	1612	1616	1619	rBV6	7721	12344	0.12%	0.014%
43	12.545	1621	1625	1629	rBV7	15538	29855	0.28%	0.033%
44	12.692	1644	1650	1660	rBV	122961	205126	1.91%	0.226%
45	12.781	1660	1665	1669	rBV4	8517	17770	0.17%	0.020%
46	12.845	1670	1676	1683	rVB8	24547	46155	0.43%	0.051%
47	12.916	1683	1688	1691	rBV	30619	46510	0.43%	0.051%
48	12.957	1691	1695	1700	rVV2	25317	53438	0.50%	0.059%
49	13.028	1703	1707	1709	rVV4	25513	40474	0.38%	0.045%
50	13.057	1709	1712	1718	rVV	31308	54735	0.51%	0.060%
51	13.175	1727	1732	1738	rBV10	5579	12595	0.12%	0.014%
52	13.240	1739	1743	1748	rBV8	6325	12114	0.11%	0.013%
53	13.328	1754	1758	1762	rVB4	12591	16580	0.15%	0.018%
54	13.416	1766	1773	1782	rBV2	73106	125832	1.17%	0.139%
55	13.587	1795	1802	1805	rBV5	16040	31491	0.29%	0.035%
56	13.740	1821	1828	1832	rBV7	22625	50188	0.47%	0.055%
57	13.792	1832	1837	1841	rBV3	42583	63185	0.59%	0.070%
58	13.851	1841	1847	1856	rBV	3435949	4981143	46.42%	5.489%
59	13.963	1862	1866	1870	rBV4	18339	27243	0.25%	0.030%
60	14.128	1888	1894	1901	rVV2	3729033	5586056	52.06%	6.156%
61	14.204	1904	1907	1910	rVV3	58918	90265	0.84%	0.099%
62	14.245	1910	1914	1932	rVB	168639	308991	2.88%	0.340%
63	14.434	1939	1946	1964	rBV	2421787	3984782	37.14%	4.391%
64	14.587	1967	1972	1978	rVV6	25807	60306	0.56%	0.066%
65	14.675	1980	1987	2001	rVV2	206554	608459	5.67%	0.670%
66	14.787	2002	2006	2011	rVV	61345	120067	1.12%	0.132%
67	14.863	2015	2019	2026	rVV9	41931	86424	0.81%	0.095%
68	14.928	2026	2030	2033	rVV5	42058	66295	0.62%	0.073%
69	14.969	2033	2037	2043	rVB3	57877	91592	0.85%	0.101%
70	15.192	2070	2075	2084	rBV	146701	238853	2.23%	0.263%
71	15.275	2086	2089	2090	rBV3	10983	12863	0.12%	0.014%
72	15.434	2109	2116	2125	rBV	5155320	7691276	71.68%	8.475%
73	15.569	2133	2139	2144	rBV	1374216	1986224	18.51%	2.189%
74	15.851	2183	2187	2200	rVB5	46351	91815	0.86%	0.101%
75	16.086	2223	2227	2233	rBV3	32397	56080	0.52%	0.062%
76	16.475	2290	2293	2298	rVB3	47039	62460	0.58%	0.069%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP110222\
 Data File : BP012466.D
 Acq On : 03 Nov 2022 00:02
 Operator : CG/JU
 Sample : N5300-13
 Misc :
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 BHA91

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP102522.M
 Title : SVOA CALIBRATION

77	16.675	2324	2327	2330	rBV6	20594	27571	0.26%	0.030%
78	17.157	2405	2409	2410	rBV3	16729	20883	0.19%	0.023%
79	17.198	2410	2416	2426	rVV	3174478	4635749	43.20%	5.108%
80	17.298	2426	2433	2449	rVB2	6103787	8916957	83.10%	9.826%
81	17.492	2462	2466	2471	rBV3	23208	47084	0.44%	0.052%
82	17.545	2471	2475	2479	rVV3	33063	45448	0.42%	0.050%
83	17.645	2488	2492	2495	rBV3	59837	76597	0.71%	0.084%
84	17.863	2526	2529	2535	rVB2	42855	50409	0.47%	0.056%
85	18.028	2553	2557	2562	rBV4	45216	73663	0.69%	0.081%
86	18.086	2563	2567	2575	rVV2	158893	254302	2.37%	0.280%
87	19.116	2738	2742	2747	rBV	94470	130864	1.22%	0.144%
88	19.186	2750	2754	2761	rBV	91794	155025	1.44%	0.171%
89	19.322	2774	2777	2784	rVB	72761	96334	0.90%	0.106%
90	19.539	2808	2814	2821	rBV	7781576	10729907	100.00%	11.824%
91	20.992	3058	3061	3070	rBV2	220978	359750	3.35%	0.396%
92	21.157	3086	3089	3092	rVB2	134996	149159	1.39%	0.164%
93	21.292	3107	3112	3118	rBV	4168872	5064183	47.20%	5.580%
94	23.527	3484	3492	3504	rVB2	4617579	9667032	90.09%	10.653%
95	23.674	3511	3517	3527	rVB2	2242379	4470205	41.66%	4.926%




Sum of corrected areas: 90747955

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP110222\
Data File : BP012466.D
Acq On : 03 Nov 2022 00:02
Operator : CG/JU
Sample : N5300-13
Misc :
ALS Vial : 20 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
BHA91

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP102522.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

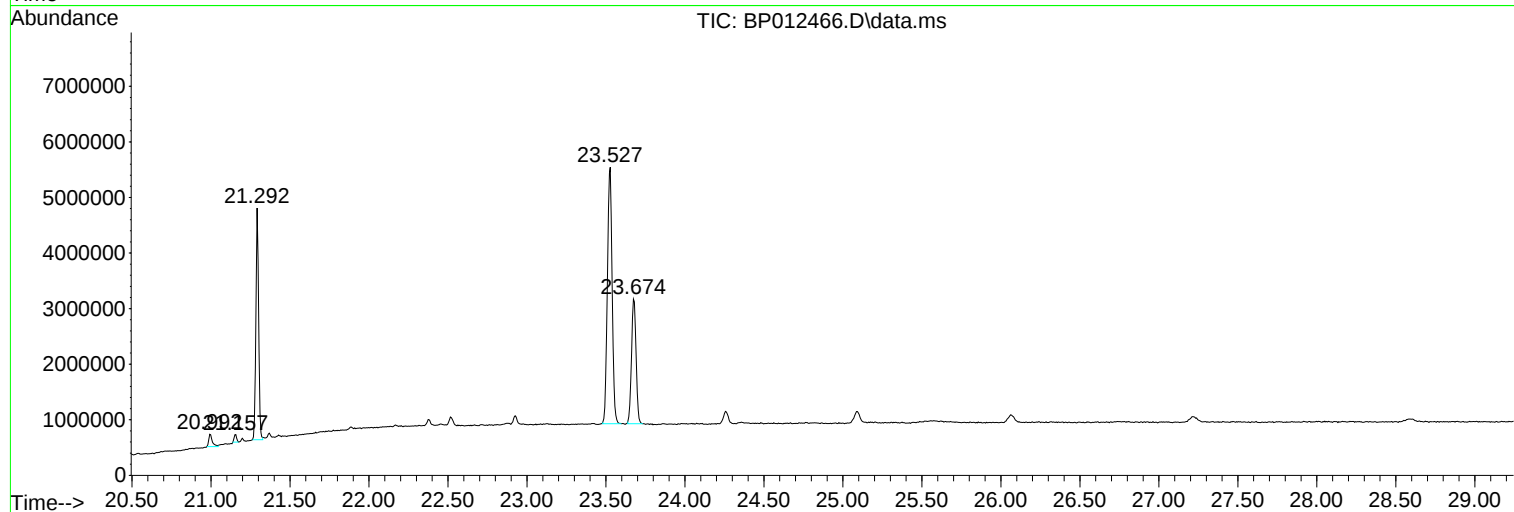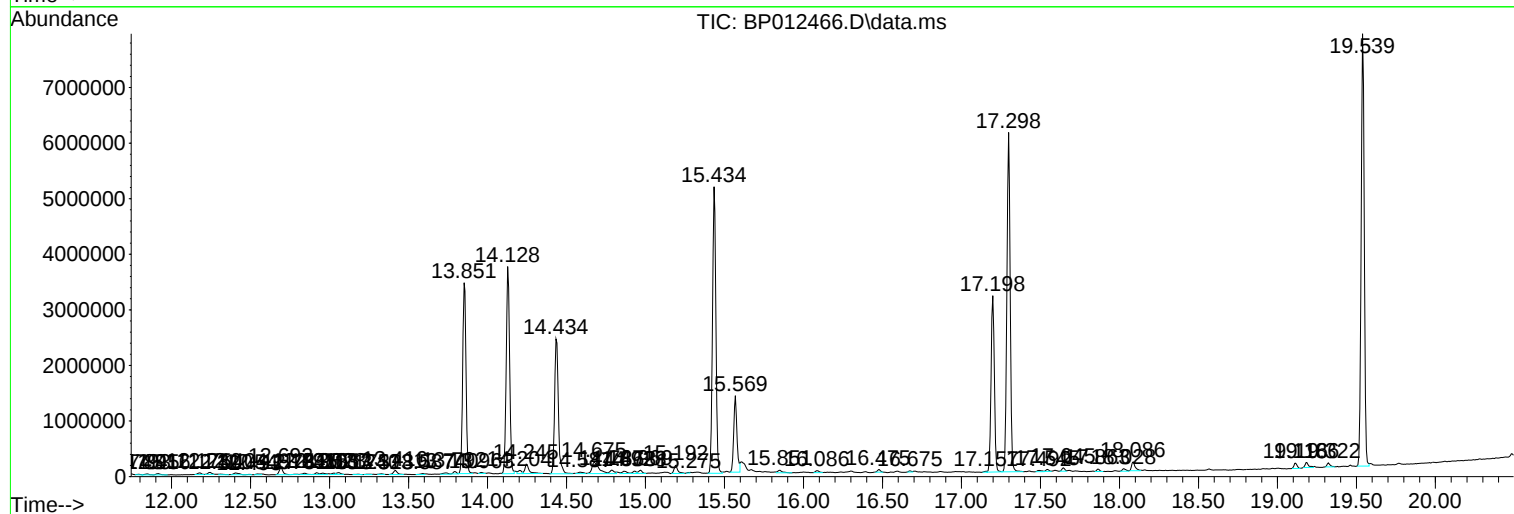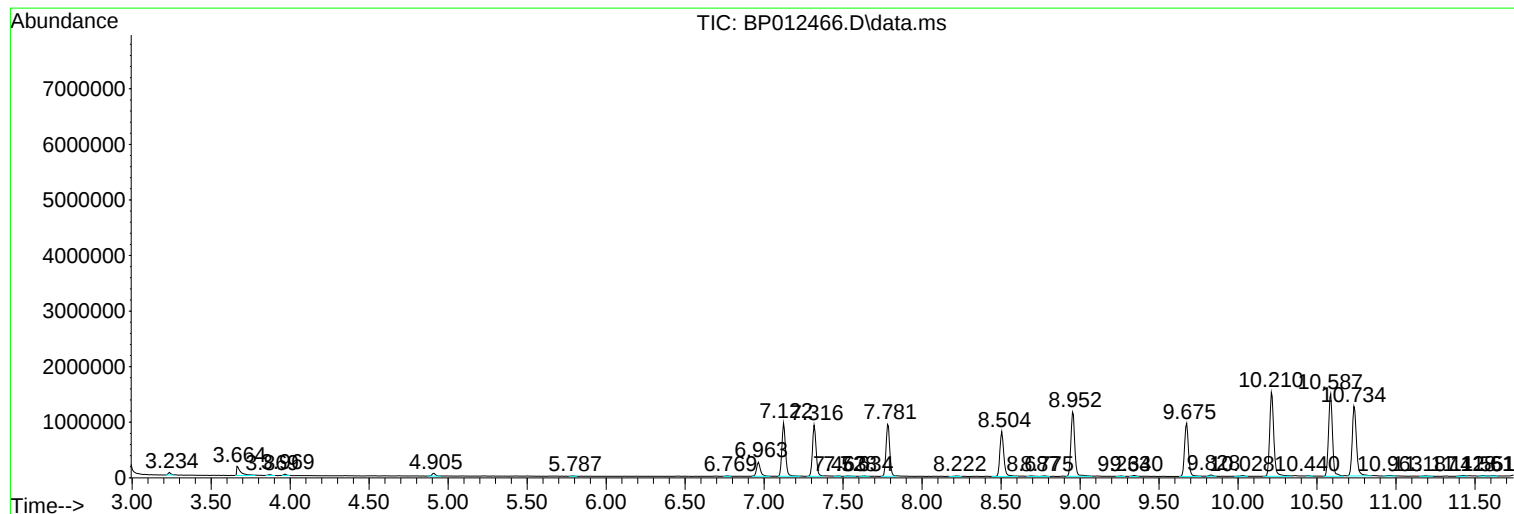

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP110222\
Data File : BP012466.D
Acq On : 03 Nov 2022 00:02
Operator : CG/JU
Sample : N5300-13
Misc :
ALS Vial : 20 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
BHA91

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP102522.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP110222\
Data File : BP012466.D
Acq On : 03 Nov 2022 00:02
Operator : CG/JU
Sample : N5300-13
Misc :
ALS Vial : 20 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
BHA91

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP102522.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST0.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc