

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP110222\
 Data File : BP012467.D
 Acq On : 03 Nov 2022 00:37
 Operator : CG/JU
 Sample : N5321-14
 Misc :
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DBWN8

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP102522.M
 Title : SVOA CALIBRATION

Signal : TIC: BP012467.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.199	32	36	39	rBV	52697	74422	0.71%	0.079%
2	3.234	39	42	47	rVB	53877	65140	0.62%	0.070%
3	3.658	112	114	135	rBV	277503	506808	4.84%	0.541%
4	3.869	146	150	159	rVB	22641	36235	0.35%	0.039%
5	3.969	163	167	173	rVB	20782	30867	0.30%	0.033%
6	4.911	319	327	333	rVB5	11117	22126	0.21%	0.024%
7	6.963	669	676	689	rBV	353015	613080	5.86%	0.655%
8	7.122	696	703	721	rBV	1090976	1748252	16.71%	1.867%
9	7.316	728	736	746	rBV	1076524	1774000	16.96%	1.894%
10	7.781	808	815	825	rBV	1058773	1755704	16.78%	1.875%
11	7.887	828	833	838	rVB4	17326	31470	0.30%	0.034%
12	8.504	930	938	954	rBV	1050501	1793686	17.15%	1.915%
13	8.952	1006	1014	1028	rBV	1273600	2230113	21.32%	2.381%
14	9.340	1074	1080	1085	rVB4	9977	19260	0.18%	0.021%
15	9.675	1129	1137	1150	rBV	1114703	1872362	17.90%	1.999%
16	10.210	1220	1228	1250	rBV	1738790	3147256	30.08%	3.361%
17	10.587	1284	1292	1309	rBV	1669527	2922859	27.94%	3.121%
18	10.734	1309	1317	1340	rBV	1528605	2815130	26.91%	3.006%
19	12.128	1541	1554	1558	rBV	34035	71267	0.68%	0.076%
20	12.181	1558	1563	1571	rVB2	27790	53237	0.51%	0.057%
21	12.481	1609	1614	1618	rBV7	6951	11541	0.11%	0.012%
22	13.057	1707	1712	1719	rBV2	32302	52696	0.50%	0.056%
23	13.163	1725	1730	1734	rBV3	11719	17213	0.16%	0.018%
24	13.245	1740	1744	1751	rVB8	9483	17357	0.17%	0.019%
25	13.328	1751	1758	1763	rBV2	16398	29381	0.28%	0.031%
26	13.404	1766	1771	1778	rVB5	7798	15848	0.15%	0.017%
27	13.639	1807	1811	1818	rBV8	10086	18201	0.17%	0.019%
28	13.857	1837	1848	1861	rBV	3451351	5093330	48.69%	5.439%
29	14.128	1885	1894	1908	rBV	3861176	5902321	56.42%	6.303%
30	14.228	1908	1911	1918	rVB8	17789	30226	0.29%	0.032%
31	14.434	1939	1946	1959	rBV	2779996	4262830	40.75%	4.552%
32	14.675	1981	1987	2006	rBV	243216	608343	5.82%	0.650%
33	15.192	2071	2075	2079	rBV	13790	19042	0.18%	0.020%
34	15.234	2079	2082	2085	rVV	12395	17171	0.16%	0.018%
35	15.275	2087	2089	2093	rVB4	9465	12309	0.12%	0.013%
36	15.386	2104	2108	2110	rBV2	18786	27654	0.26%	0.030%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP110222\
 Data File : BP012467.D
 Acq On : 03 Nov 2022 00:37
 Operator : CG/JU
 Sample : N5321-14
 Misc :
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DBWN8

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP102522.M
 Title : SVOA CALIBRATION

37	15.434	2110	2116	2133	rVV	5168024	7654051	73.17%	8.174%
38	15.569	2133	2139	2152	rVV	1666323	2399036	22.93%	2.562%
39	15.675	2153	2157	2165	rVB4	27397	56179	0.54%	0.060%
40	16.045	2217	2220	2226	rVB2	40128	52835	0.51%	0.056%
41	16.204	2243	2247	2256	rVB4	26791	62293	0.60%	0.067%
42	17.198	2410	2416	2426	rVB	3567766	5255661	50.24%	5.612%
43	17.298	2426	2433	2449	rBV	6111686	8675966	82.93%	9.265%
44	17.445	2456	2458	2462	rVB3	14125	16655	0.16%	0.018%
45	18.086	2562	2567	2575	rBV	140214	221108	2.11%	0.236%
46	18.616	2653	2657	2663	rVB2	58019	72307	0.69%	0.077%
47	19.110	2738	2741	2747	rBV	89556	124519	1.19%	0.133%
48	19.186	2750	2754	2759	rBV	88020	143039	1.37%	0.153%
49	19.322	2774	2777	2784	rBV	104463	149059	1.42%	0.159%
50	19.539	2808	2814	2827	rBV	7610325	10461279	100.00%	11.171%
51	20.998	3059	3062	3069	rVB2	136141	159252	1.52%	0.170%
52	21.292	3107	3112	3120	rBV	4578809	5820325	55.64%	6.215%
53	23.521	3484	3491	3503	rVB2	4668206	9426281	90.11%	10.066%
54	23.680	3511	3518	3529	rVB2	2550690	5175409	49.47%	5.527%




Sum of corrected areas: 93643991

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP110222\
Data File : BP012467.D
Acq On : 03 Nov 2022 00:37
Operator : CG/JU
Sample : N5321-14
Misc :
ALS Vial : 21 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DBWN8

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP102522.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

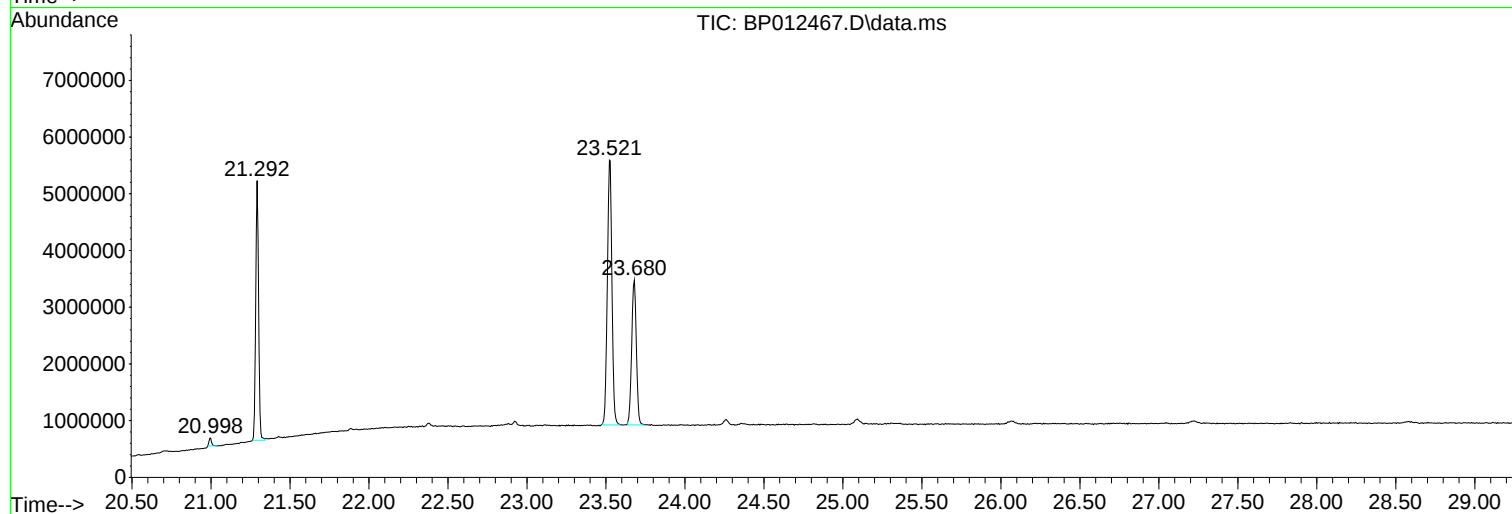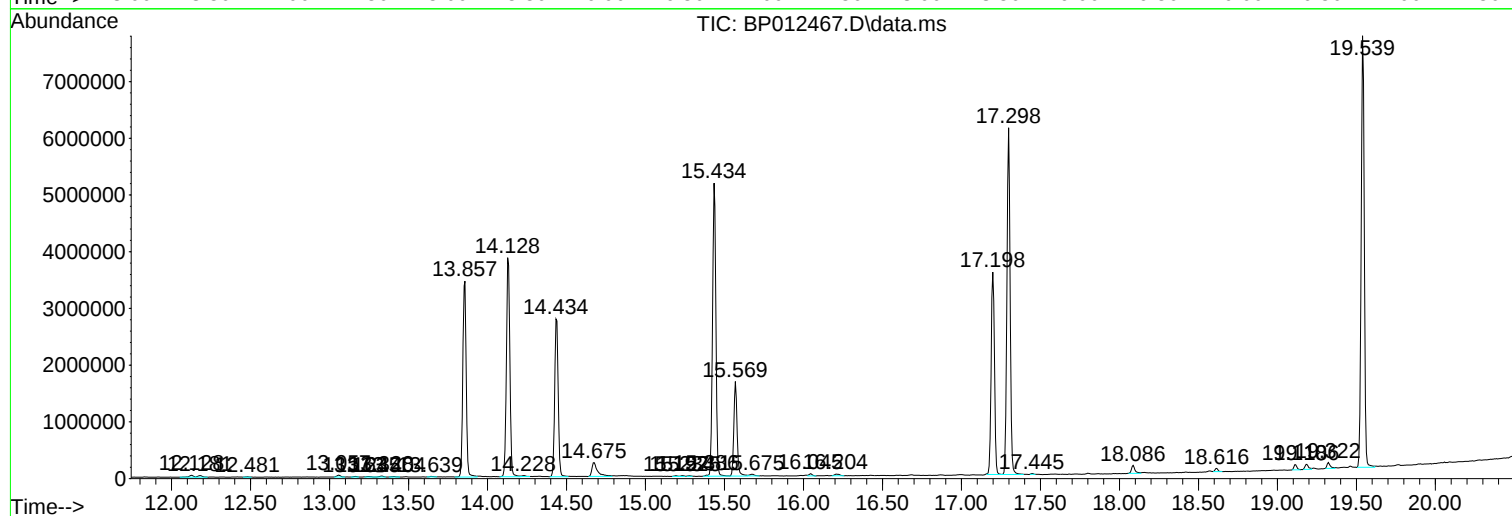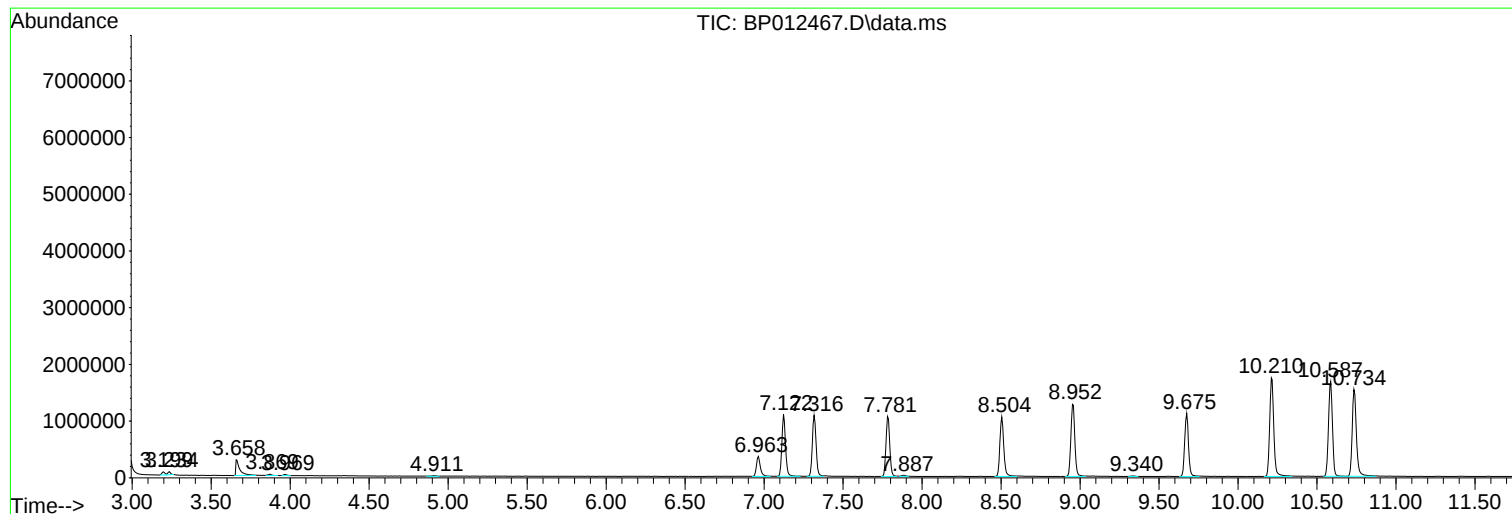

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP110222\
Data File : BP012467.D
Acq On : 03 Nov 2022 00:37
Operator : CG/JU
Sample : N5321-14
Misc :
ALS Vial : 21 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DBWN8

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP102522.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP110222\
Data File : BP012467.D
Acq On : 03 Nov 2022 00:37
Operator : CG/JU
Sample : N5321-14
Misc :
ALS Vial : 21 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DBWN8

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP102522.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST0.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc