

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP110222\
 Data File : BP012468.D
 Acq On : 03 Nov 2022 01:11
 Operator : CG/JU
 Sample : N5321-15
 Misc :
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DBWP4

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP102522.M
 Title : SVOA CALIBRATION

Signal : TIC: BP012468.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.234	38	42	49	rBV	54425	78256	0.77%	0.096%
2	3.664	113	115	133	rBV	266437	505976	4.98%	0.620%
3	3.870	146	150	155	rVB	17174	26581	0.26%	0.033%
4	3.970	163	167	174	rVB	17584	27262	0.27%	0.033%
5	6.964	670	676	687	rBV	244356	430652	4.24%	0.528%
6	7.122	696	703	717	rBV	920125	1512931	14.90%	1.854%
7	7.316	729	736	746	rBV	849081	1401570	13.80%	1.718%
8	7.781	808	815	826	rBV	866757	1427520	14.06%	1.750%
9	8.505	930	938	952	rBV	751554	1310705	12.91%	1.607%
10	8.952	1007	1014	1034	rBV	1118831	1920236	18.91%	2.354%
11	9.334	1074	1079	1088	rVB5	7552	14015	0.14%	0.017%
12	9.675	1130	1137	1155	rBV	891010	1515545	14.93%	1.858%
13	10.210	1221	1228	1252	rBV	1391861	2480091	24.43%	3.040%
14	10.587	1284	1292	1309	rVB	1339318	2342857	23.07%	2.872%
15	10.734	1309	1317	1341	rBV	1286373	2421877	23.85%	2.969%
16	12.181	1558	1563	1571	rBV	21004	41372	0.41%	0.051%
17	13.251	1734	1745	1750	rBV6	6925	16716	0.16%	0.020%
18	13.328	1753	1758	1762	rBV6	8540	13088	0.13%	0.016%
19	13.410	1765	1772	1776	rBV6	6721	14048	0.14%	0.017%
20	13.851	1841	1847	1862	rBV	3173661	4587147	45.18%	5.623%
21	14.128	1887	1894	1913	rBV	3473404	5142612	50.65%	6.304%
22	14.434	1939	1946	1957	rBV	2300304	3447274	33.95%	4.225%
23	14.675	1981	1987	2004	rBV	168034	447394	4.41%	0.548%
24	14.881	2019	2022	2029	rVB7	16291	25008	0.25%	0.031%
25	15.434	2109	2116	2133	rBV	4889063	6988772	68.83%	8.566%
26	15.569	2133	2139	2150	rVV	1452542	2058595	20.27%	2.523%
27	15.669	2154	2156	2162	rVB3	23083	36277	0.36%	0.044%
28	16.457	2287	2290	2295	rVB3	9952	12467	0.12%	0.015%
29	16.869	2357	2360	2367	rBV9	7286	14364	0.14%	0.018%
30	17.198	2409	2416	2426	rBV	3079675	4399706	43.33%	5.393%
31	17.298	2426	2433	2449	rVV2	5626649	8283185	81.58%	10.153%
32	18.087	2563	2567	2575	rBV	80938	130517	1.29%	0.160%
33	19.116	2738	2742	2747	rBV	80543	107640	1.06%	0.132%
34	19.186	2750	2754	2757	rBV	84457	113587	1.12%	0.139%
35	19.322	2774	2777	2781	rBV3	69355	93136	0.92%	0.114%
36	19.539	2808	2814	2830	rBV	7549791	10153442	100.00%	12.446%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP110222\
Data File : BP012468.D
Acq On : 03 Nov 2022 01:11
Operator : CG/JU
Sample : N5321-15
Misc :
ALS Vial : 22 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DBWP4

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP102522.M
Title : SVOA CALIBRATION

37	21.292	3107	3112	3118	rBV	3846143	4811110	47.38%	5.897%
38	23.522	3484	3491	3504	rVB2	4486227	9005680	88.70%	11.039%
39	23.674	3511	3517	3528	rVB2	2155896	4223561	41.60%	5.177%




Sum of corrected areas: 81582772

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP110222\
Data File : BP012468.D
Acq On : 03 Nov 2022 01:11
Operator : CG/JU
Sample : N5321-15
Misc :
ALS Vial : 22 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DBWP4

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP102522.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

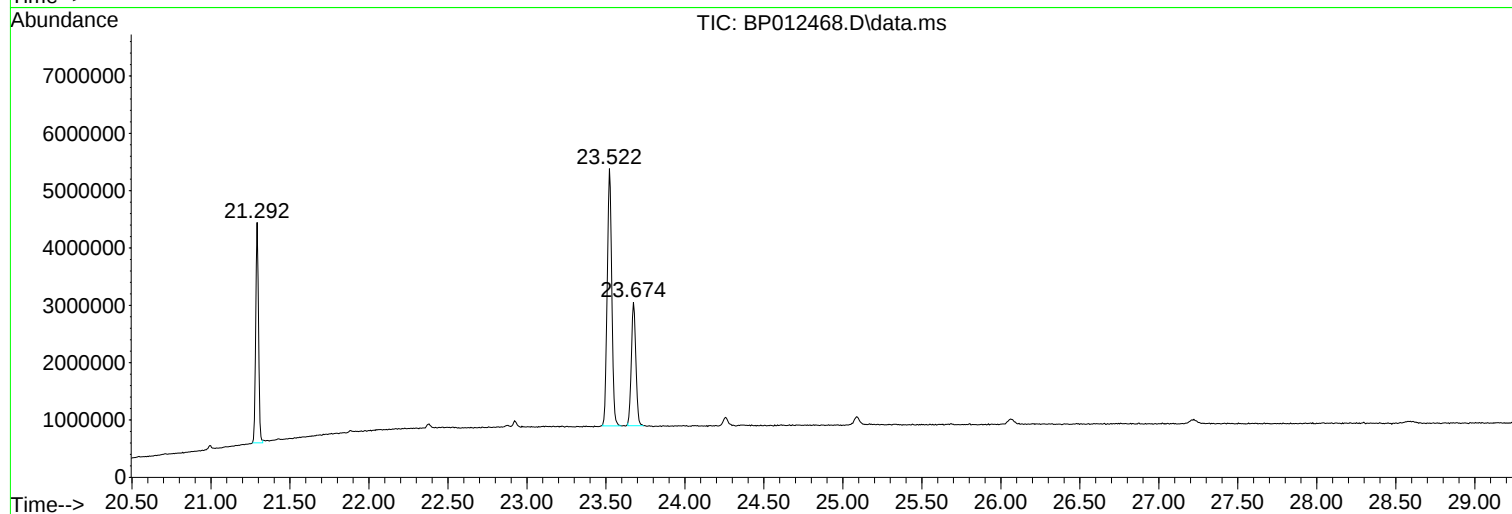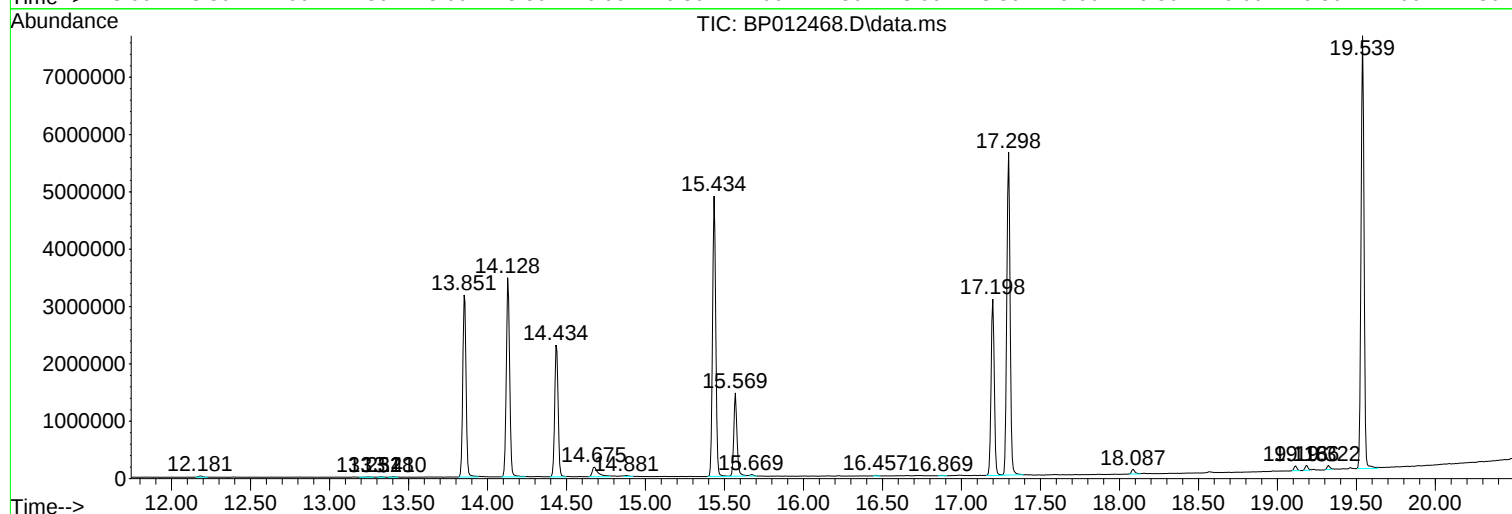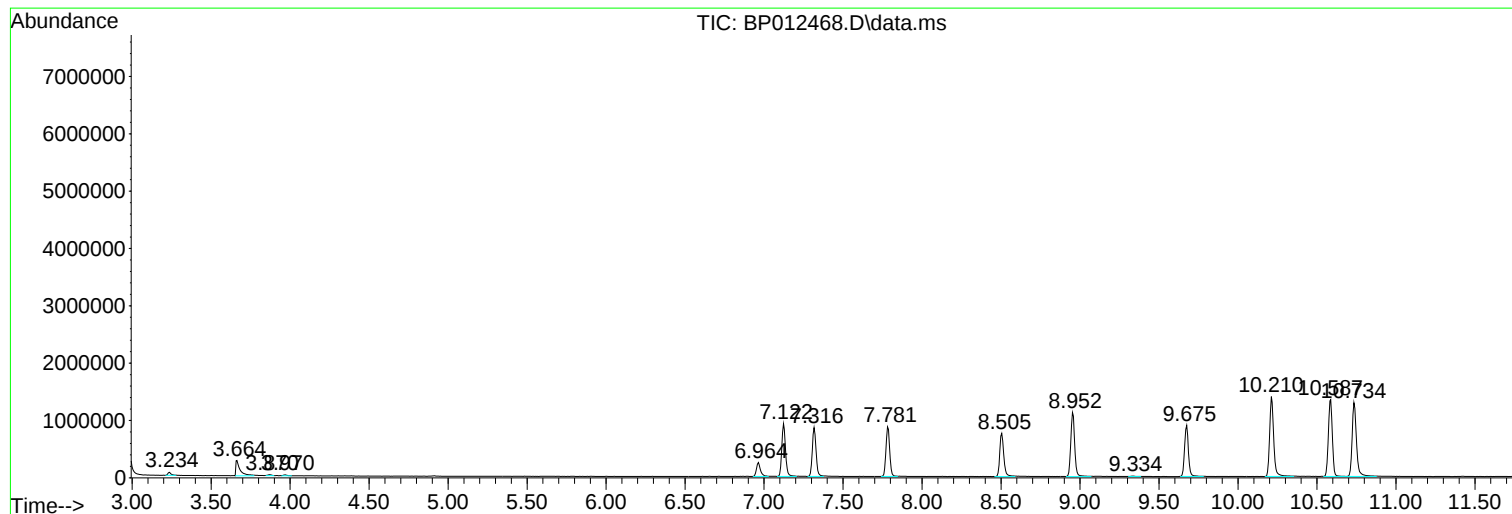

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP110222\
Data File : BP012468.D
Acq On : 03 Nov 2022 01:11
Operator : CG/JU
Sample : N5321-15
Misc :
ALS Vial : 22 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DBWP4

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP102522.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP110222\
Data File : BP012468.D
Acq On : 03 Nov 2022 01:11
Operator : CG/JU
Sample : N5321-15
Misc :
ALS Vial : 22 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DBWP4

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP102522.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST0.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc