

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP110222\
 Data File : BP012469.D
 Acq On : 03 Nov 2022 01:46
 Operator : CG/JU
 Sample : N5321-16
 Misc :
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DBWP5

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP102522.M
 Title : SVOA CALIBRATION

Signal : TIC: BP012469.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.234	38	42	53	rVB	53738	83704	0.77%	0.088%
2	3.664	112	115	131	rBV	266100	482933	4.43%	0.505%
3	3.870	145	150	154	rBV	18740	30545	0.28%	0.032%
4	3.970	163	167	174	rVB	19872	31645	0.29%	0.033%
5	4.911	323	327	330	rBV2	10145	13695	0.13%	0.014%
6	6.964	669	676	691	rVB	333117	568623	5.21%	0.595%
7	7.122	697	703	722	rBV	1055945	1714369	15.71%	1.793%
8	7.316	729	736	746	rBV	1055199	1709339	15.66%	1.788%
9	7.516	765	770	777	rVB7	16388	26953	0.25%	0.028%
10	7.781	807	815	822	rBV	1013922	1658868	15.20%	1.735%
11	7.846	822	826	839	rVB	70780	130660	1.20%	0.137%
12	8.505	928	938	957	rBV	1001952	1719617	15.76%	1.798%
13	8.893	998	1004	1007	rBV3	10826	16496	0.15%	0.017%
14	8.952	1007	1014	1031	rVV	1275709	2179584	19.97%	2.279%
15	9.334	1074	1079	1085	rBV3	19025	31139	0.29%	0.033%
16	9.675	1128	1137	1151	rBV	1066767	1844188	16.90%	1.929%
17	10.210	1220	1228	1245	rBV	1713666	3093931	28.35%	3.236%
18	10.587	1282	1292	1304	rBV	1582129	2739608	25.10%	2.865%
19	10.734	1310	1317	1336	rBV	1434621	2634497	24.14%	2.755%
20	11.269	1403	1408	1409	rBV4	8703	14670	0.13%	0.015%
21	11.304	1409	1414	1424	rVV	135122	224130	2.05%	0.234%
22	11.828	1498	1503	1512	rVB4	10228	21911	0.20%	0.023%
23	12.181	1557	1563	1572	rVB	27230	50729	0.46%	0.053%
24	12.787	1660	1666	1670	rBV2	11813	20218	0.19%	0.021%
25	12.963	1690	1696	1704	rBV2	30348	59339	0.54%	0.062%
26	13.251	1735	1745	1748	rBV5	17606	35520	0.33%	0.037%
27	13.328	1753	1758	1763	rVB3	21454	36710	0.34%	0.038%
28	13.398	1768	1770	1779	rVB5	8647	15271	0.14%	0.016%
29	13.851	1841	1847	1860	rVV	3581012	5170468	47.38%	5.407%
30	14.128	1887	1894	1912	rBV	3937231	5975333	54.76%	6.249%
31	14.434	1939	1946	1964	rBV	2679856	4054629	37.15%	4.240%
32	14.669	1980	1986	2004	rBV	280206	653073	5.98%	0.683%
33	15.192	2070	2075	2078	rBV	27241	38057	0.35%	0.040%
34	15.269	2083	2088	2093	rVB	43821	68261	0.63%	0.071%
35	15.434	2109	2116	2131	rBV	5303306	7882181	72.23%	8.243%
36	15.569	2132	2139	2148	rBV	1720640	2525049	23.14%	2.641%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP110222\
 Data File : BP012469.D
 Acq On : 03 Nov 2022 01:46
 Operator : CG/JU
 Sample : N5321-16
 Misc :
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DBWP5

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP102522.M
 Title : SVOA CALIBRATION

37	15.657	2149	2154	2162	rVB2	148513	261858	2.40%	0.274%
38	16.151	2233	2238	2245	rBV5	22085	50906	0.47%	0.053%
39	16.457	2284	2290	2297	rBV	193750	284298	2.61%	0.297%
40	16.604	2310	2315	2319	rBV8	12878	22785	0.21%	0.024%
41	16.651	2319	2323	2328	rBV2	63605	84829	0.78%	0.089%
42	16.798	2344	2348	2351	rVB5	19551	26949	0.25%	0.028%
43	16.957	2371	2375	2380	rBV5	24901	45958	0.42%	0.048%
44	17.198	2409	2416	2425	rBV	3436406	5074115	46.50%	5.306%
45	17.298	2426	2433	2448	rVV	6419135	9217905	84.47%	9.640%
46	17.486	2462	2465	2470	rVB	26233	31908	0.29%	0.033%
47	17.681	2495	2498	2503	rBV	32162	47940	0.44%	0.050%
48	18.039	2555	2559	2562	rBV3	71591	106931	0.98%	0.112%
49	18.086	2563	2567	2577	rVB	176686	302783	2.77%	0.317%
50	18.316	2600	2606	2611	rBV7	50584	117017	1.07%	0.122%
51	18.404	2618	2621	2626	rBV6	39518	57397	0.53%	0.060%
52	18.457	2626	2630	2646	rVV6	83948	323961	2.97%	0.339%
53	18.628	2656	2659	2668	rVB10	38202	77747	0.71%	0.081%
54	18.945	2709	2713	2720	rBV2	137665	257119	2.36%	0.269%
55	19.110	2738	2741	2748	rBV2	93127	124116	1.14%	0.130%
56	19.181	2750	2753	2759	rBV	95195	137593	1.26%	0.144%
57	19.322	2774	2777	2789	rBV2	114312	171367	1.57%	0.179%
58	19.539	2808	2814	2824	rBV	8202391	10912779	100.00%	11.412%
59	20.992	3058	3061	3068	rBV3	173568	271346	2.49%	0.284%
60	21.292	3107	3112	3122	rBV	4326280	5545766	50.82%	5.800%
61	23.521	3484	3491	3503	rVB2	4727009	9727210	89.14%	10.172%
62	23.674	3511	3517	3527	rVB2	2410633	4784158	43.84%	5.003%




Sum of corrected areas: 95622684

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP110222\
Data File : BP012469.D
Acq On : 03 Nov 2022 01:46
Operator : CG/JU
Sample : N5321-16
Misc :
ALS Vial : 23 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DBWP5

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP102522.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

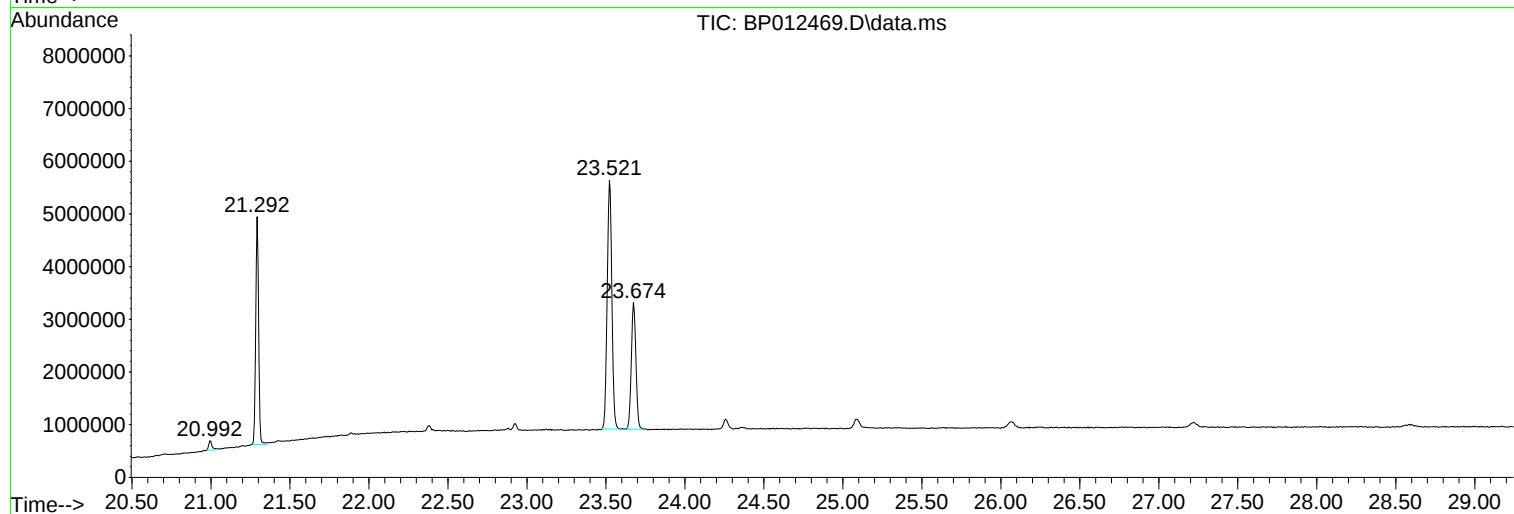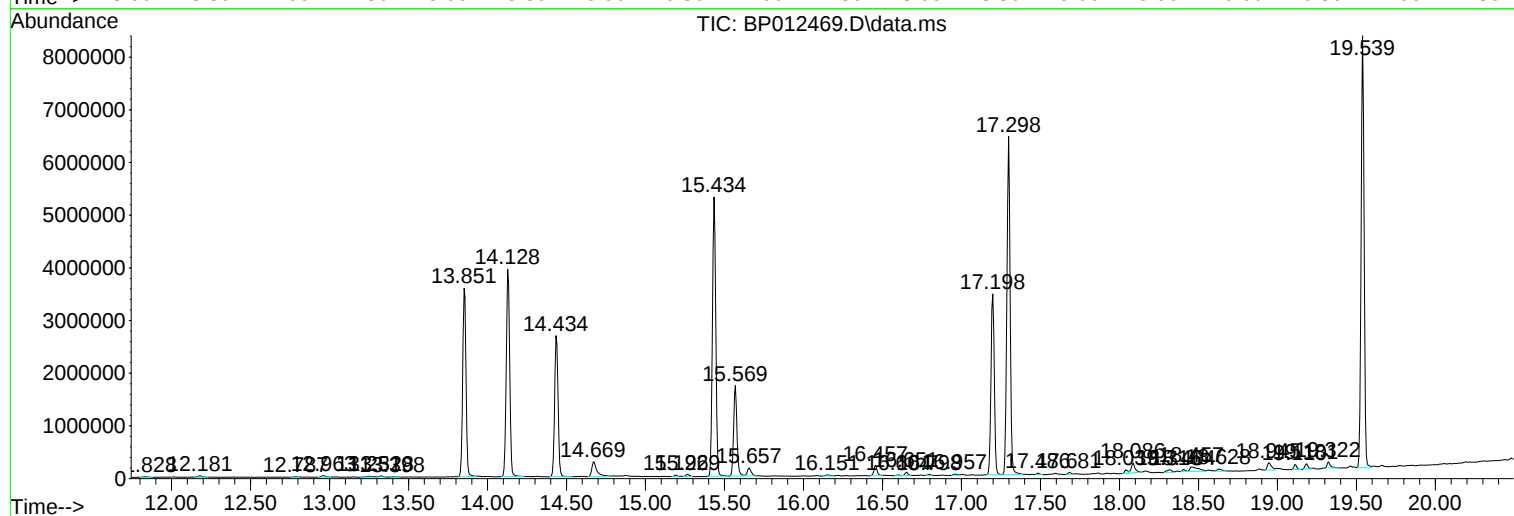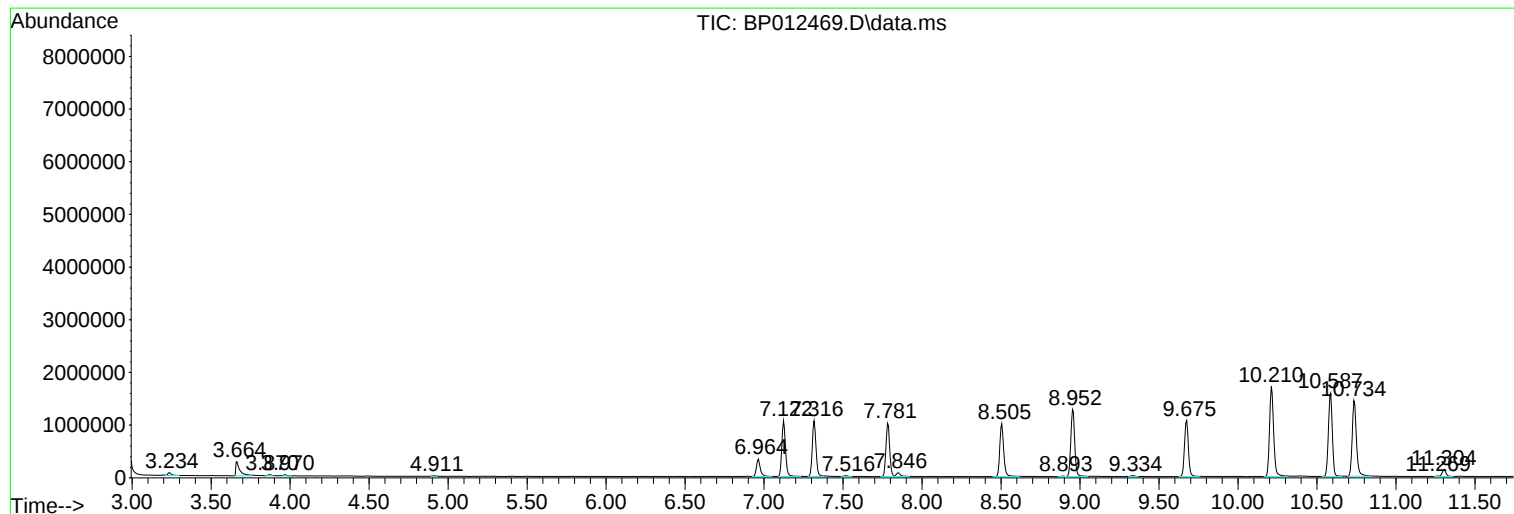

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP110222\
Data File : BP012469.D
Acq On : 03 Nov 2022 01:46
Operator : CG/JU
Sample : N5321-16
Misc :
ALS Vial : 23 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DBWP5

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP102522.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP110222\
Data File : BP012469.D
Acq On : 03 Nov 2022 01:46
Operator : CG/JU
Sample : N5321-16
Misc :
ALS Vial : 23 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DBWP5

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP102522.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST0.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc