

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP110222\
 Data File : BP012470.D
 Acq On : 03 Nov 2022 02:20
 Operator : CG/JU
 Sample : N5321-17
 Misc :
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DBWP6

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP102522.M
 Title : SVOA CALIBRATION

Signal : TIC: BP012470.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.234	38	42	53	rVB	59503	93026	0.87%	0.104%
2	3.658	111	114	130	rBV	296156	542041	5.08%	0.603%
3	3.869	145	150	157	rVB2	20718	35737	0.33%	0.040%
4	3.969	161	167	175	rVB	115064	179997	1.69%	0.200%
5	4.911	323	327	332	rBV3	8372	12000	0.11%	0.013%
6	6.963	670	676	690	rBV	315498	555810	5.21%	0.619%
7	7.122	696	703	719	rBV	1138360	1816739	17.02%	2.022%
8	7.316	729	736	747	rBV	1064742	1731006	16.22%	1.927%
9	7.781	807	815	825	rBV	939991	1532749	14.36%	1.706%
10	8.504	930	938	950	rBV	977547	1663793	15.59%	1.852%
11	8.951	1007	1014	1027	rBV	1324257	2283410	21.39%	2.541%
12	9.334	1073	1079	1087	rVB2	14946	24810	0.23%	0.028%
13	9.675	1129	1137	1154	rBV	1084138	1862403	17.45%	2.073%
14	10.210	1219	1228	1252	rBV	1704830	3019053	28.28%	3.360%
15	10.581	1284	1291	1304	rBV	1435532	2490344	23.33%	2.772%
16	10.734	1310	1317	1340	rBV	1414791	2619934	24.54%	2.916%
17	11.257	1401	1406	1409	rBV3	9737	16933	0.16%	0.019%
18	11.304	1409	1414	1423	rVV	38015	67540	0.63%	0.075%
19	11.828	1498	1503	1508	rBV3	8889	15581	0.15%	0.017%
20	12.181	1558	1563	1574	rVB3	25981	50262	0.47%	0.056%
21	12.957	1691	1695	1702	rVB7	8310	15646	0.15%	0.017%
22	13.328	1753	1758	1764	rVB2	17475	29558	0.28%	0.033%
23	13.851	1839	1847	1861	rBV	3545765	5104732	47.82%	5.681%
24	14.128	1886	1894	1907	rBV	4005821	5977839	56.00%	6.653%
25	14.434	1939	1946	1963	rVB	2461776	3701858	34.68%	4.120%
26	14.669	1978	1986	2006	rBV	235615	592966	5.56%	0.660%
27	14.822	2008	2012	2017	rBV7	12274	23371	0.22%	0.026%
28	15.434	2109	2116	2130	rBV	5453817	7815486	73.22%	8.698%
29	15.569	2133	2139	2151	rVV	1565402	2293245	21.48%	2.552%
30	15.669	2151	2156	2165	rVB5	34591	77020	0.72%	0.086%
31	16.222	2247	2250	2255	rVB7	9439	12849	0.12%	0.014%
32	16.598	2310	2314	2319	rVB7	6765	11087	0.10%	0.012%
33	16.657	2319	2324	2328	rBV6	8015	13712	0.13%	0.015%
34	17.198	2409	2416	2425	rBV	3258816	4632530	43.40%	5.156%
35	17.298	2426	2433	2444	rBV	6144640	8881097	83.20%	9.884%
36	17.557	2474	2477	2480	rBV	11480	16023	0.15%	0.018%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP110222\
 Data File : BP012470.D
 Acq On : 03 Nov 2022 02:20
 Operator : CG/JU
 Sample : N5321-17
 Misc :
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DBWP6

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP102522.M
 Title : SVOA CALIBRATION

37	18.086	2562	2567	2575	rBV	133568	205105	1.92%	0.228%
38	18.480	2631	2634	2637	rBV2	22815	38150	0.36%	0.042%
39	19.116	2738	2742	2747	rVB2	85128	112395	1.05%	0.125%
40	19.186	2749	2754	2758	rBV	97817	147018	1.38%	0.164%
41	19.322	2773	2777	2783	rBV3	108178	167544	1.57%	0.186%
42	19.539	2808	2814	2827	rBV	8040837	10674366	100.00%	11.880%
43	21.292	3107	3112	3118	rBV	3931318	4953875	46.41%	5.514%
44	23.521	3484	3491	3501	rVB2	4623940	9392226	87.99%	10.453%
45	23.674	3511	3517	3530	rVB2	2170433	4346328	40.72%	4.837%




Sum of corrected areas: 89849194

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP110222\
Data File : BP012470.D
Acq On : 03 Nov 2022 02:20
Operator : CG/JU
Sample : N5321-17
Misc :
ALS Vial : 24 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DBWP6

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP102522.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

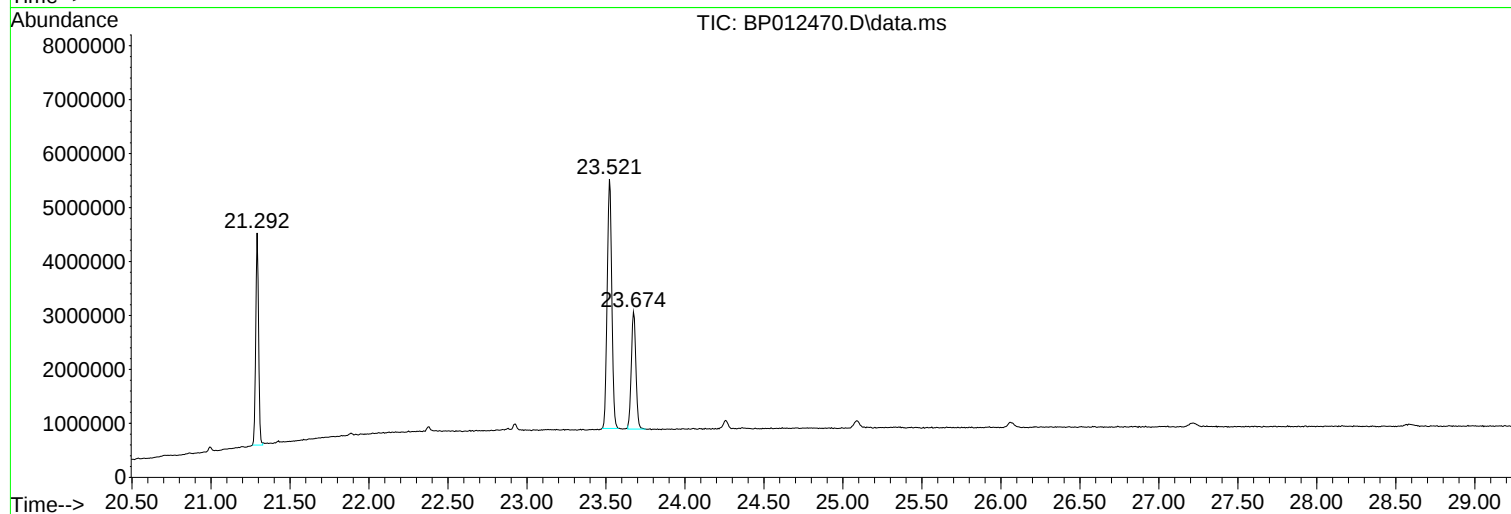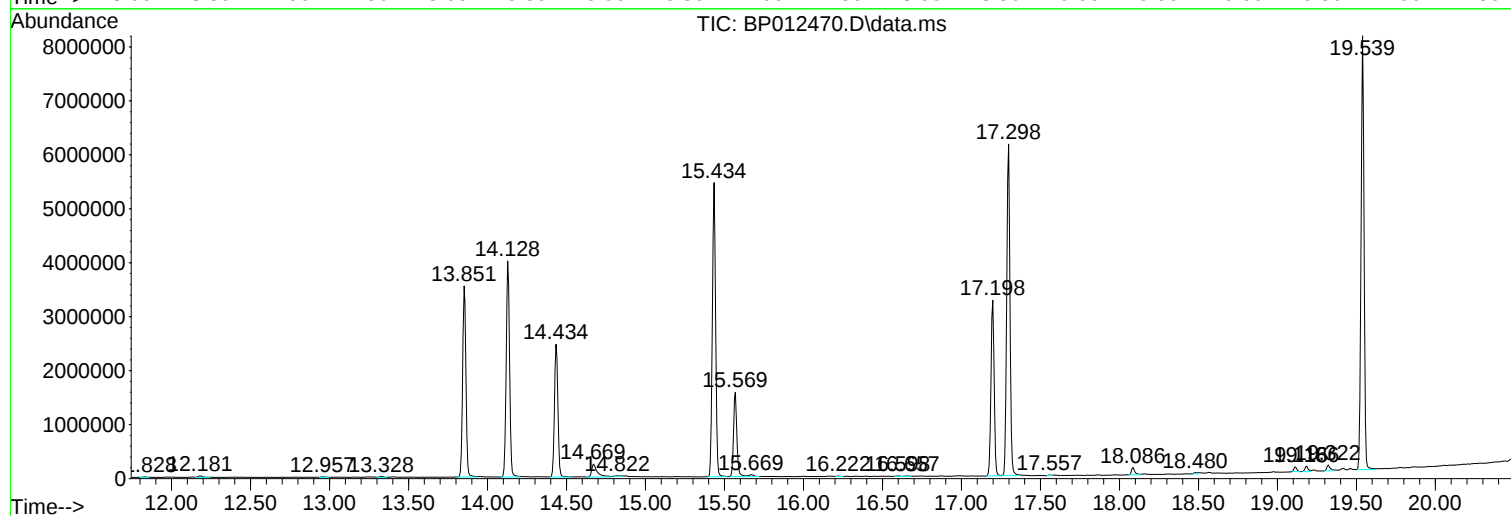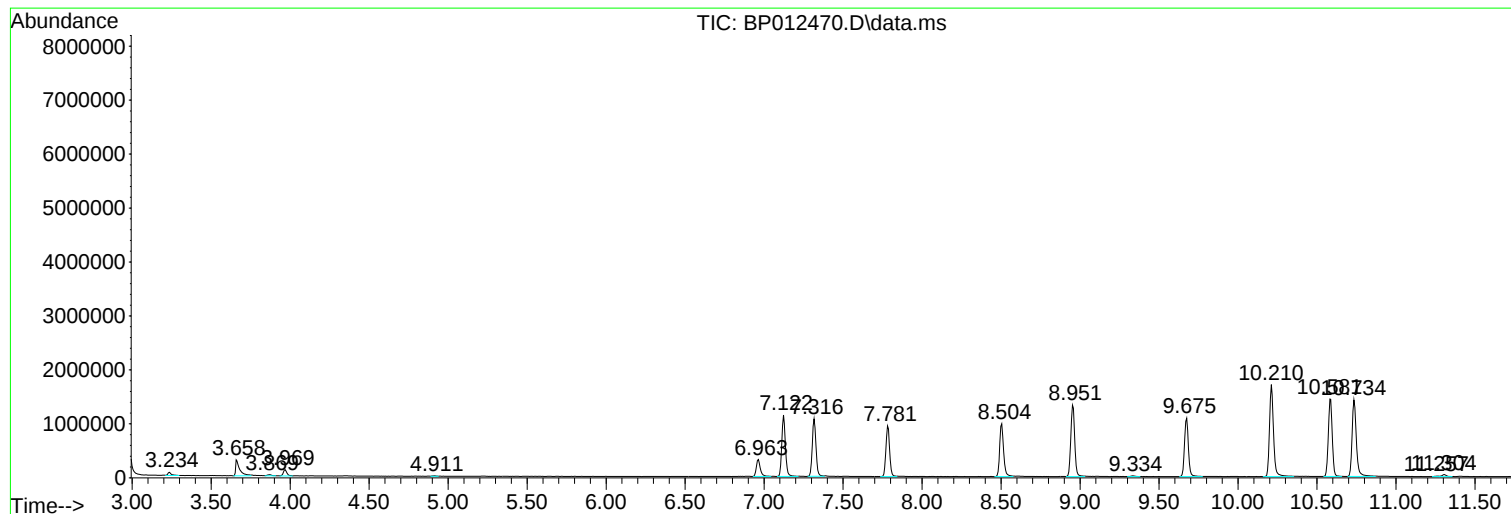

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP110222\
Data File : BP012470.D
Acq On : 03 Nov 2022 02:20
Operator : CG/JU
Sample : N5321-17
Misc :
ALS Vial : 24 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DBWP6

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP102522.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP110222\
Data File : BP012470.D
Acq On : 03 Nov 2022 02:20
Operator : CG/JU
Sample : N5321-17
Misc :
ALS Vial : 24 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DBWP6

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP102522.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc