

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP110222\
 Data File : BP012476.D
 Acq On : 03 Nov 2022 06:19
 Operator : CG/JU
 Sample : PB148676BL
 Misc :
 ALS Vial : 31 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SBLK676

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP102522.M
 Title : SVOA CALIBRATION

Signal : TIC: BP012476.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.234	38	42	51	rVB	73926	105567	1.15%	0.117%
2	3.652	111	113	136	rBV	551091	1003442	10.97%	1.111%
3	3.964	163	166	171	rBV	16974	24458	0.27%	0.027%
4	6.958	667	675	696	rBV	1270533	2107886	23.05%	2.334%
5	7.122	696	703	721	rVB	1038883	1680078	18.37%	1.860%
6	7.316	729	736	760	rVB	1208411	2043425	22.35%	2.263%
7	7.781	808	815	832	rBV	1130580	1843685	20.16%	2.041%
8	8.499	930	937	957	rBV	1628156	2789405	30.51%	3.089%
9	8.952	1005	1014	1030	rBV	1253378	2108463	23.06%	2.335%
10	9.669	1126	1136	1151	rBV	1058359	1816702	19.87%	2.012%
11	10.210	1221	1228	1250	rBV	1605010	2930903	32.06%	3.245%
12	10.581	1282	1291	1304	rBV	1732334	2984630	32.64%	3.305%
13	10.734	1309	1317	1340	rBV	962385	1852372	20.26%	2.051%
14	12.187	1557	1564	1572	rBV	22680	51434	0.56%	0.057%
15	13.163	1724	1730	1736	rBV6	7066	14818	0.16%	0.016%
16	13.228	1736	1741	1746	rBV9	5323	12270	0.13%	0.014%
17	13.328	1752	1758	1764	rVB5	14859	26695	0.29%	0.030%
18	13.398	1767	1770	1776	rBV6	5670	9552	0.10%	0.011%
19	13.851	1840	1847	1859	rBV	3187892	4457751	48.75%	4.936%
20	14.128	1886	1894	1911	rBV	3576457	5376474	58.80%	5.953%
21	14.434	1937	1946	1954	rBV	3057187	4422796	48.37%	4.897%
22	14.657	1978	1984	2013	rBV	1065382	2235526	24.45%	2.475%
23	15.075	2051	2055	2058	rBV6	5781	9156	0.10%	0.010%
24	15.434	2109	2116	2130	rBV	4619578	6885616	75.31%	7.624%
25	15.569	2132	2139	2152	rBV	989615	1515810	16.58%	1.678%
26	15.675	2153	2157	2161	rVB3	19550	29119	0.32%	0.032%
27	16.498	2293	2297	2302	rBV7	9006	15139	0.17%	0.017%
28	16.869	2356	2360	2366	rBV9	9114	14214	0.16%	0.016%
29	16.981	2377	2379	2387	rVB5	9192	15283	0.17%	0.017%
30	17.198	2408	2416	2426	rBV	3796993	5670127	62.01%	6.278%
31	17.292	2426	2432	2452	rVB2	5038073	7825542	85.59%	8.665%
32	18.092	2564	2568	2574	rBV7	15349	33355	0.36%	0.037%
33	18.363	2611	2614	2618	rVB5	11343	13909	0.15%	0.015%
34	19.110	2737	2741	2747	rBV	69192	105727	1.16%	0.117%
35	19.180	2749	2753	2757	rBV	65742	95748	1.05%	0.106%
36	19.539	2808	2814	2826	rBV	6570351	9143343	100.00%	10.124%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP110222\
Data File : BP012476.D
Acq On : 03 Nov 2022 06:19
Operator : CG/JU
Sample : PB148676BL
Misc :
ALS Vial : 31 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK676

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP102522.M
Title : SVOA CALIBRATION

37	21.292	3107	3112	3121	rBV	4639918	5944844	65.02%	6.583%
38	23.521	3484	3491	3504	rVB2	3766532	7915820	86.57%	8.765%
39	23.674	3510	3517	3531	rVB2	2541581	5181497	56.67%	5.737%




Sum of corrected areas: 90312581

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP110222\
Data File : BP012476.D
Acq On : 03 Nov 2022 06:19
Operator : CG/JU
Sample : PB148676BL
Misc :
ALS Vial : 31 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK676

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP102522.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

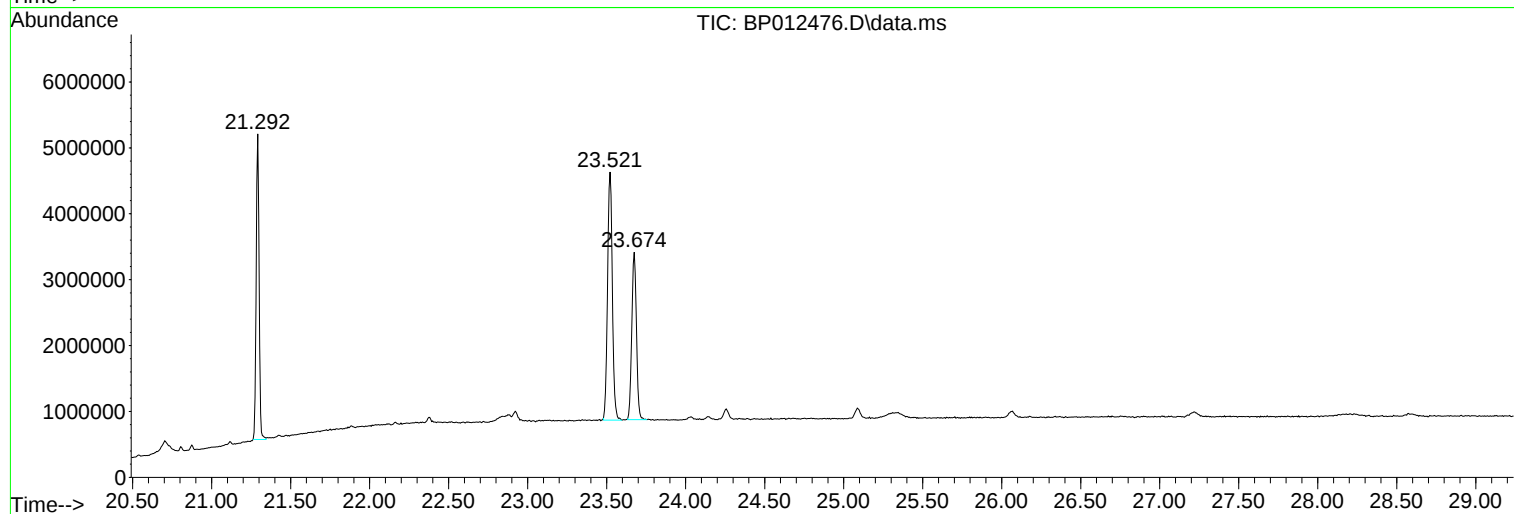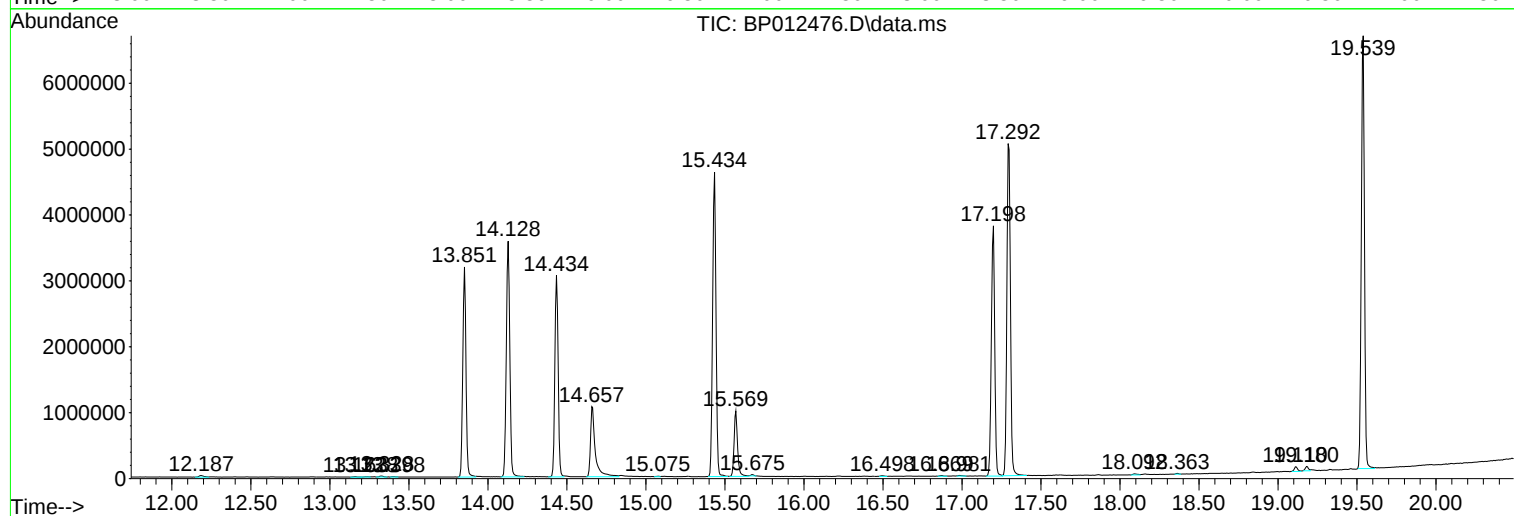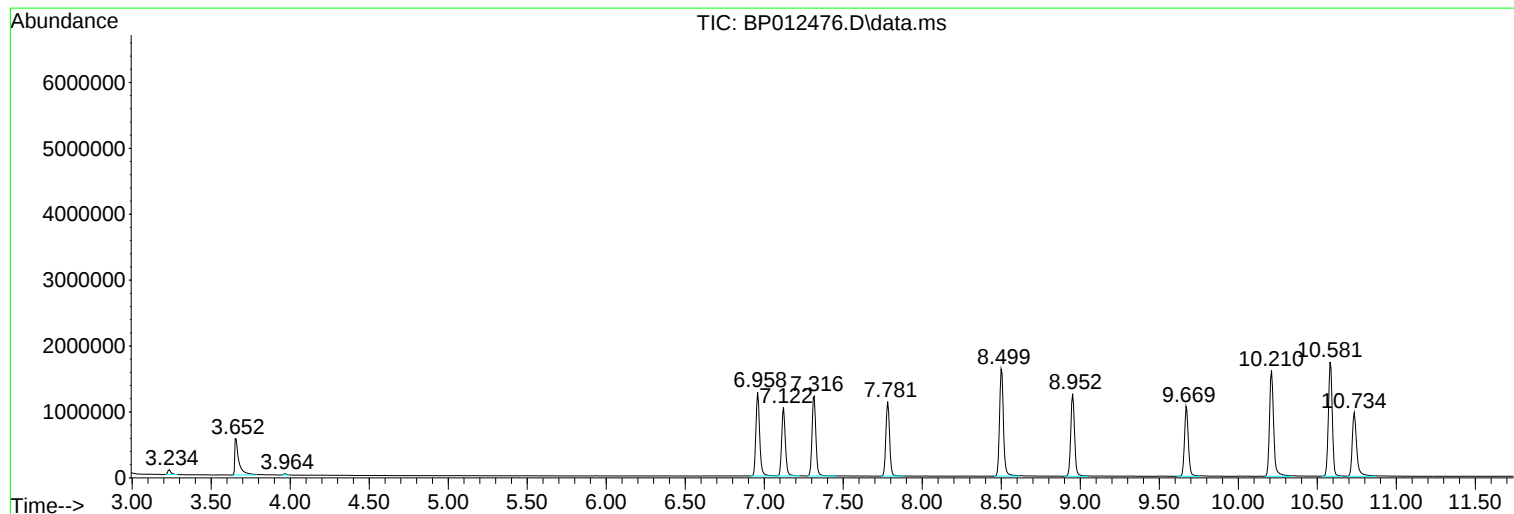

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP110222\
Data File : BP012476.D
Acq On : 03 Nov 2022 06:19
Operator : CG/JU
Sample : PB148676BL
Misc :
ALS Vial : 31 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK676

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP102522.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP110222\
Data File : BP012476.D
Acq On : 03 Nov 2022 06:19
Operator : CG/JU
Sample : PB148676BL
Misc :
ALS Vial : 31 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK676

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP102522.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST0.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc