

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP110222\
 Data File : BP012477.D
 Acq On : 03 Nov 2022 06:53
 Operator : CG/JU
 Sample : PB148677BL
 Misc :
 ALS Vial : 32 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SBLK677

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP102522.M
 Title : SVOA CALIBRATION

Signal : TIC: BP012477.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.234	38	42	53	rVB	75029	113578	1.31%	0.129%
2	3.658	112	114	128	rBV	489691	843777	9.72%	0.961%
3	3.964	163	166	174	rVB	25281	38013	0.44%	0.043%
4	6.958	668	675	691	rBV	1195553	1992080	22.96%	2.270%
5	7.122	696	703	718	rVB	988699	1599787	18.43%	1.823%
6	7.310	728	735	749	rBV	1154754	1947333	22.44%	2.219%
7	7.781	807	815	829	rBV	1199441	1914044	22.06%	2.181%
8	8.499	929	937	954	rBV	1576517	2672581	30.80%	3.045%
9	8.952	1004	1014	1034	rBV	1178267	1992920	22.96%	2.271%
10	9.669	1128	1136	1157	rBV	980074	1712410	19.73%	1.951%
11	10.210	1216	1228	1246	rBV	1554174	2804871	32.32%	3.196%
12	10.581	1284	1291	1303	rBV	1808679	3069712	35.37%	3.498%
13	10.734	1309	1317	1347	rBV	1740182	3259371	37.56%	3.714%
14	12.187	1554	1564	1573	rVB2	21703	47912	0.55%	0.055%
15	13.322	1753	1757	1763	rVV3	12841	21594	0.25%	0.025%
16	13.398	1767	1770	1776	rVB4	5464	10052	0.12%	0.011%
17	13.851	1840	1847	1859	rBV	3050485	4210688	48.52%	4.798%
18	13.945	1861	1863	1870	rVB7	8461	12238	0.14%	0.014%
19	14.128	1886	1894	1911	rBV	3308067	5050103	58.19%	5.755%
20	14.434	1939	1946	1963	rBV	3089259	4571498	52.68%	5.209%
21	14.663	1978	1985	2005	rBV	933319	1974377	22.75%	2.250%
22	15.116	2058	2062	2066	rVB7	5735	8813	0.10%	0.010%
23	15.434	2108	2116	2130	rBV	4367963	6521365	75.15%	7.431%
24	15.569	2132	2139	2153	rVV	881253	1317747	15.18%	1.502%
25	15.675	2153	2157	2165	rVB2	23759	41299	0.48%	0.047%
26	16.216	2245	2249	2256	rVB9	5564	9825	0.11%	0.011%
27	16.981	2375	2379	2384	rBV3	9463	15984	0.18%	0.018%
28	17.198	2409	2416	2426	rBV	3779214	5715833	65.86%	6.513%
29	17.292	2426	2432	2450	rVV2	5030063	7508149	86.52%	8.556%
30	17.863	2526	2529	2533	rBV5	10725	12886	0.15%	0.015%
31	19.116	2738	2742	2748	rBV3	66062	95988	1.11%	0.109%
32	19.180	2750	2753	2759	rVV	58032	86286	0.99%	0.098%
33	19.539	2808	2814	2826	rBV	6544754	8678135	100.00%	9.889%
34	21.292	3107	3112	3119	rBV	4389081	5676693	65.41%	6.469%
35	23.521	3484	3491	3504	rVB2	3469417	7365646	84.88%	8.393%
36	23.674	3510	3517	3528	rVB2	2364328	4844051	55.82%	5.520%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP110222\
Data File : BP012477.D
Acq On : 03 Nov 2022 06:53
Operator : CG/JU
Sample : PB148677BL
Misc :
ALS Vial : 32 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK677

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP102522.M
Title : SVOA CALIBRATION




Sum of corrected areas: 87757639

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP110222\
Data File : BP012477.D
Acq On : 03 Nov 2022 06:53
Operator : CG/JU
Sample : PB148677BL
Misc :
ALS Vial : 32 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK677

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP102522.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

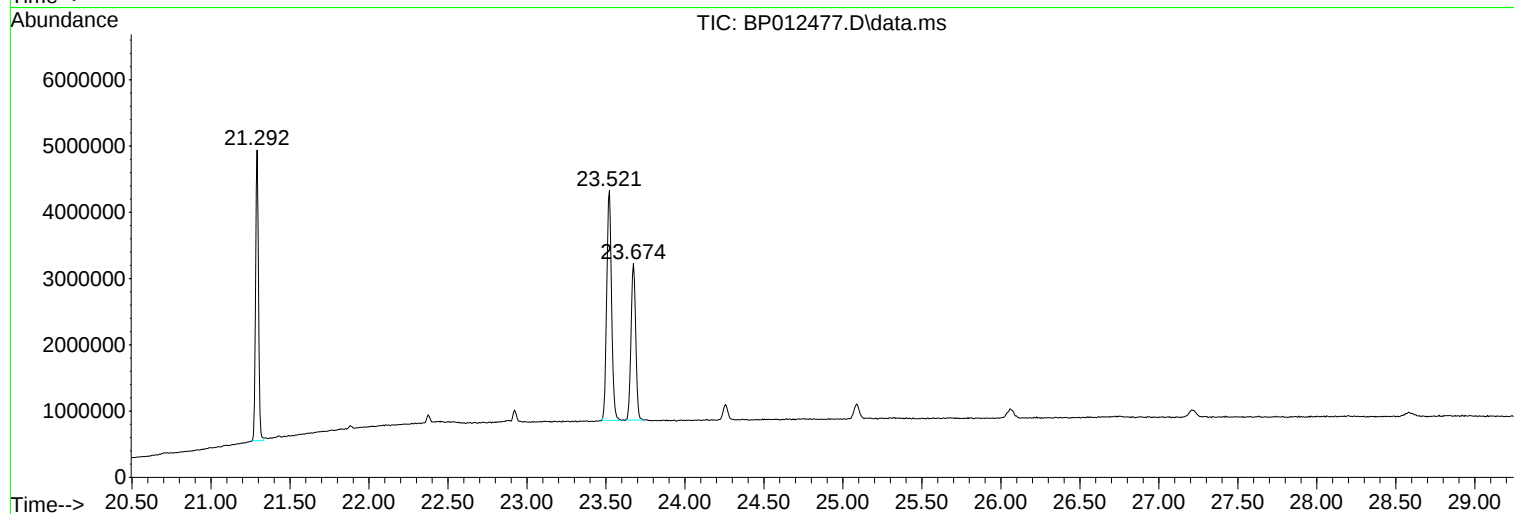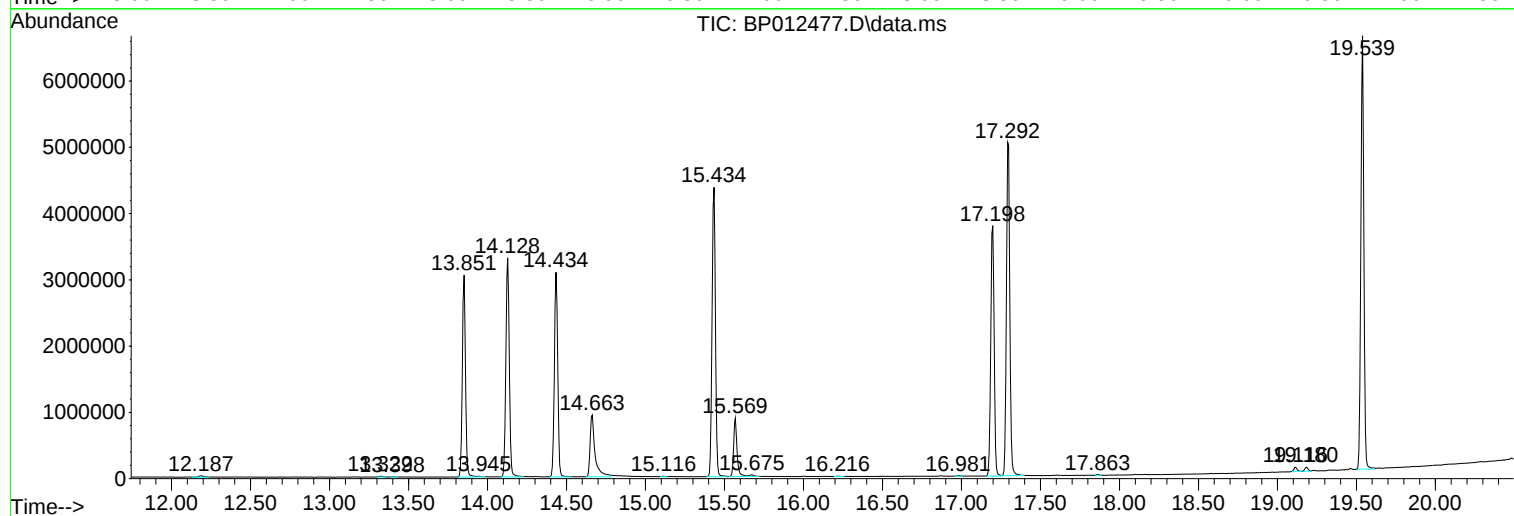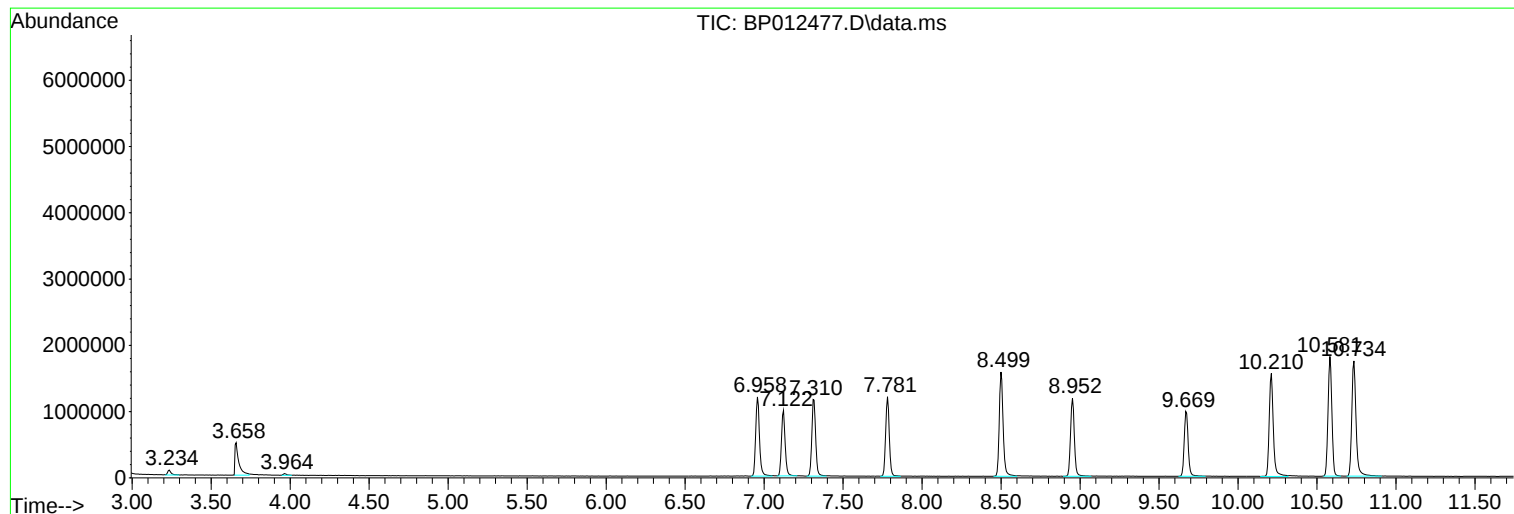

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP110222\
Data File : BP012477.D
Acq On : 03 Nov 2022 06:53
Operator : CG/JU
Sample : PB148677BL
Misc :
ALS Vial : 32 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK677

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP102522.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP110222\
Data File : BP012477.D
Acq On : 03 Nov 2022 06:53
Operator : CG/JU
Sample : PB148677BL
Misc :
ALS Vial : 32 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK677

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP102522.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST0.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc