

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP110222\
 Data File : BP012491.D
 Acq On : 03 Nov 2022 16:03
 Operator : CG/JU
 Sample : PB148620BL
 Misc :
 ALS Vial : 47 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SBLK620

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP102522.M
 Title : SVOA CALIBRATION

Signal : TIC: BP012491.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.234	38	42	50	rVB	72570	101347	1.24%	0.133%
2	3.658	111	114	129	rBV	429556	762022	9.34%	1.003%
3	3.969	162	167	171	rBV2	16961	25708	0.32%	0.034%
4	6.957	668	675	696	rBV	1101617	1898874	23.27%	2.499%
5	7.122	696	703	718	rVV	930387	1502464	18.41%	1.977%
6	7.316	729	736	754	rBV	1106171	1822279	22.33%	2.398%
7	7.781	808	815	830	rBV	860170	1379198	16.90%	1.815%
8	8.504	931	938	960	rBV	1439284	2518889	30.87%	3.315%
9	8.952	1006	1014	1034	rBV	1090803	1866521	22.87%	2.457%
10	9.675	1129	1137	1154	rBV	922408	1599966	19.61%	2.106%
11	10.210	1220	1228	1245	rBV	1383240	2577519	31.59%	3.392%
12	10.581	1283	1291	1307	rBV	1291651	2281671	27.96%	3.003%
13	10.734	1310	1317	1343	rBV	729775	1505375	18.45%	1.981%
14	12.193	1556	1565	1571	rBV2	17880	41109	0.50%	0.054%
15	13.404	1766	1771	1778	rVB6	4508	10176	0.12%	0.013%
16	13.851	1840	1847	1860	rBV	2765258	3972411	48.68%	5.228%
17	14.128	1887	1894	1911	rBV	3186378	4745678	58.16%	6.246%
18	14.434	1939	1946	1960	rBV	2184292	3379951	41.42%	4.448%
19	14.663	1978	1985	2014	rBV	815435	1892709	23.19%	2.491%
20	15.434	2109	2116	2129	rBV	4245602	6149686	75.36%	8.094%
21	15.569	2133	2139	2153	rVV	1006077	1527610	18.72%	2.010%
22	15.669	2153	2156	2168	rVB2	25702	53364	0.65%	0.070%
23	16.228	2246	2251	2256	rVB8	5664	9540	0.12%	0.013%
24	16.986	2377	2380	2385	rBV3	6876	11418	0.14%	0.015%
25	17.198	2409	2416	2426	rBV	3104958	4300997	52.71%	5.661%
26	17.298	2426	2433	2452	rVV2	4701107	7039358	86.26%	9.264%
27	19.116	2738	2742	2747	rBV	60648	87300	1.07%	0.115%
28	19.186	2750	2754	2760	rBV	59755	87914	1.08%	0.116%
29	19.539	2808	2814	2829	rBV	6034590	8160186	100.00%	10.740%
30	21.292	3107	3112	3123	rBV	3183351	4386989	53.76%	5.774%
31	23.527	3485	3492	3508	rVB2	3184246	6570167	80.51%	8.647%
32	23.680	3512	3518	3533	rVB	1864753	3713884	45.51%	4.888%




Sum of corrected areas: 75982280

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP110222\
Data File : BP012491.D
Acq On : 03 Nov 2022 16:03
Operator : CG/JU
Sample : PB148620BL
Misc :
ALS Vial : 47 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK620

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP102522.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

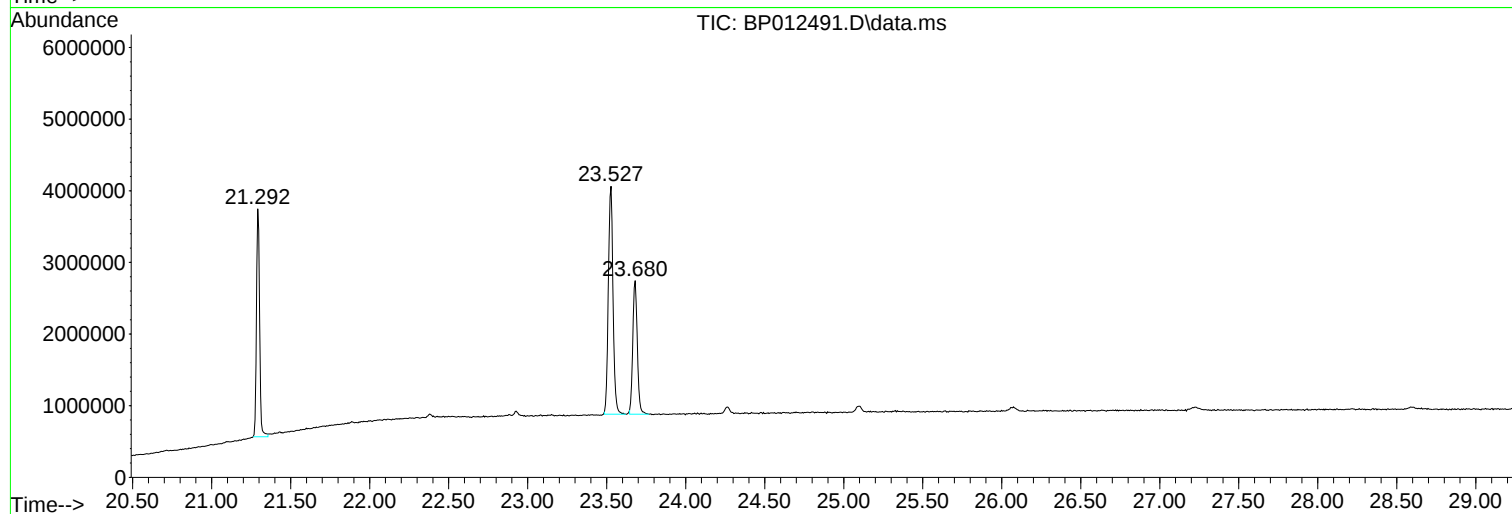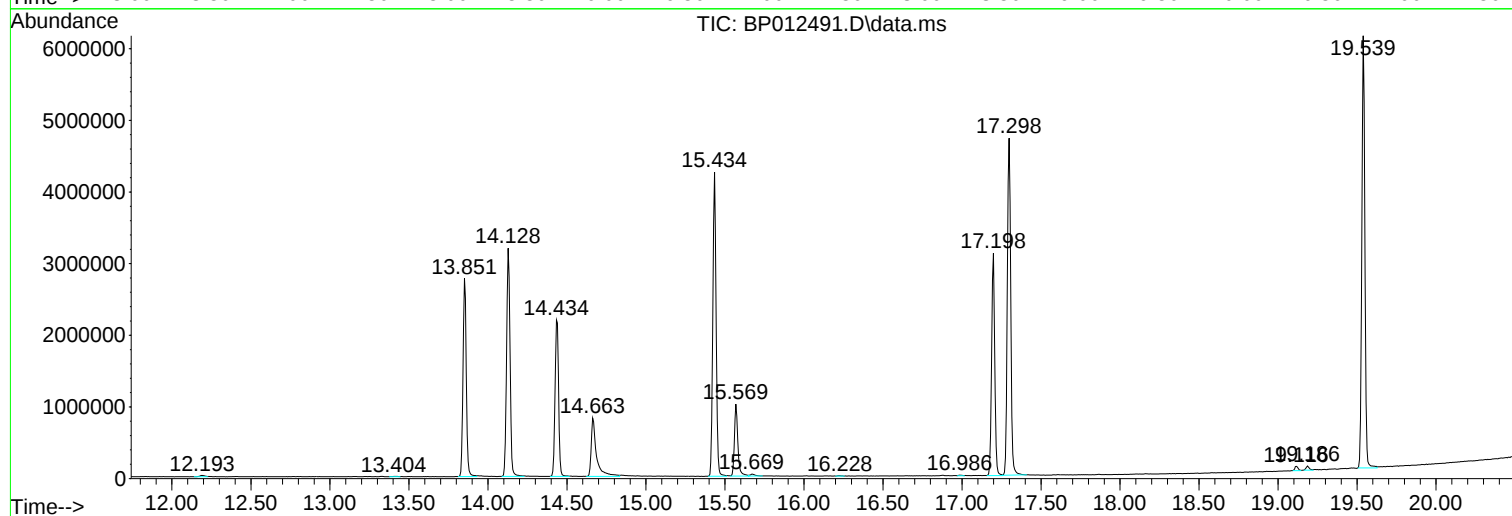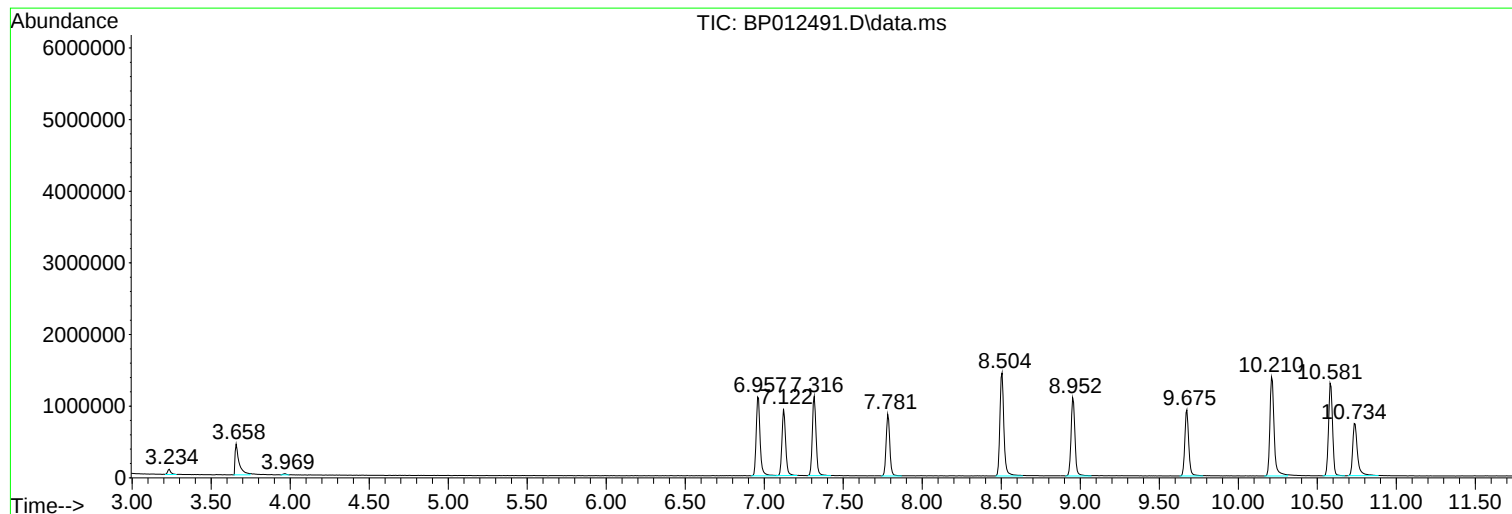

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP110222\
Data File : BP012491.D
Acq On : 03 Nov 2022 16:03
Operator : CG/JU
Sample : PB148620BL
Misc :
ALS Vial : 47 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK620

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP102522.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP110222\
Data File : BP012491.D
Acq On : 03 Nov 2022 16:03
Operator : CG/JU
Sample : PB148620BL
Misc :
ALS Vial : 47 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK620

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP102522.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST0.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc