

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP110222\
 Data File : BP012499.D
 Acq On : 03 Nov 2022 20:42
 Operator : CG/JU
 Sample : N5319-01
 Misc :
 ALS Vial : 55 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 BHA96

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP102522.M
 Title : SVOA CALIBRATION

Signal : TIC: BP012499.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.234	38	42	52	rVB	38706	59999	0.72%	0.083%
2	3.522	87	91	103	rBV	52328	98855	1.19%	0.138%
3	3.663	113	115	131	rBV	156576	299945	3.62%	0.417%
4	3.863	146	149	154	rVB2	12670	18526	0.22%	0.026%
5	3.963	162	166	172	rVB	26848	40899	0.49%	0.057%
6	6.963	669	676	689	rBV	189347	347167	4.19%	0.483%
7	7.122	696	703	719	rBV	757648	1267789	15.32%	1.764%
8	7.316	728	736	746	rBV	727388	1205734	14.57%	1.678%
9	7.781	805	815	832	rBV	877705	1438110	17.37%	2.001%
10	8.145	873	877	883	rVB6	5950	11008	0.13%	0.015%
11	8.504	930	938	952	rBV	604181	1091660	13.19%	1.519%
12	8.951	1005	1014	1029	rBV	951427	1623389	19.61%	2.259%
13	9.328	1074	1078	1087	rVB3	12990	23999	0.29%	0.033%
14	9.669	1128	1136	1155	rBV	742005	1311928	15.85%	1.825%
15	10.210	1221	1228	1249	rBV	1147376	2089567	25.24%	2.907%
16	10.392	1253	1259	1266	rBV3	17938	42419	0.51%	0.059%
17	10.581	1283	1291	1306	rBV	1389789	2343216	28.31%	3.260%
18	10.733	1310	1317	1338	rBV	920280	1754164	21.19%	2.441%
19	11.428	1429	1435	1437	rBV7	4854	8724	0.11%	0.012%
20	12.180	1556	1563	1571	rBV	19076	36686	0.44%	0.051%
21	12.398	1594	1600	1602	rBV7	4477	8474	0.10%	0.012%
22	12.422	1602	1604	1610	rVB7	4390	8503	0.10%	0.012%
23	13.027	1702	1707	1711	rBV5	17865	29475	0.36%	0.041%
24	13.239	1739	1743	1747	rVB6	7787	10231	0.12%	0.014%
25	13.327	1750	1758	1764	rBV3	13304	24274	0.29%	0.034%
26	13.398	1767	1770	1775	rVB4	5435	8681	0.10%	0.012%
27	13.769	1826	1833	1840	rBV5	21891	53689	0.65%	0.075%
28	13.851	1840	1847	1862	rBV	2514512	3594395	43.42%	5.001%
29	14.127	1884	1894	1914	rBV	2792606	4267967	51.56%	5.938%
30	14.433	1939	1946	1953	rBV	2365810	3524999	42.58%	4.904%
31	14.498	1953	1957	1962	rVV	122257	188951	2.28%	0.263%
32	14.557	1962	1967	1981	rVB	231896	376903	4.55%	0.524%
33	14.680	1983	1988	2003	rBV2	97245	283893	3.43%	0.395%
34	15.269	2086	2088	2096	rVB9	7541	12131	0.15%	0.017%
35	15.433	2109	2116	2122	rBV	3717648	5637574	68.11%	7.844%
36	15.486	2122	2125	2132	rVB	103081	146361	1.77%	0.204%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP110222\
 Data File : BP012499.D
 Acq On : 03 Nov 2022 20:42
 Operator : CG/JU
 Sample : N5319-01
 Misc :
 ALS Vial : 55 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 BHA96

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP102522.M
 Title : SVOA CALIBRATION

37	15.563	2132	2138	2150	rBV	1134471	1715683	20.73%	2.387%
38	15.786	2172	2176	2184	rVB7	10032	21155	0.26%	0.029%
39	15.945	2197	2203	2208	rBV	54507	83500	1.01%	0.116%
40	16.216	2247	2249	2253	rVB5	8858	9382	0.11%	0.013%
41	16.268	2255	2258	2264	rVV6	10876	15138	0.18%	0.021%
42	16.374	2272	2276	2283	rVB	27131	41376	0.50%	0.058%
43	16.539	2301	2304	2308	rVB5	8249	10458	0.13%	0.015%
44	16.598	2310	2314	2319	rVV7	8669	16106	0.19%	0.022%
45	16.792	2342	2347	2353	rVB	94844	121132	1.46%	0.169%
46	16.857	2354	2358	2365	rVB4	28906	46515	0.56%	0.065%
47	16.957	2371	2375	2378	rBV3	27804	38364	0.46%	0.053%
48	17.192	2408	2415	2426	rBV	2965488	4553814	55.01%	6.336%
49	17.292	2426	2432	2454	rVB2	4591710	7049622	85.16%	9.808%
50	17.863	2527	2529	2532	rVB3	15029	13662	0.17%	0.019%
51	18.080	2562	2566	2573	rBV2	119814	204431	2.47%	0.284%
52	18.257	2594	2596	2601	rVB2	25295	27021	0.33%	0.038%
53	19.115	2737	2742	2746	rBV2	106886	148981	1.80%	0.207%
54	19.180	2749	2753	2756	rBV	71611	106993	1.29%	0.149%
55	19.321	2773	2777	2786	rBV3	78354	138312	1.67%	0.192%
56	19.539	2808	2814	2827	rBV	5902368	8277698	100.00%	11.517%
57	21.292	3107	3112	3122	rBV	3709822	4727130	57.11%	6.577%
58	23.521	3484	3491	3504	rVB2	3446608	7055937	85.24%	9.817%
59	23.674	3510	3517	3537	rVB2	1973668	4161045	50.27%	5.789%




Sum of corrected areas: 71873740

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP110222\
Data File : BP012499.D
Acq On : 03 Nov 2022 20:42
Operator : CG/JU
Sample : N5319-01
Misc :
ALS Vial : 55 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
BHA96

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP102522.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

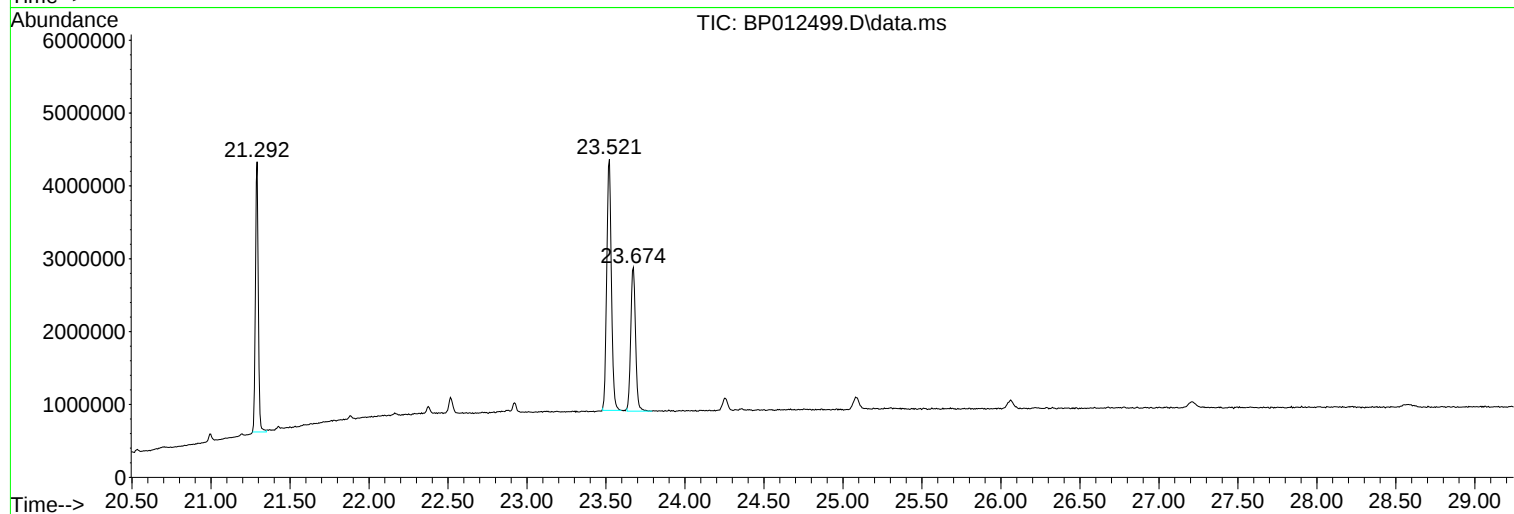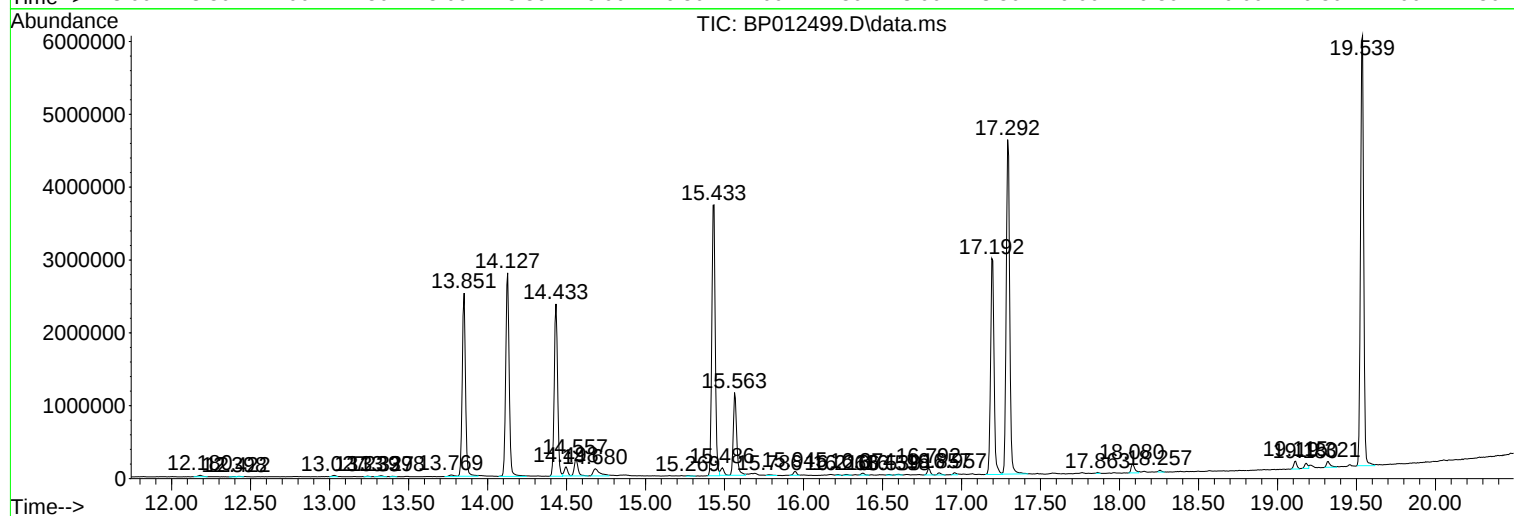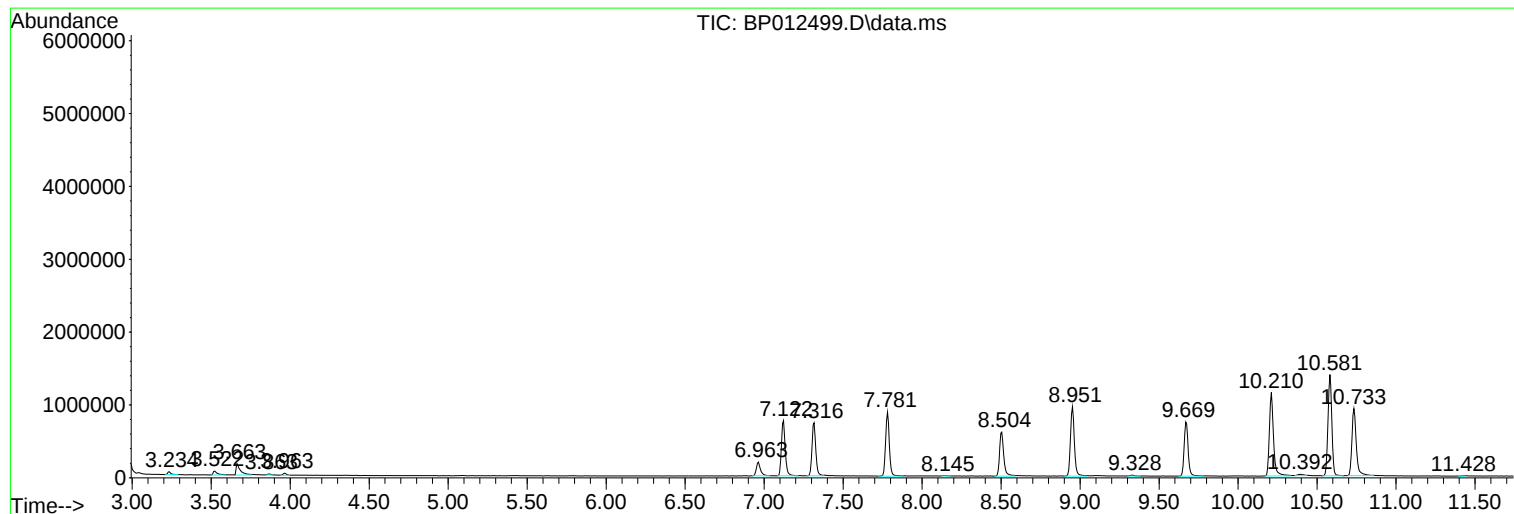

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP110222\
Data File : BP012499.D
Acq On : 03 Nov 2022 20:42
Operator : CG/JU
Sample : N5319-01
Misc :
ALS Vial : 55 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
BHA96










Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP102522.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 Carbonic acid, butyl 2-dime... Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
14.557	2.14 ng/ul	376903	Acenaphthene-d10	14.433

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			Carbonic acid, butyl 2-dimethyla...	189	C9H19NO3	1000331-41-4	80
2			1H-Indole-2-carboxamide, 1-[2-(d...	307	C19H21N3O	1000337-90-1	78
3			Phenylacetic acid, 2-dimethylami...	207	C12H17NO2	036882-00-5	72
4			N,N-Dimethyltryptamine	188	C12H16N2	000061-50-7	72
5			N,N-Dimethyltryptamine	188	C12H16N2	000061-50-7	72

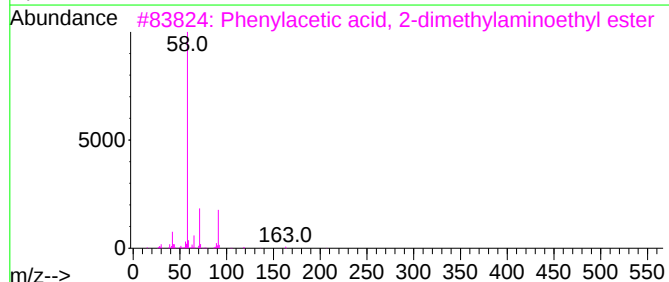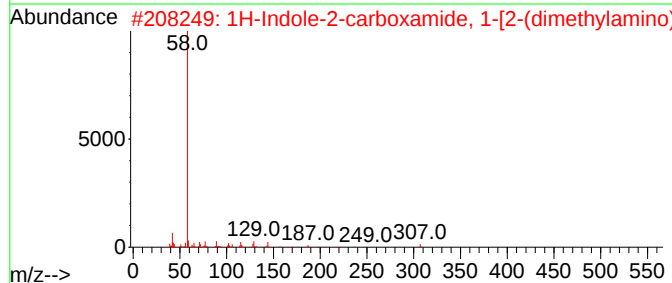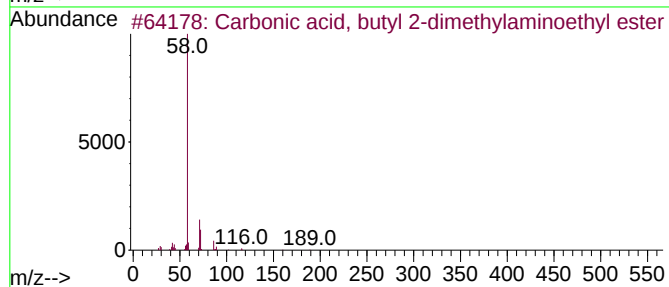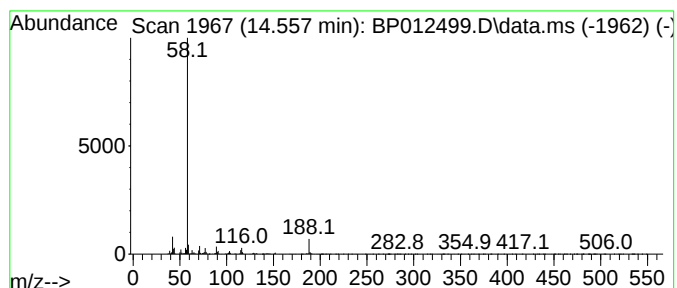

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP110222\
Data File : BP012499.D
Acq On : 03 Nov 2022 20:42
Operator : CG/JU
Sample : N5319-01
Misc :
ALS Vial : 55 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
BHA96

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP102522.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
Carbonic acid, ...	14.557	2.1	ng/u1	376903	3	14.433	3525000	20.0