

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP110222\
 Data File : BP012500.D
 Acq On : 03 Nov 2022 21:17
 Operator : CG/JU
 Sample : N5319-13
 Misc :
 ALS Vial : 56 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 BHAA7

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP102522.M
 Title : SVOA CALIBRATION

Signal : TIC: BP012500.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.234	38	42	47	rBV	39363	50062	0.57%	0.068%
2	3.664	113	115	134	rBV	199929	388407	4.45%	0.527%
3	3.864	145	149	156	rVB2	18077	30556	0.35%	0.041%
4	3.964	163	166	172	rVB	16880	25033	0.29%	0.034%
5	6.964	670	676	689	rBV	190076	367199	4.21%	0.498%
6	7.122	696	703	724	rBV	865584	1478175	16.94%	2.007%
7	7.311	729	735	745	rBV	769067	1311938	15.04%	1.781%
8	7.781	806	815	832	rBV	825531	1373129	15.74%	1.864%
9	8.499	931	937	957	rBV	661426	1186307	13.60%	1.610%
10	8.952	1007	1014	1033	rBV	1115563	1909050	21.88%	2.591%
11	9.334	1072	1079	1084	rBV2	16526	27994	0.32%	0.038%
12	9.669	1127	1136	1150	rBV	865715	1483079	17.00%	2.013%
13	10.210	1219	1228	1249	rBV	1305713	2391734	27.41%	3.247%
14	10.581	1283	1291	1304	rBV	1318325	2231880	25.58%	3.030%
15	10.734	1309	1317	1337	rBV	1075028	2071317	23.74%	2.812%
16	11.428	1429	1435	1442	rBV	5838	15939	0.18%	0.022%
17	12.181	1556	1563	1574	rBV2	22694	44020	0.50%	0.060%
18	13.034	1701	1708	1711	rBV8	8918	17039	0.20%	0.023%
19	13.240	1736	1743	1749	rBV4	14783	26032	0.30%	0.035%
20	13.322	1753	1757	1763	rVB7	8481	14493	0.17%	0.020%
21	13.398	1763	1770	1775	rBV6	7260	14151	0.16%	0.019%
22	13.851	1839	1847	1862	rBV	2934209	4245273	48.65%	5.763%
23	14.122	1883	1893	1908	rBV2	3221532	5010050	57.42%	6.801%
24	14.316	1922	1926	1930	rVB6	10218	16431	0.19%	0.022%
25	14.434	1939	1946	1965	rBV	2275006	3320108	38.05%	4.507%
26	14.681	1982	1988	2003	rBV3	80480	258561	2.96%	0.351%
27	15.275	2085	2089	2094	rVB6	10485	16111	0.18%	0.022%
28	15.434	2109	2116	2132	rBV	4319167	6584143	75.46%	8.938%
29	15.563	2132	2138	2152	rVV	1166808	1791633	20.53%	2.432%
30	15.669	2153	2156	2170	rVB5	28264	67560	0.77%	0.092%
31	16.163	2234	2240	2245	rBV10	6678	16543	0.19%	0.022%
32	16.216	2247	2249	2254	rVB6	9593	10636	0.12%	0.014%
33	16.945	2369	2373	2376	rBV5	5900	10654	0.12%	0.014%
34	17.192	2409	2415	2425	rBV	2869985	4175756	47.85%	5.668%
35	17.292	2426	2432	2449	rVV	4815051	7402388	84.83%	10.048%
36	18.081	2562	2566	2572	rBV	122667	195238	2.24%	0.265%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP110222\
 Data File : BP012500.D
 Acq On : 03 Nov 2022 21:17
 Operator : CG/JU
 Sample : N5319-13
 Misc :
 ALS Vial : 56 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 BHAA7

Integration Parameters: LSCINT.P
 Integrator: RTE
 Smoothing : OFF Filtering: 5
 Sampling : 1 Min Area: 0.1 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP102522.M
 Title : SVOA CALIBRATION

37	18.151	2576	2578	2584	rVB	13444	20732	0.24%	0.028%
38	19.110	2738	2741	2745	rVB2	67957	80641	0.92%	0.109%
39	19.181	2750	2753	2757	rBV	64754	82445	0.94%	0.112%
40	19.322	2773	2777	2784	rBV2	77400	129243	1.48%	0.175%
41	19.539	2808	2814	2825	rBV	6351059	8725888	100.00%	11.845%
42	20.992	3059	3061	3067	rVB5	126795	154289	1.77%	0.209%
43	21.292	3107	3112	3122	rBV	3336993	4277944	49.03%	5.807%
44	23.521	3484	3491	3503	rVB	3423475	6994596	80.16%	9.495%
45	23.674	3511	3517	3528	rVB2	1817339	3624029	41.53%	4.919%




Sum of corrected areas: 73668426

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP110222\
Data File : BP012500.D
Acq On : 03 Nov 2022 21:17
Operator : CG/JU
Sample : N5319-13
Misc :
ALS Vial : 56 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
BHAA7

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP102522.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

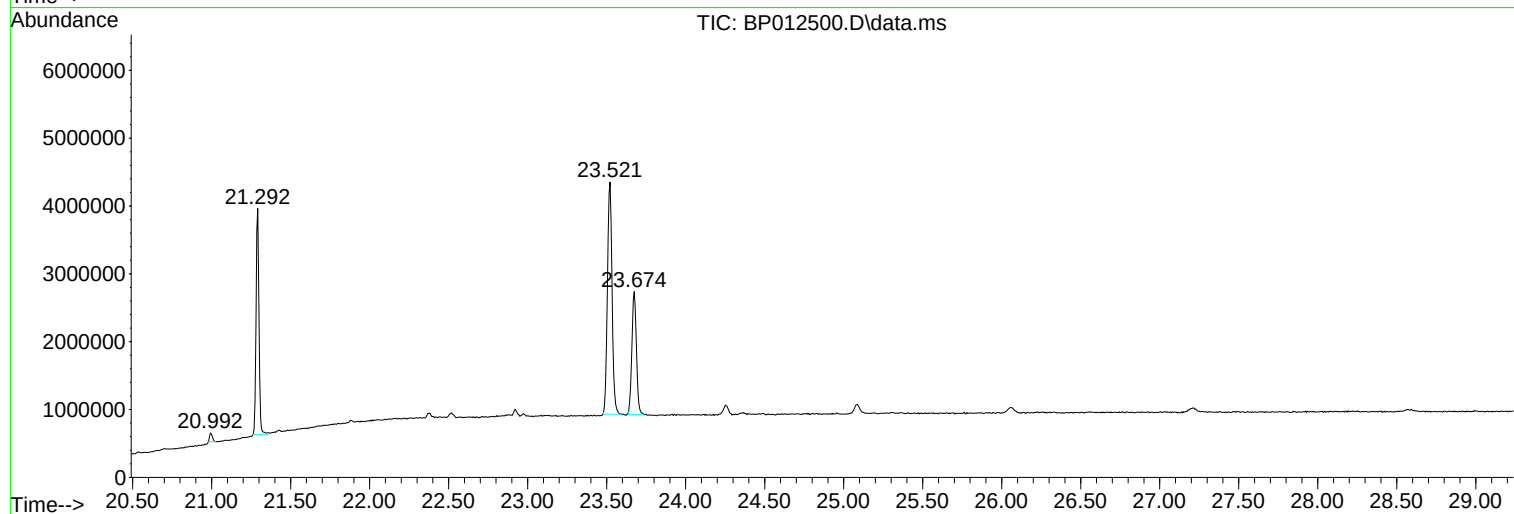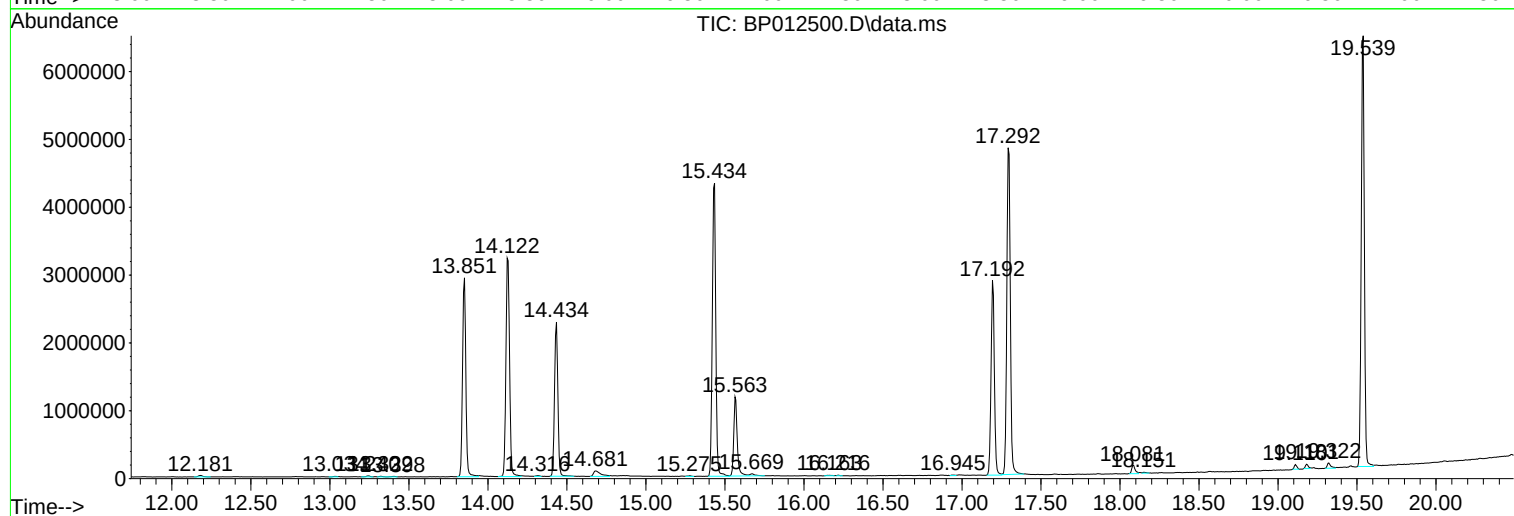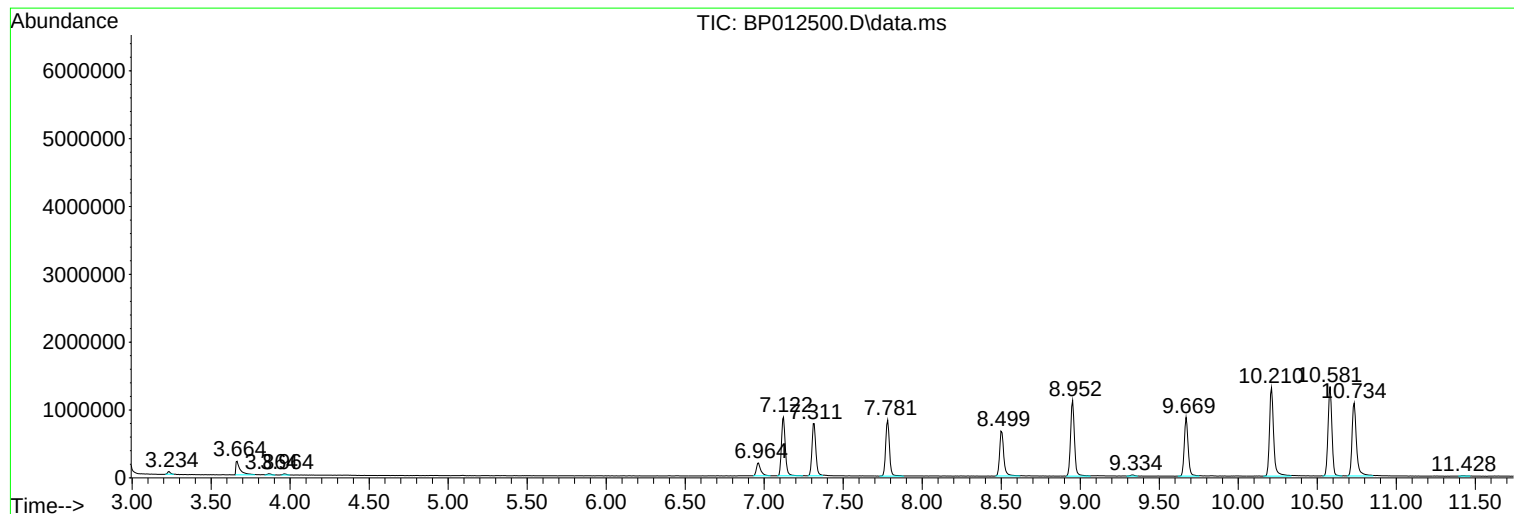

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP110222\
Data File : BP012500.D
Acq On : 03 Nov 2022 21:17
Operator : CG/JU
Sample : N5319-13
Misc :
ALS Vial : 56 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
BHAA7

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP102522.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP110222\
Data File : BP012500.D
Acq On : 03 Nov 2022 21:17
Operator : CG/JU
Sample : N5319-13
Misc :
ALS Vial : 56 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
BHAA7

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP102522.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST0.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc