

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP110222\
 Data File : BP012501.D
 Acq On : 03 Nov 2022 21:51
 Operator : CG/JU
 Sample : N5319-02
 Misc :
 ALS Vial : 57 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 BHA97

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP102522.M
 Title : SVOA CALIBRATION

Signal : TIC: BP012501.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.034	5	8	20	rVB	60526	97887	1.08%	0.117%
2	3.229	38	41	51	rVB	47150	71954	0.79%	0.086%
3	3.529	89	92	98	rBV	20740	33263	0.37%	0.040%
4	3.658	112	114	129	rBV	199331	365947	4.04%	0.439%
5	3.870	144	150	155	rBV	16971	28453	0.31%	0.034%
6	3.964	162	166	172	rVB	19692	26801	0.30%	0.032%
7	4.417	238	243	252	rVB	35977	59512	0.66%	0.071%
8	5.093	351	358	368	rBV2	63485	120106	1.33%	0.144%
9	5.217	374	379	386	rBV	26539	41606	0.46%	0.050%
10	6.964	668	676	688	rBV	206832	386037	4.26%	0.463%
11	7.122	696	703	720	rBV	895228	1499943	16.55%	1.798%
12	7.311	729	735	753	rBV	826904	1407411	15.53%	1.687%
13	7.781	806	815	825	rBV	927101	1525355	16.83%	1.829%
14	8.146	870	877	882	rVB4	12668	27483	0.30%	0.033%
15	8.322	903	907	912	rBV3	6811	11788	0.13%	0.014%
16	8.499	929	937	950	rBV	678035	1222820	13.49%	1.466%
17	8.775	977	984	991	rVB	34999	57665	0.64%	0.069%
18	8.952	1006	1014	1034	rBV	1112357	1915042	21.13%	2.296%
19	9.122	1034	1043	1050	rVB9	9104	24587	0.27%	0.029%
20	9.328	1072	1078	1084	rVB4	12260	21172	0.23%	0.025%
21	9.669	1129	1136	1151	rBV	893397	1509738	16.66%	1.810%
22	10.011	1189	1194	1200	rVB4	8495	15689	0.17%	0.019%
23	10.211	1221	1228	1246	rBV	1325997	2456139	27.10%	2.945%
24	10.393	1252	1259	1269	rVB4	17626	47509	0.52%	0.057%
25	10.581	1283	1291	1305	rBV	1455106	2489060	27.47%	2.984%
26	10.734	1310	1317	1332	rBV	1060075	2014290	22.23%	2.415%
27	11.940	1513	1522	1528	rBV2	16644	33142	0.37%	0.040%
28	12.175	1557	1562	1571	rVB2	21838	37294	0.41%	0.045%
29	12.405	1596	1601	1607	rBV9	4220	11303	0.12%	0.014%
30	12.599	1628	1634	1642	rBV9	9599	19817	0.22%	0.024%
31	12.675	1642	1647	1654	rVB8	7576	12367	0.14%	0.015%
32	12.846	1671	1676	1680	rBV3	8572	12679	0.14%	0.015%
33	12.981	1693	1699	1701	rBV	14001	22959	0.25%	0.028%
34	13.028	1701	1707	1717	rVB	277692	444123	4.90%	0.532%
35	13.157	1722	1729	1733	rBV9	6331	13861	0.15%	0.017%
36	13.240	1736	1743	1746	rBV8	9487	16822	0.19%	0.020%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP110222\
 Data File : BP012501.D
 Acq On : 03 Nov 2022 21:51
 Operator : CG/JU
 Sample : N5319-02
 Misc :
 ALS Vial : 57 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 BHA97

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP102522.M
 Title : SVOA CALIBRATION

37	13.322	1753	1757	1761	rBV4	7376	12305	0.14%	0.015%
38	13.399	1766	1770	1774	rVB7	8346	13584	0.15%	0.016%
39	13.487	1780	1785	1791	rVB3	13779	21407	0.24%	0.026%
40	13.604	1800	1805	1810	rBV9	5914	12181	0.13%	0.015%
41	13.746	1820	1829	1831	rBV6	10411	25614	0.28%	0.031%
42	13.851	1840	1847	1860	rBV	2979461	4328314	47.76%	5.189%
43	13.975	1864	1868	1874	rVB	48862	72788	0.80%	0.087%
44	14.081	1882	1886	1887	rBV3	8325	9670	0.11%	0.012%
45	14.128	1887	1894	1904	rVV	3178448	4895646	54.02%	5.870%
46	14.199	1904	1906	1908	rVV3	25294	32663	0.36%	0.039%
47	14.222	1908	1910	1921	rVB	38139	71376	0.79%	0.086%
48	14.434	1937	1946	1954	rBV2	2485512	5353925	59.08%	6.419%
49	14.493	1954	1956	1964	rVV	114652	165636	1.83%	0.199%
50	14.557	1964	1967	1974	rVB	41712	67003	0.74%	0.080%
51	14.681	1982	1988	2003	rBV3	114991	349883	3.86%	0.419%
52	14.787	2003	2006	2012	rVV3	23348	49050	0.54%	0.059%
53	14.863	2015	2019	2027	rVB	32024	59309	0.65%	0.071%
54	14.969	2032	2037	2039	rBV2	10940	15715	0.17%	0.019%
55	15.187	2071	2074	2078	rVB	11879	14950	0.16%	0.018%
56	15.269	2084	2088	2092	rBV6	6110	9423	0.10%	0.011%
57	15.334	2096	2099	2105	rVB5	12621	16051	0.18%	0.019%
58	15.428	2109	2115	2122	rVV	4360117	6559295	72.38%	7.864%
59	15.487	2122	2125	2130	rVV	128951	186746	2.06%	0.224%
60	15.563	2133	2138	2150	rVV	1290319	1915280	21.13%	2.296%
61	15.687	2151	2159	2165	rVB2	163005	288822	3.19%	0.346%
62	15.746	2166	2169	2173	rBV2	23108	29862	0.33%	0.036%
63	15.945	2197	2203	2210	rBV3	71487	118491	1.31%	0.142%
64	16.081	2221	2226	2229	rBV5	22788	35045	0.39%	0.042%
65	16.128	2229	2234	2236	rBV2	34922	55440	0.61%	0.066%
66	16.269	2254	2258	2263	rBV	30886	50348	0.56%	0.060%
67	16.328	2264	2268	2272	rVV3	31015	53397	0.59%	0.064%
68	16.375	2272	2276	2282	rVB	129276	195537	2.16%	0.234%
69	16.487	2290	2295	2300	rBV6	26495	58550	0.65%	0.070%
70	16.540	2301	2304	2307	rVV3	20384	25413	0.28%	0.030%
71	16.598	2308	2314	2319	rVB5	26640	48885	0.54%	0.059%
72	16.657	2320	2324	2328	rVV	20782	31471	0.35%	0.038%
73	16.734	2334	2337	2342	rVB3	30330	39003	0.43%	0.047%
74	16.793	2342	2347	2354	rVB	140016	183983	2.03%	0.221%
75	16.863	2355	2359	2364	rVB6	20249	31061	0.34%	0.037%
76	16.957	2371	2375	2380	rBV4	30866	42952	0.47%	0.051%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP110222\
 Data File : BP012501.D
 Acq On : 03 Nov 2022 21:51
 Operator : CG/JU
 Sample : N5319-02
 Misc :
 ALS Vial : 57 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 BHA97

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP102522.M
 Title : SVOA CALIBRATION

77	17.192	2409	2415	2426	rBV	3256811	4634941	51.14%	5.557%
78	17.292	2426	2432	2443	rBV2	5428231	7795282	86.02%	9.346%
79	17.463	2459	2461	2469	rVB7	19391	28662	0.32%	0.034%
80	17.557	2473	2477	2484	rBV4	17912	56232	0.62%	0.067%
81	17.757	2508	2511	2521	rVB5	29918	51354	0.57%	0.062%
82	17.887	2529	2533	2539	rBV	88726	126644	1.40%	0.152%
83	18.034	2555	2558	2562	rVB5	25470	29481	0.33%	0.035%
84	18.081	2562	2566	2576	rBV	142253	246625	2.72%	0.296%
85	18.234	2588	2592	2602	rVB3	114004	189875	2.10%	0.228%
86	18.334	2605	2609	2611	rBV	75616	95796	1.06%	0.115%
87	18.381	2613	2617	2622	rVB	131045	187722	2.07%	0.225%
88	18.628	2656	2659	2666	rVB	63415	86325	0.95%	0.104%
89	19.110	2737	2741	2746	rBV	193653	245053	2.70%	0.294%
90	19.181	2749	2753	2756	rBV	78069	114188	1.26%	0.137%
91	19.257	2763	2766	2770	rBV	111246	124113	1.37%	0.149%
92	19.322	2773	2777	2787	rBV3	94302	179516	1.98%	0.215%
93	19.534	2808	2813	2820	rBV	6566474	9062651	100.00%	10.866%
94	20.122	2910	2913	2918	rVB	59895	71328	0.79%	0.086%
95	20.533	2980	2983	2988	rBV4	71067	96547	1.07%	0.116%
96	21.286	3107	3111	3121	rBV	3541270	4780141	52.75%	5.731%
97	23.516	3483	3490	3506	rVB2	3636652	7589770	83.75%	9.100%
98	23.669	3510	3516	3525	rVB2	1971635	3965571	43.76%	4.755%




Sum of corrected areas: 83405515

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP110222\
Data File : BP012501.D
Acq On : 03 Nov 2022 21:51
Operator : CG/JU
Sample : N5319-02
Misc :
ALS Vial : 57 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
BHA97

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP102522.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

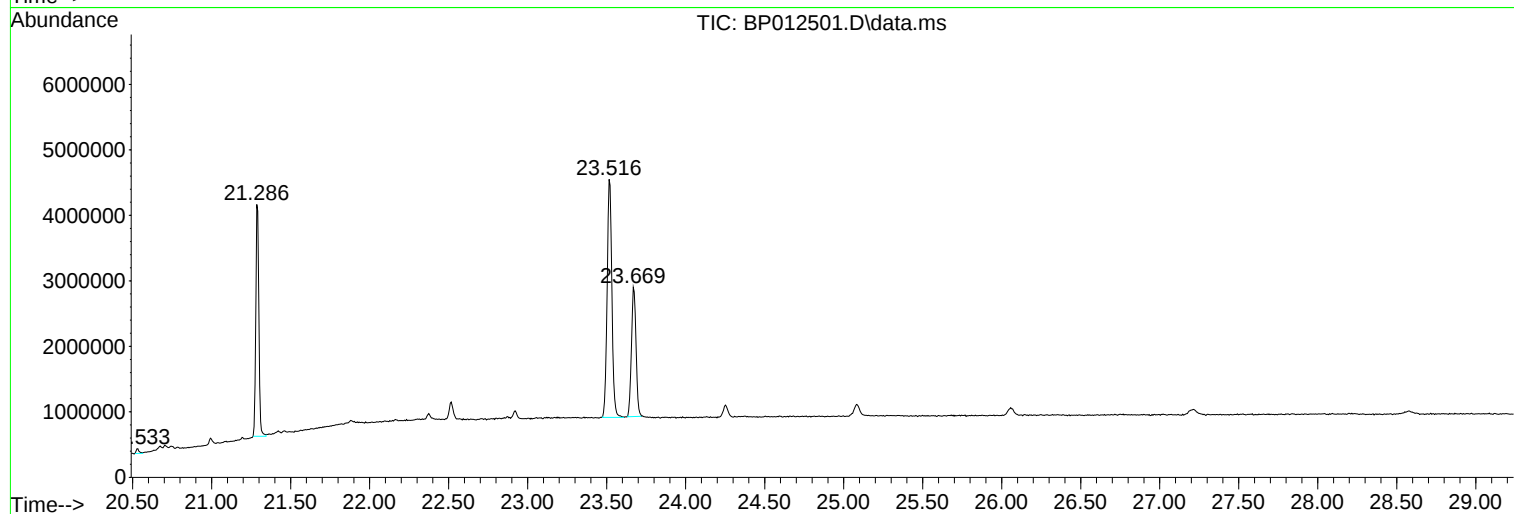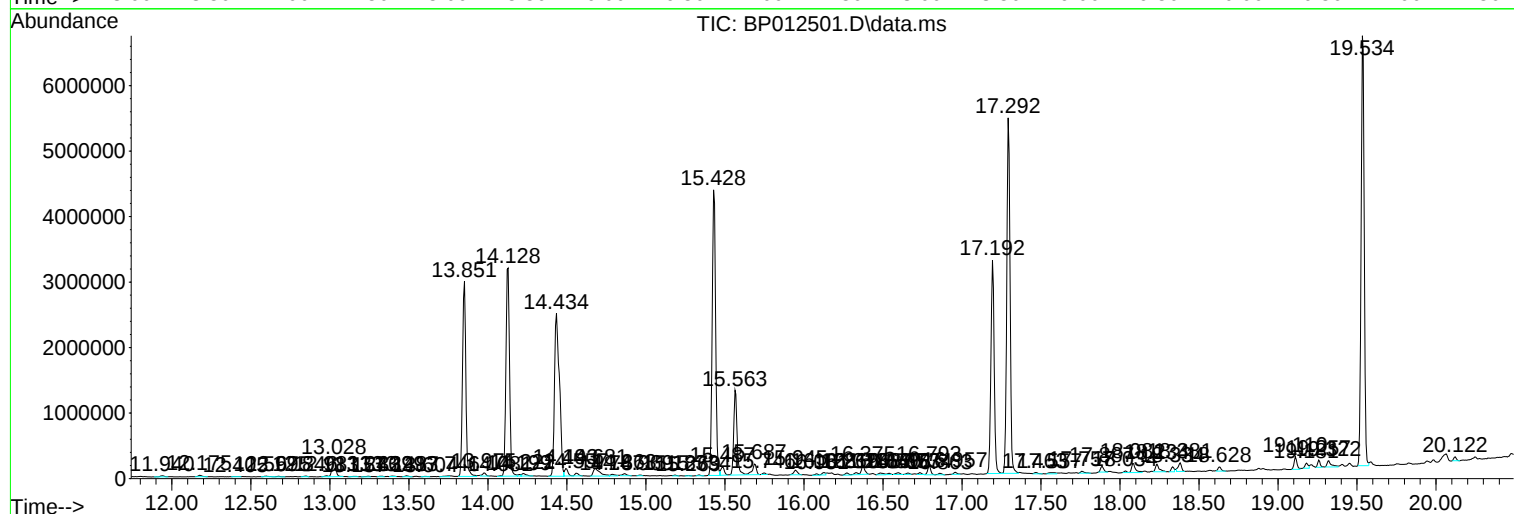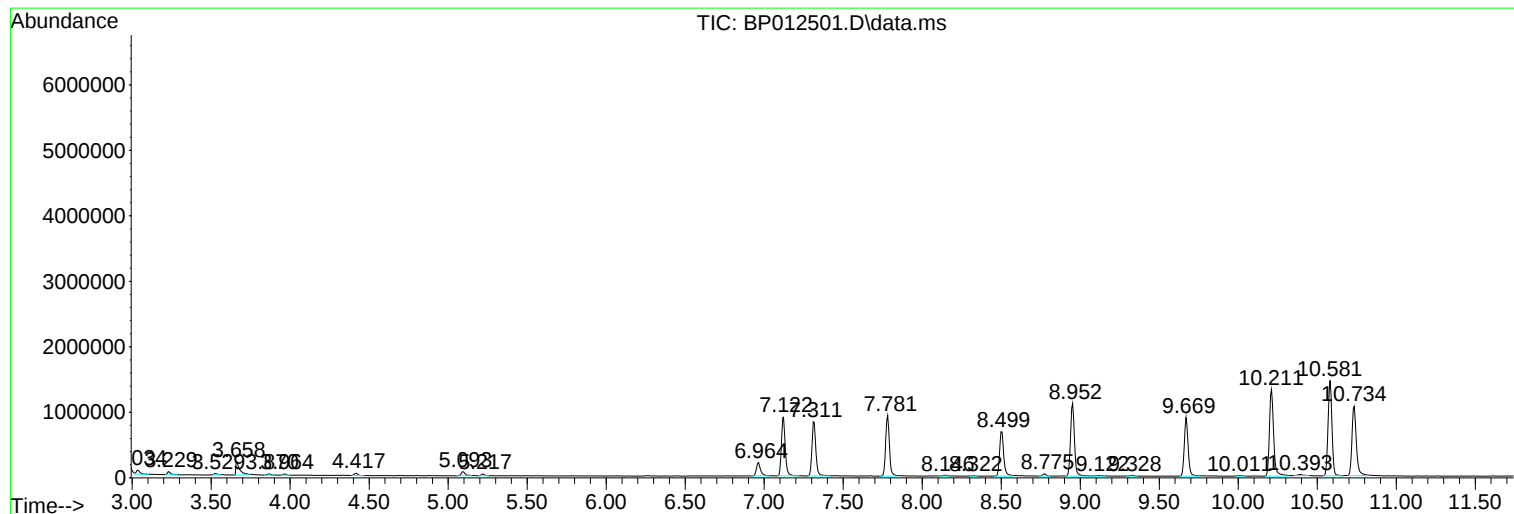

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP110222\
Data File : BP012501.D
Acq On : 03 Nov 2022 21:51
Operator : CG/JU
Sample : N5319-02
Misc :
ALS Vial : 57 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
BHA97

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP102522.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP110222\
Data File : BP012501.D
Acq On : 03 Nov 2022 21:51
Operator : CG/JU
Sample : N5319-02
Misc :
ALS Vial : 57 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
BHA97

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP102522.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST0.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc