

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP110222\
 Data File : BP012503.D
 Acq On : 03 Nov 2022 23:00
 Operator : CG/JU
 Sample : N5319-14
 Misc :
 ALS Vial : 59 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 BHAA8

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP102522.M
 Title : SVOA CALIBRATION

Signal : TIC: BP012503.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.234	38	42	51	rVB	50435	74126	0.74%	0.083%
2	3.658	111	114	138	rBV	293556	555650	5.57%	0.623%
3	3.864	145	149	156	rVB	21560	33928	0.34%	0.038%
4	3.964	162	166	172	rVB	20219	29185	0.29%	0.033%
5	5.093	349	358	365	rBV2	26464	46477	0.47%	0.052%
6	6.958	669	675	688	rBV	244933	441727	4.43%	0.495%
7	7.117	695	702	718	rBV	1063920	1768441	17.73%	1.982%
8	7.311	728	735	745	rBV	976117	1613443	16.18%	1.808%
9	7.781	807	815	828	rBV	1077645	1791342	17.96%	2.008%
10	8.499	928	937	950	rBV	825004	1418609	14.23%	1.590%
11	8.946	1005	1013	1033	rBV	1270957	2230029	22.36%	2.499%
12	9.328	1070	1078	1082	rVB3	11943	22290	0.22%	0.025%
13	9.669	1129	1136	1149	rBV	1032900	1777139	17.82%	1.992%
14	10.205	1220	1227	1250	rBV	1531367	2816005	28.24%	3.156%
15	10.581	1283	1291	1305	rVB	1710774	2925005	29.33%	3.278%
16	10.734	1308	1317	1345	rBV	1250231	2519127	25.26%	2.823%
17	12.181	1556	1563	1570	rBV	25384	47255	0.47%	0.053%
18	12.781	1660	1665	1672	rBV9	5136	10960	0.11%	0.012%
19	13.028	1702	1707	1718	rVB9	10653	30809	0.31%	0.035%
20	13.240	1737	1743	1747	rBV5	10459	17093	0.17%	0.019%
21	13.322	1752	1757	1764	rVV2	33873	58584	0.59%	0.066%
22	13.404	1766	1771	1779	rVB9	9506	18410	0.18%	0.021%
23	13.751	1825	1830	1836	rBV9	5380	13111	0.13%	0.015%
24	13.851	1839	1847	1867	rBV	3126703	4753450	47.67%	5.328%
25	14.122	1884	1893	1910	rBV	3660506	5641684	56.58%	6.323%
26	14.434	1939	1946	1953	rBV	2868977	4351620	43.64%	4.877%
27	14.675	1980	1987	2005	rBV2	120777	361210	3.62%	0.405%
28	14.846	2011	2016	2020	rBV8	6217	15390	0.15%	0.017%
29	15.269	2084	2088	2093	rVB7	6746	11662	0.12%	0.013%
30	15.428	2109	2115	2124	rBV	4911487	7254061	72.74%	8.130%
31	15.563	2132	2138	2151	rBV	1437941	2087520	20.93%	2.340%
32	15.669	2152	2156	2159	rVV2	35793	63192	0.63%	0.071%
33	15.698	2159	2161	2168	rVB	32145	46260	0.46%	0.052%
34	15.957	2200	2205	2210	rBV2	17773	25522	0.26%	0.029%
35	16.145	2231	2237	2254	rBV	109502	259323	2.60%	0.291%
36	16.481	2289	2294	2302	rBV5	16002	36183	0.36%	0.041%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP110222\
 Data File : BP012503.D
 Acq On : 03 Nov 2022 23:00
 Operator : CG/JU
 Sample : N5319-14
 Misc :
 ALS Vial : 59 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 BHAA8

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP102522.M
 Title : SVOA CALIBRATION

37	16.869	2357	2360	2364	rVB5	8997	12386	0.12%	0.014%
38	17.192	2408	2415	2426	rBV	3950444	5543499	55.59%	6.213%
39	17.292	2426	2432	2457	rVV2	5640503	8519101	85.43%	9.548%
40	17.481	2459	2464	2472	rVV	89122	119635	1.20%	0.134%
41	18.081	2562	2566	2572	rBV2	109084	159889	1.60%	0.179%
42	19.110	2737	2741	2745	rBV	89259	111182	1.11%	0.125%
43	19.181	2749	2753	2759	rBV	84180	140032	1.40%	0.157%
44	19.316	2773	2776	2785	rBV3	83949	140899	1.41%	0.158%
45	19.534	2807	2813	2826	rBV	7144504	9971970	100.00%	11.176%
46	20.528	2980	2982	2986	rVB3	71153	69391	0.70%	0.078%
47	21.286	3106	3111	3119	rBV	4184065	5780718	57.97%	6.479%
48	23.516	3483	3490	3502	rVB2	4133804	8508976	85.33%	9.537%
49	23.669	3510	3516	3529	rVB2	2525281	4980836	49.95%	5.582%




Sum of corrected areas: 89224336

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP110222\
Data File : BP012503.D
Acq On : 03 Nov 2022 23:00
Operator : CG/JU
Sample : N5319-14
Misc :
ALS Vial : 59 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
BHAA8

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP102522.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

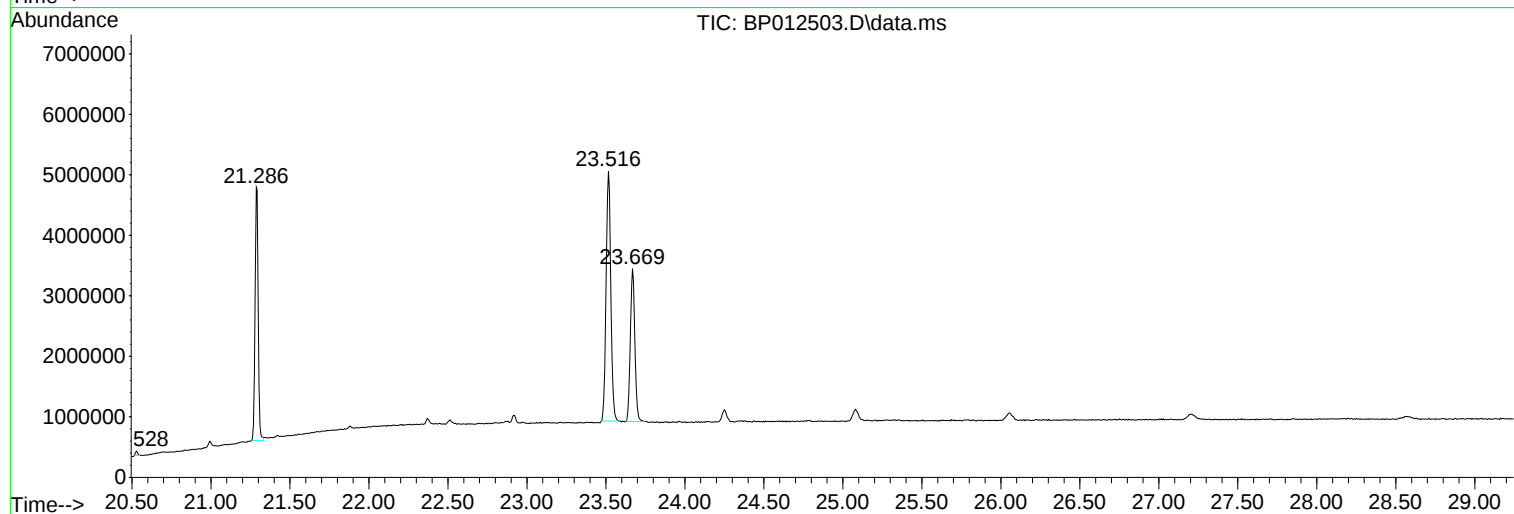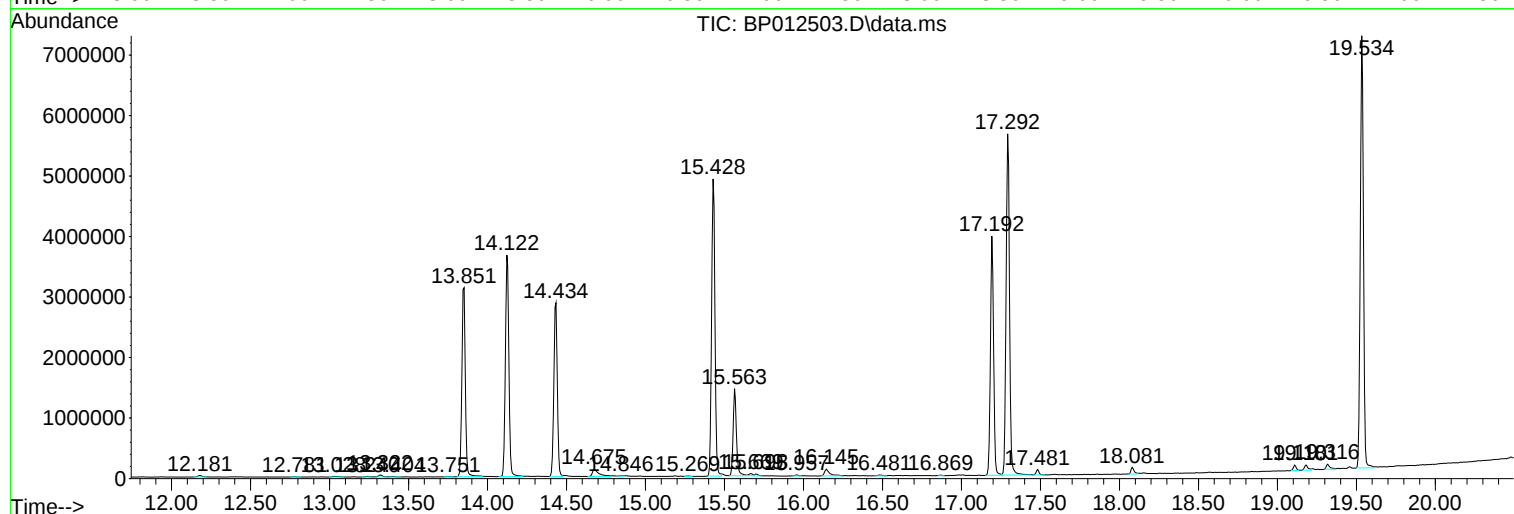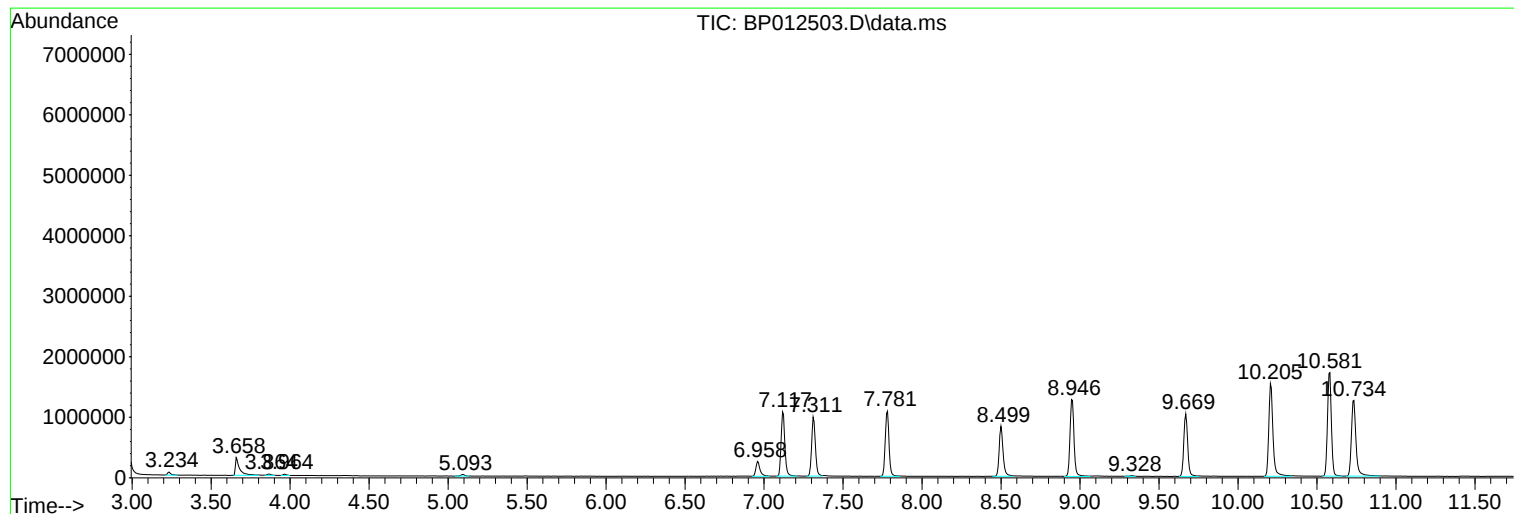

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP110222\
Data File : BP012503.D
Acq On : 03 Nov 2022 23:00
Operator : CG/JU
Sample : N5319-14
Misc :
ALS Vial : 59 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
BHAA8

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP102522.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP110222\
Data File : BP012503.D
Acq On : 03 Nov 2022 23:00
Operator : CG/JU
Sample : N5319-14
Misc :
ALS Vial : 59 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
BHAA8

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP102522.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST0.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc