

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP110222\
 Data File : BP012504.D
 Acq On : 03 Nov 2022 23:35
 Operator : CG/JU
 Sample : N5319-15
 Misc :
 ALS Vial : 60 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 BHAB0

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP102522.M
 Title : SVOA CALIBRATION

Signal : TIC: BP012504.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.234	38	42	52	rVB	48388	78093	0.77%	0.091%
2	3.664	113	115	134	rBV	178451	357514	3.54%	0.416%
3	3.864	145	149	156	rVB	17249	27914	0.28%	0.032%
4	3.964	161	166	172	rBV	16946	28573	0.28%	0.033%
5	5.093	353	358	365	rVB5	13007	24431	0.24%	0.028%
6	6.957	669	675	688	rBV	200033	367844	3.64%	0.428%
7	7.116	696	702	716	rBV	1001682	1674737	16.59%	1.947%
8	7.310	729	735	754	rVB	903535	1479339	14.65%	1.720%
9	7.781	807	815	831	rBV	970299	1660205	16.45%	1.930%
10	8.499	931	937	950	rBV	717634	1245709	12.34%	1.448%
11	8.952	1006	1014	1030	rBV	1218070	2121112	21.01%	2.466%
12	9.328	1071	1078	1083	rVB3	11830	21409	0.21%	0.025%
13	9.669	1127	1136	1154	rBV	981969	1683621	16.68%	1.958%
14	10.204	1220	1227	1249	rBV	1418617	2635443	26.11%	3.064%
15	10.375	1251	1256	1281	rVV2	61871	209821	2.08%	0.244%
16	10.581	1283	1291	1304	rVB	1593916	2737853	27.12%	3.183%
17	10.728	1309	1316	1338	rBV	1237689	2301680	22.80%	2.676%
18	11.434	1427	1436	1442	rBV	6673	21159	0.21%	0.025%
19	12.175	1555	1562	1573	rBV2	26116	53347	0.53%	0.062%
20	12.775	1659	1664	1668	rBV8	6723	11415	0.11%	0.013%
21	13.040	1704	1709	1711	rBV5	8438	16608	0.16%	0.019%
22	13.240	1737	1743	1746	rBV4	7608	13924	0.14%	0.016%
23	13.322	1752	1757	1763	rBV5	10415	18823	0.19%	0.022%
24	13.398	1765	1770	1776	rBV4	7404	13264	0.13%	0.015%
25	13.845	1838	1846	1859	rBV	3170380	4700130	46.56%	5.465%
26	14.122	1885	1893	1907	rBV	3584223	5500641	54.49%	6.396%
27	14.434	1939	1946	1955	rBV	2669395	4097254	40.59%	4.764%
28	14.675	1982	1987	2005	rBV	95296	292300	2.90%	0.340%
29	15.269	2084	2088	2094	rVB6	9670	16163	0.16%	0.019%
30	15.428	2108	2115	2129	rBV	4849121	7320875	72.52%	8.512%
31	15.563	2132	2138	2151	rBV	1414381	2024090	20.05%	2.353%
32	15.669	2152	2156	2160	rVV2	21768	28271	0.28%	0.033%
33	16.151	2234	2238	2245	rBV3	22628	49126	0.49%	0.057%
34	16.598	2311	2314	2319	rBV7	8577	11752	0.12%	0.014%
35	17.192	2408	2415	2425	rBV	3724470	5201876	51.53%	6.048%
36	17.292	2426	2432	2444	rVV2	5641573	8481049	84.01%	9.861%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP110222\
 Data File : BP012504.D
 Acq On : 03 Nov 2022 23:35
 Operator : CG/JU
 Sample : N5319-15
 Misc :
 ALS Vial : 60 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 BHAB0

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP102522.M
 Title : SVOA CALIBRATION

37	17.863	2525	2529	2533	rBV3	33600	43362	0.43%	0.050%
38	18.080	2562	2566	2575	rBV2	143209	233852	2.32%	0.272%
39	19.110	2737	2741	2746	rBV2	89604	126682	1.25%	0.147%
40	19.180	2749	2753	2756	rBV	84754	122489	1.21%	0.142%
41	19.316	2773	2776	2784	rBV2	106218	174007	1.72%	0.202%
42	19.533	2807	2813	2827	rBV	7111997	10094840	100.00%	11.737%
43	21.286	3106	3111	3119	rBV	4058226	5466422	54.15%	6.356%
44	23.515	3483	3490	3502	rVB2	4103479	8556217	84.76%	9.948%
45	23.668	3510	3516	3527	rVB	2304539	4662269	46.18%	5.421%




Sum of corrected areas: 86007505

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP110222\
Data File : BP012504.D
Acq On : 03 Nov 2022 23:35
Operator : CG/JU
Sample : N5319-15
Misc :
ALS Vial : 60 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
BHAB0

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP102522.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

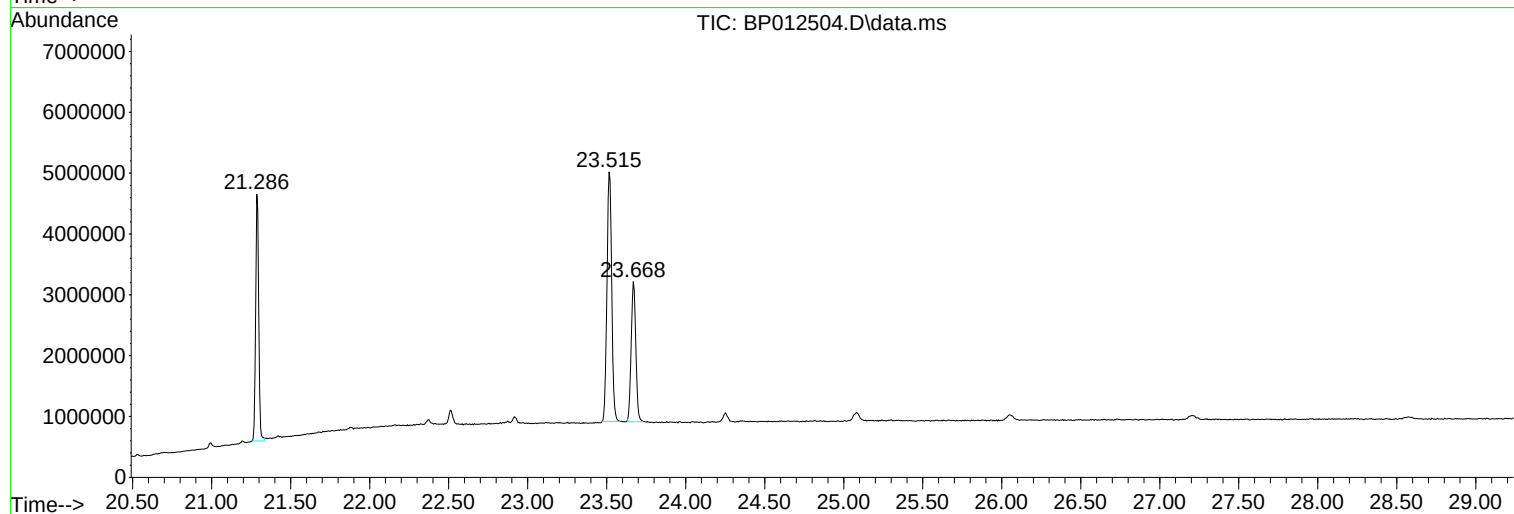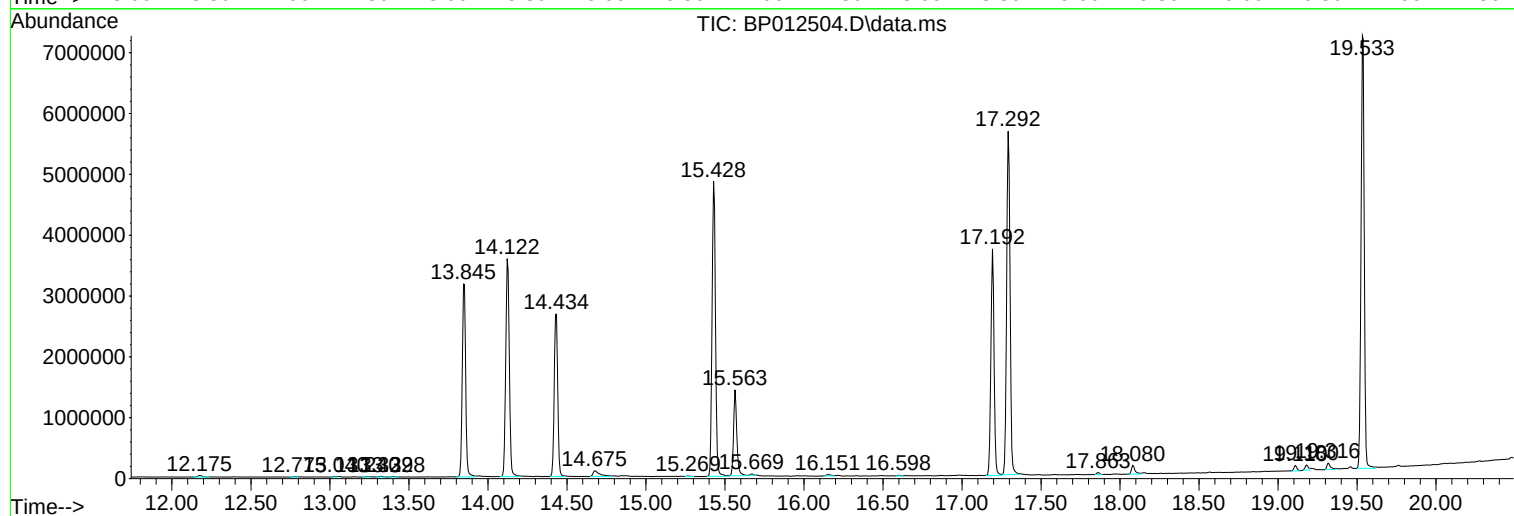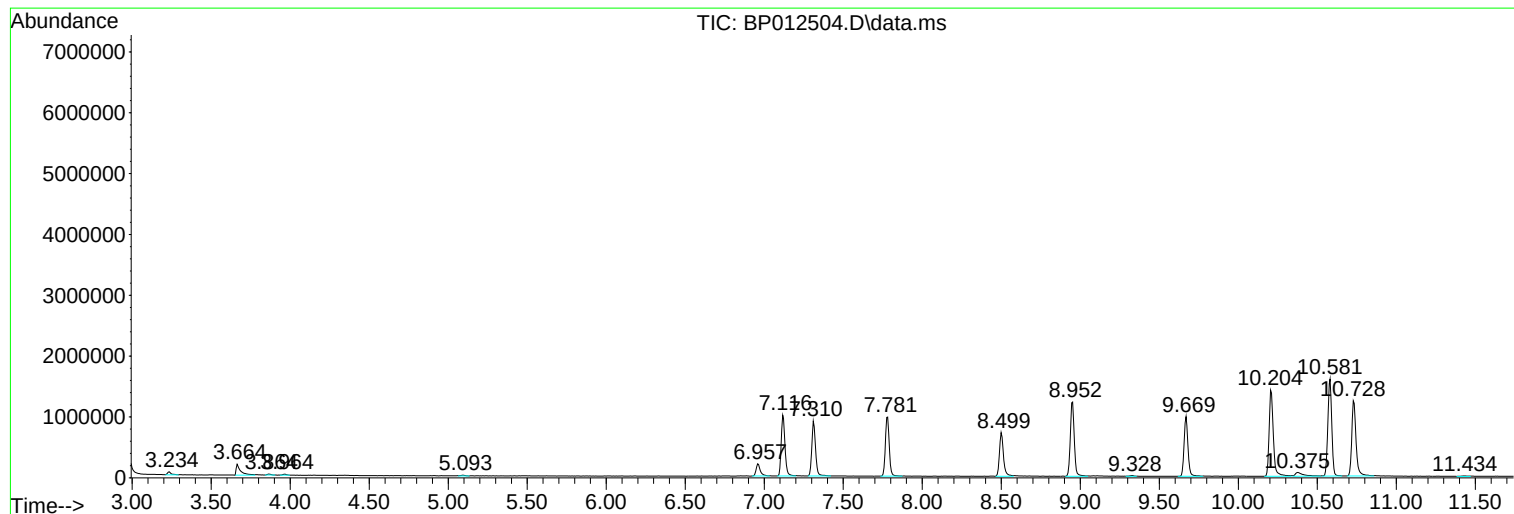

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP110222\
Data File : BP012504.D
Acq On : 03 Nov 2022 23:35
Operator : CG/JU
Sample : N5319-15
Misc :
ALS Vial : 60 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
BHAB0

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP102522.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP110222\
Data File : BP012504.D
Acq On : 03 Nov 2022 23:35
Operator : CG/JU
Sample : N5319-15
Misc :
ALS Vial : 60 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
BHAB0

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP102522.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST0.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc