

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP110222\
 Data File : BP012509.D
 Acq On : 04 Nov 2022 03:01
 Operator : CG/JU
 Sample : PB148748BL
 Misc :
 ALS Vial : 66 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SBLK748

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP102522.M
 Title : SVOA CALIBRATION

Signal : TIC: BP012509.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.234	38	42	51	rVB	68435	100868	1.22%	0.132%
2	3.964	163	166	172	rVB2	18268	24361	0.29%	0.032%
3	6.952	668	674	690	rBV	1121177	1934493	23.36%	2.525%
4	7.116	695	702	716	rVV	952622	1537415	18.56%	2.007%
5	7.310	728	735	752	rBV	1138977	1877391	22.67%	2.451%
6	7.775	807	814	826	rBV	920670	1489542	17.98%	1.945%
7	8.499	927	937	962	rBV	1441510	2592607	31.30%	3.385%
8	8.946	1005	1013	1033	rBV	1139432	1933313	23.34%	2.524%
9	9.669	1128	1136	1148	rBV	912125	1630761	19.69%	2.129%
10	10.204	1219	1227	1259	rBV	1322745	2725368	32.91%	3.558%
11	10.575	1283	1290	1310	rBV	1466524	2468542	29.80%	3.223%
12	12.187	1557	1564	1573	rBV2	17083	43467	0.52%	0.057%
13	13.322	1752	1757	1761	rBV7	5316	8291	0.10%	0.011%
14	13.398	1766	1770	1775	rVB5	5130	8510	0.10%	0.011%
15	13.845	1837	1846	1861	rBV	2914860	4229700	51.07%	5.522%
16	14.122	1885	1893	1914	rBV	3260649	4953530	59.81%	6.467%
17	14.428	1938	1945	1963	rBV	2485603	3743028	45.19%	4.886%
18	14.657	1978	1984	2011	rBV	702306	1812190	21.88%	2.366%
19	15.428	2108	2115	2132	rBV	4417717	6442170	77.78%	8.410%
20	15.563	2132	2138	2152	rVV	879790	1330577	16.07%	1.737%
21	15.669	2152	2156	2161	rVB2	22819	37383	0.45%	0.049%
22	16.216	2245	2249	2253	rBV7	6211	10600	0.13%	0.014%
23	16.869	2356	2360	2370	rVB7	7514	17981	0.22%	0.023%
24	16.981	2376	2379	2384	rVB3	7368	9758	0.12%	0.013%
25	17.192	2408	2415	2426	rBV	3172038	4732537	57.14%	6.178%
26	17.292	2426	2432	2454	rVB	4959033	7255372	87.60%	9.472%
27	17.863	2525	2529	2532	rBV6	7023	9719	0.12%	0.013%
28	19.110	2737	2741	2746	rBV	67014	84510	1.02%	0.110%
29	19.180	2749	2753	2758	rVV	53913	76304	0.92%	0.100%
30	19.533	2807	2813	2830	rBV	6037759	8282417	100.00%	10.813%
31	21.286	3106	3111	3121	rBV	3458840	4577187	55.26%	5.975%
32	23.515	3483	3490	3504	rVB	3310349	6629263	80.04%	8.654%
33	23.668	3510	3516	3532	rVB2	1943195	3990408	48.18%	5.209%




Sum of corrected areas: 76599563

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP110222\
Data File : BP012509.D
Acq On : 04 Nov 2022 03:01
Operator : CG/JU
Sample : PB148748BL
Misc :
ALS Vial : 66 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK748

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP102522.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

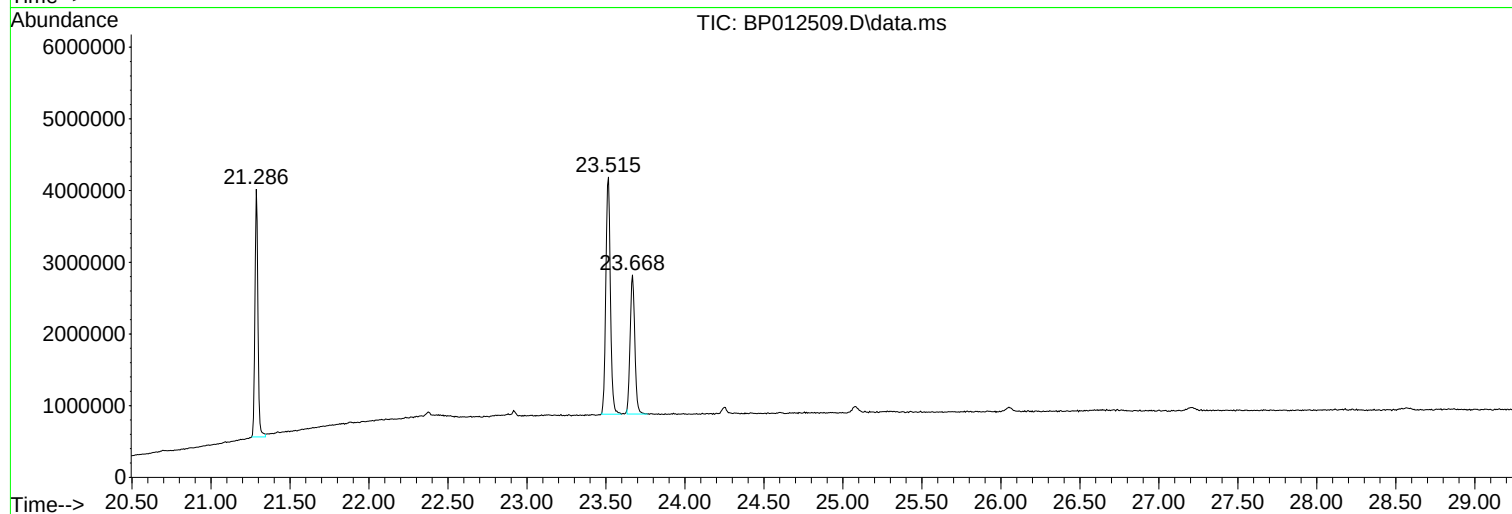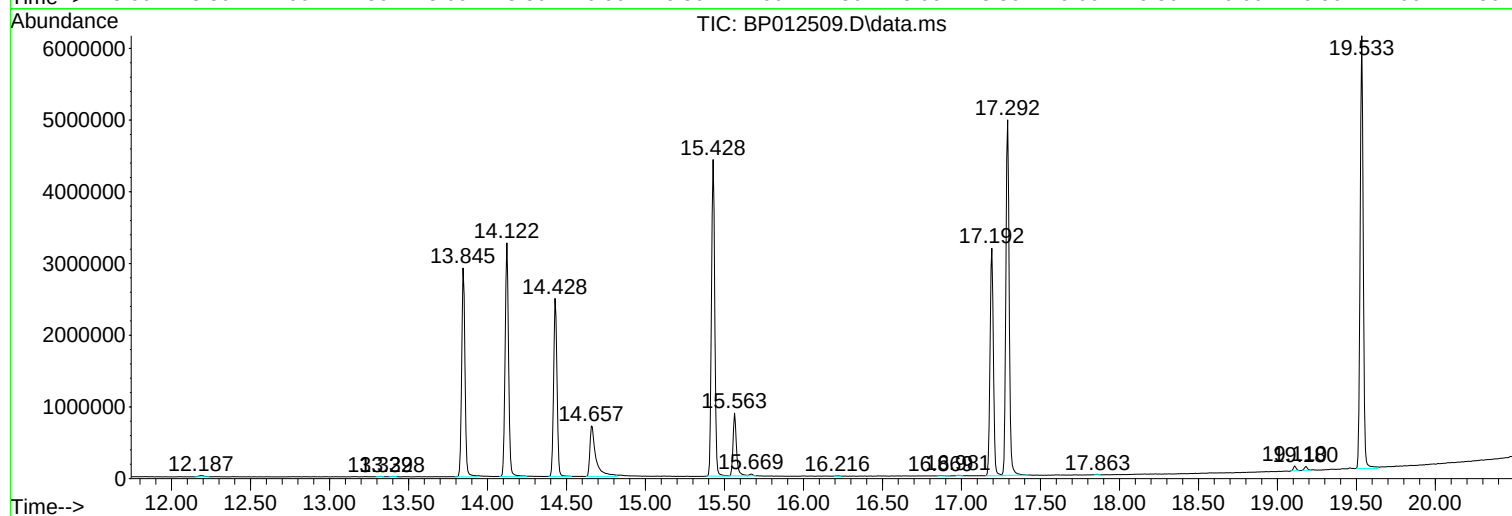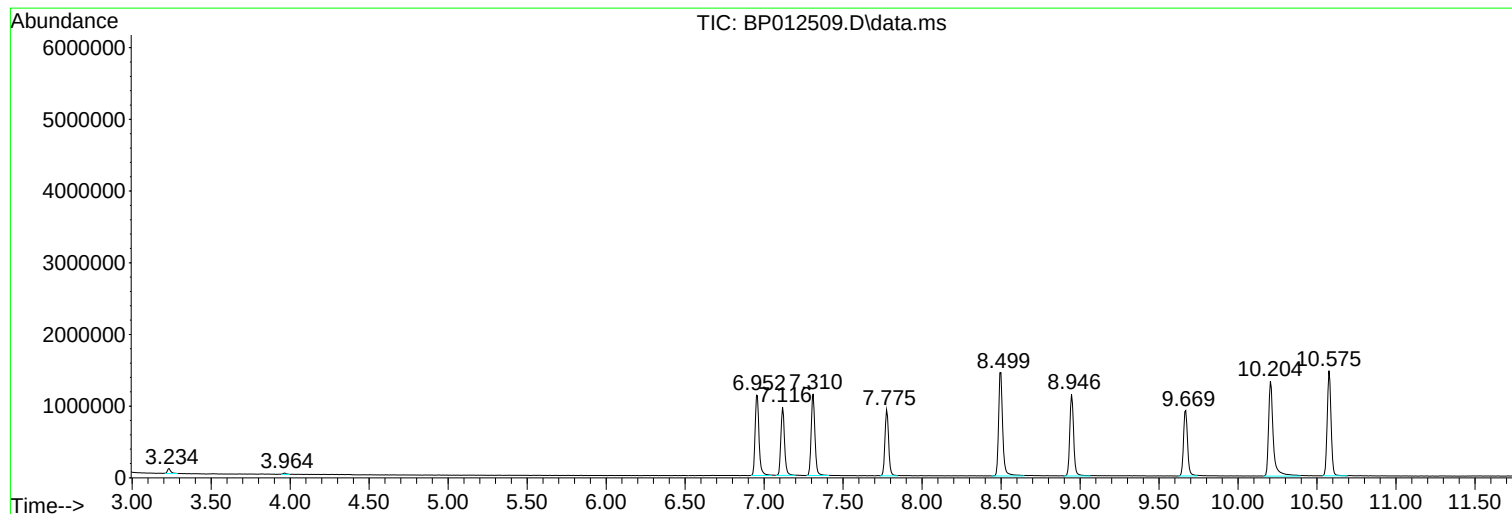

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP110222\
Data File : BP012509.D
Acq On : 04 Nov 2022 03:01
Operator : CG/JU
Sample : PB148748BL
Misc :
ALS Vial : 66 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK748

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP102522.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP110222\
Data File : BP012509.D
Acq On : 04 Nov 2022 03:01
Operator : CG/JU
Sample : PB148748BL
Misc :
ALS Vial : 66 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK748

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP102522.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST0.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc