

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP110222\
 Data File : BP012513.D
 Acq On : 04 Nov 2022 05:17
 Operator : CG/JU
 Sample : N5320-02
 Misc :
 ALS Vial : 70 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 BHAB4

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP102522.M
 Title : SVOA CALIBRATION

Signal : TIC: BP012513.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.028	4	7	27	rVB	227807	398871	4.00%	0.420%
2	3.228	37	41	46	rBV	60732	83783	0.84%	0.088%
3	3.658	112	114	129	rBV	351061	638084	6.39%	0.671%
4	3.864	145	149	155	rVB	24231	38145	0.38%	0.040%
5	3.964	161	166	172	rVB	23278	35330	0.35%	0.037%
6	5.087	349	357	367	rBV	141234	235878	2.36%	0.248%
7	5.411	408	412	420	rBV	19851	46496	0.47%	0.049%
8	5.493	420	426	431	rVB5	11835	18809	0.19%	0.020%
9	5.781	468	475	484	rVB	25638	45622	0.46%	0.048%
10	5.928	494	500	503	rBV8	6975	11140	0.11%	0.012%
11	6.046	514	520	525	rBV8	5714	11812	0.12%	0.012%
12	6.258	548	556	562	rBV2	14532	28823	0.29%	0.030%
13	6.446	583	588	595	rVB3	26811	43315	0.43%	0.046%
14	6.887	660	663	667	rVB5	8020	11278	0.11%	0.012%
15	6.958	667	675	687	rBV	270409	476311	4.77%	0.501%
16	7.116	695	702	716	rBV	1179888	1923552	19.27%	2.024%
17	7.311	727	735	749	rBV	1049311	1778964	17.82%	1.872%
18	7.422	750	754	759	rVB6	8390	13533	0.14%	0.014%
19	7.475	759	763	767	rBV4	13805	18521	0.19%	0.019%
20	7.775	805	814	830	rBV	1123131	1816589	18.20%	1.911%
21	7.881	830	832	839	rVV5	8443	15164	0.15%	0.016%
22	7.975	843	848	857	rVB3	32430	59917	0.60%	0.063%
23	8.140	869	876	879	rBV6	14296	28421	0.28%	0.030%
24	8.175	879	882	890	rVB2	15273	26537	0.27%	0.028%
25	8.416	917	923	930	rBV2	3795	10640	0.11%	0.011%
26	8.499	930	937	956	rBV	854446	1546058	15.49%	1.627%
27	8.775	978	984	991	rVB7	15588	28873	0.29%	0.030%
28	8.875	994	1001	1005	rBV5	13836	26271	0.26%	0.028%
29	8.946	1006	1013	1029	rBV	1415168	2436686	24.41%	2.564%
30	9.105	1035	1040	1048	rVB	9914	18979	0.19%	0.020%
31	9.216	1054	1059	1062	rBV6	7149	13177	0.13%	0.014%
32	9.328	1071	1078	1083	rVB10	9441	24270	0.24%	0.026%
33	9.405	1086	1091	1096	rVB6	8824	15584	0.16%	0.016%
34	9.563	1114	1118	1122	rBV6	9608	15145	0.15%	0.016%
35	9.610	1122	1126	1128	rVV	10827	16533	0.17%	0.017%
36	9.663	1128	1135	1152	rVB2	1208370	2165229	21.69%	2.278%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP110222\
 Data File : BP012513.D
 Acq On : 04 Nov 2022 05:17
 Operator : CG/JU
 Sample : N5320-02
 Misc :
 ALS Vial : 70 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 BHAB4

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP102522.M
 Title : SVOA CALIBRATION

37	9.822	1158	1162	1168	rVB9	10477	16482	0.17%	0.017%
38	9.969	1179	1187	1189	rBV7	8205	17004	0.17%	0.018%
39	10.110	1210	1211	1219	rVB8	7153	11378	0.11%	0.012%
40	10.205	1219	1227	1240	rBV	1705449	3059589	30.65%	3.219%
41	10.393	1253	1259	1270	rVB3	29760	64640	0.65%	0.068%
42	10.575	1282	1290	1301	rBV	1780475	2986636	29.92%	3.142%
43	10.669	1301	1306	1309	rVV2	48158	77196	0.77%	0.081%
44	10.728	1309	1316	1335	rVB	1656526	3131911	31.38%	3.295%
45	10.987	1358	1360	1366	rVB7	10723	18406	0.18%	0.019%
46	11.181	1388	1393	1398	rBV7	12370	22801	0.23%	0.024%
47	11.275	1401	1409	1417	rBV	27962	58469	0.59%	0.062%
48	11.787	1490	1496	1507	rVB10	13078	34674	0.35%	0.036%
49	11.934	1510	1521	1528	rBV	72152	148109	1.48%	0.156%
50	12.169	1556	1561	1567	rBV	30046	55327	0.55%	0.058%
51	12.399	1591	1600	1603	rBV	8432	20626	0.21%	0.022%
52	12.551	1622	1626	1629	rBV6	9273	13458	0.13%	0.014%
53	12.951	1688	1694	1702	rBV	128102	227920	2.28%	0.240%
54	13.028	1702	1707	1709	rVV6	8746	14762	0.15%	0.016%
55	13.063	1709	1713	1724	rVB	40975	72042	0.72%	0.076%
56	13.287	1745	1751	1755	rBV	63261	101186	1.01%	0.106%
57	13.393	1766	1769	1775	rVB3	6991	10491	0.11%	0.011%
58	13.557	1795	1797	1803	rVB6	7743	11299	0.11%	0.012%
59	13.710	1820	1823	1826	rBV5	7135	10909	0.11%	0.011%
60	13.846	1839	1846	1855	rBV	3496354	5057837	50.67%	5.322%
61	13.910	1855	1857	1861	rVB	24946	33238	0.33%	0.035%
62	14.122	1886	1893	1907	rVV	4093409	6081768	60.93%	6.399%
63	14.222	1907	1910	1921	rVB2	20706	44511	0.45%	0.047%
64	14.428	1938	1945	1960	rBV	3001624	4487292	44.95%	4.721%
65	14.557	1964	1967	1973	rBV	8553	14918	0.15%	0.016%
66	14.675	1981	1987	1992	rBV	111197	255445	2.56%	0.269%
67	15.187	2070	2074	2077	rBV2	7889	12260	0.12%	0.013%
68	15.428	2108	2115	2129	rVV	5387608	7818183	78.32%	8.226%
69	15.563	2132	2138	2152	rVV	1370513	2051694	20.55%	2.159%
70	15.669	2152	2156	2158	rVV2	31546	53233	0.53%	0.056%
71	15.698	2158	2161	2165	rVB	46263	60656	0.61%	0.064%
72	15.945	2197	2203	2213	rBV2	75402	155236	1.56%	0.163%
73	16.075	2216	2225	2230	rVV	38578	78998	0.79%	0.083%
74	16.157	2234	2239	2241	rVV5	25258	47849	0.48%	0.050%
75	16.192	2241	2245	2253	rVB2	46117	88292	0.88%	0.093%
76	16.492	2290	2296	2302	rBV9	22682	47598	0.48%	0.050%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP110222\
 Data File : BP012513.D
 Acq On : 04 Nov 2022 05:17
 Operator : CG/JU
 Sample : N5320-02
 Misc :
 ALS Vial : 70 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 BHAB4

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP102522.M
 Title : SVOA CALIBRATION

77	16.869	2355	2360	2366	rVB9	16869	26932	0.27%	0.028%
78	17.192	2404	2415	2425	rBV	3801096	5797912	58.08%	6.100%
79	17.292	2425	2432	2448	rVV2	5741306	8793494	88.09%	9.252%
80	17.722	2502	2505	2513	rVB3	23112	37901	0.38%	0.040%
81	18.081	2562	2566	2575	rBV3	70726	113905	1.14%	0.120%
82	18.234	2588	2592	2596	rBV	62978	80854	0.81%	0.085%
83	18.328	2605	2608	2611	rBV	38369	49495	0.50%	0.052%
84	18.375	2613	2616	2622	rVB	95031	137245	1.37%	0.144%
85	19.110	2737	2741	2746	rBV	85050	116332	1.17%	0.122%
86	19.175	2749	2752	2757	rVV	68896	101029	1.01%	0.106%
87	19.322	2773	2777	2782	rBV3	53421	87768	0.88%	0.092%
88	19.533	2807	2813	2819	rBV	7523027	9981917	100.00%	10.503%
89	19.586	2819	2822	2828	rVB	129466	194447	1.95%	0.205%
90	21.286	3106	3111	3121	rBV	4324765	5601582	56.12%	5.894%
91	23.516	3483	3490	3504	rVB2	4021415	8415578	84.31%	8.855%
92	23.669	3509	3516	3528	rVB2	2325352	4808380	48.17%	5.059%


Sum of corrected areas: 95041434

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP110222\
Data File : BP012513.D
Acq On : 04 Nov 2022 05:17
Operator : CG/JU
Sample : N5320-02
Misc :
ALS Vial : 70 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
BHAB4

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP102522.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

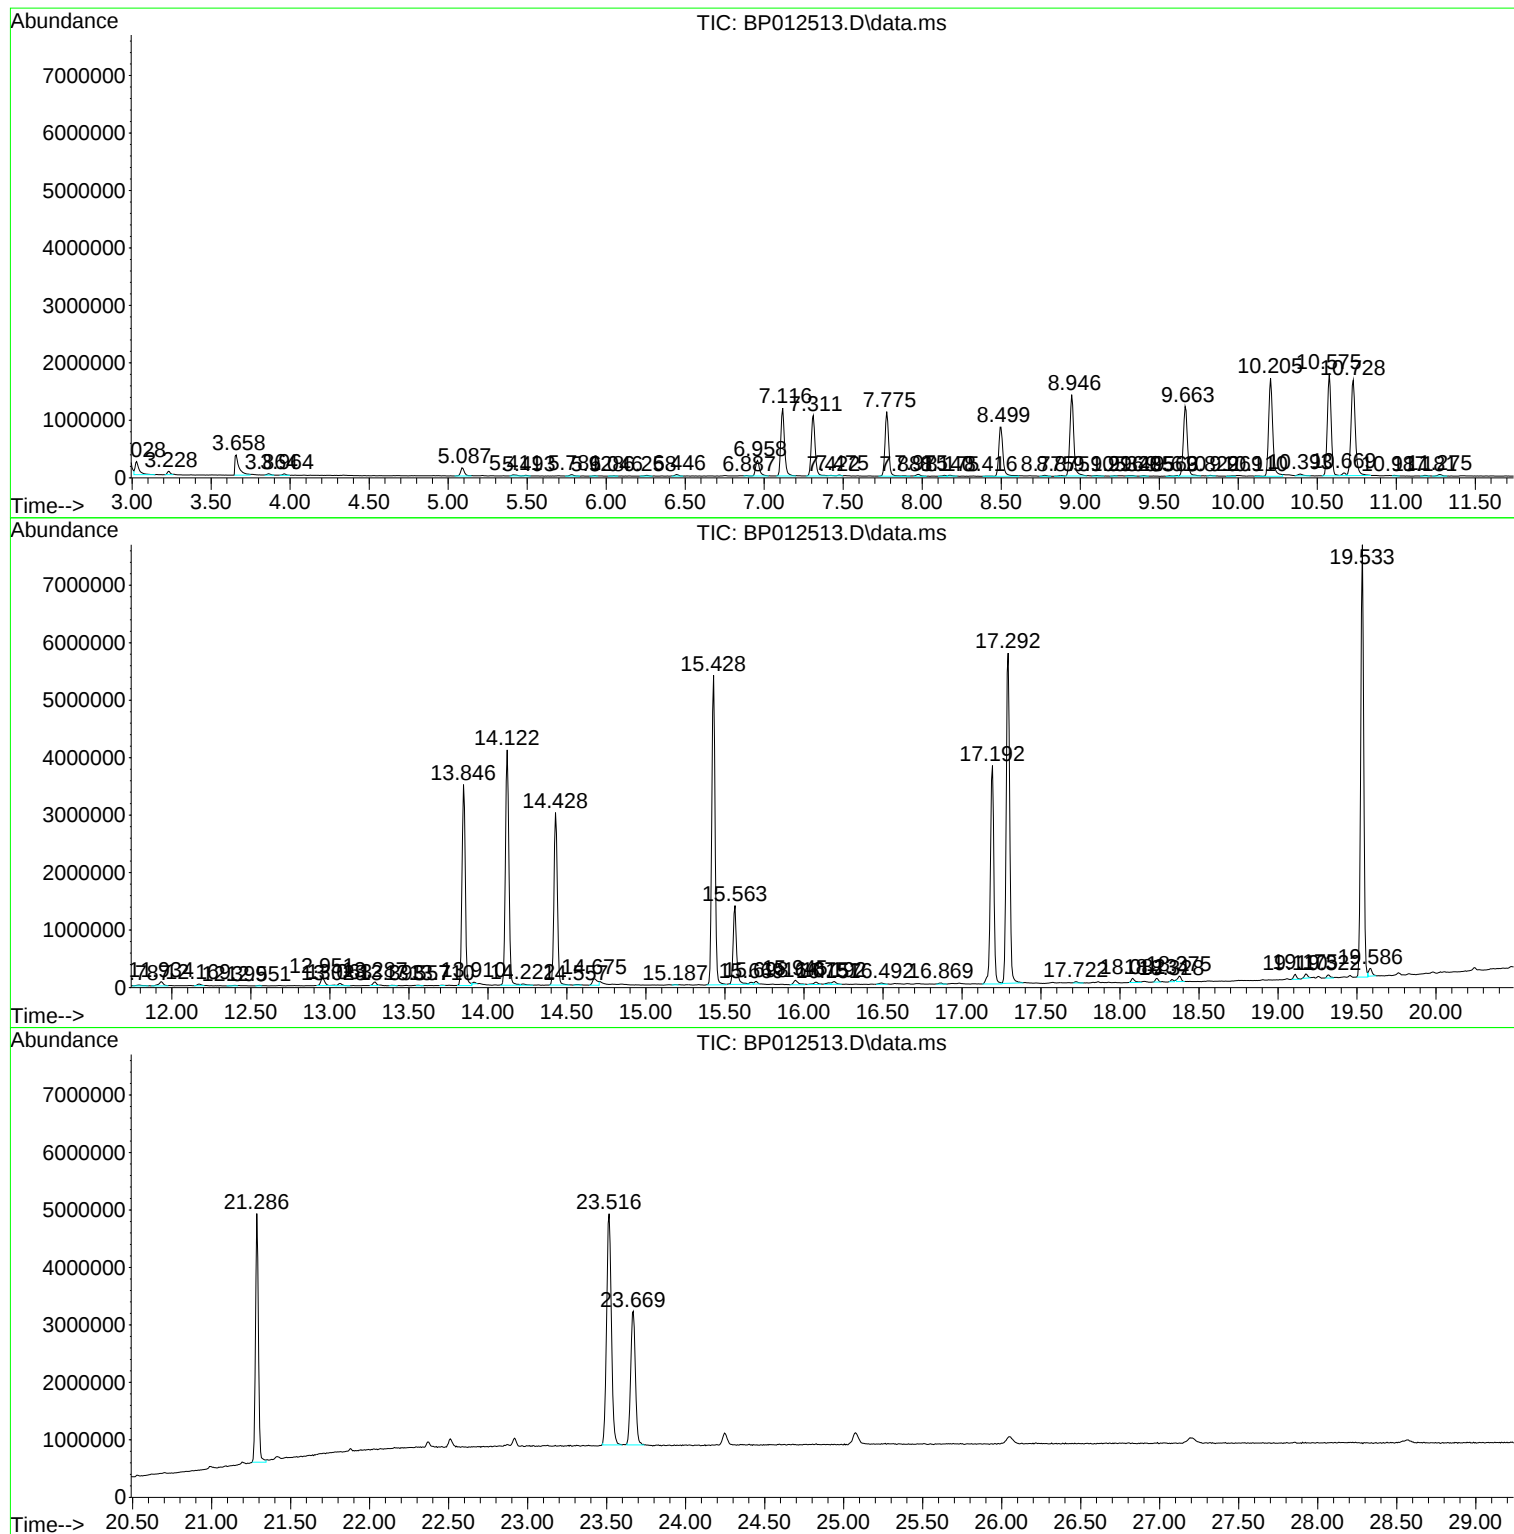

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP110222\
Data File : BP012513.D
Acq On : 04 Nov 2022 05:17
Operator : CG/JU
Sample : N5320-02
Misc :
ALS Vial : 70 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
BHAB4










Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP102522.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 Triethylamine Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
3.028	4.39 ng/ul	398871	1,4-Dichlorobenzene-d4	7.775

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			Triethylamine	101	C6H15N	000121-44-8	91
2			Triethylamine	101	C6H15N	000121-44-8	91
3			Triethylamine	101	C6H15N	000121-44-8	91
4			Triethylamine	101	C6H15N	000121-44-8	91
5			Triethylamine	101	C6H15N	000121-44-8	83

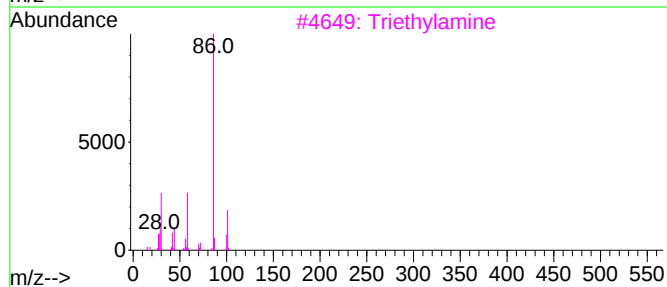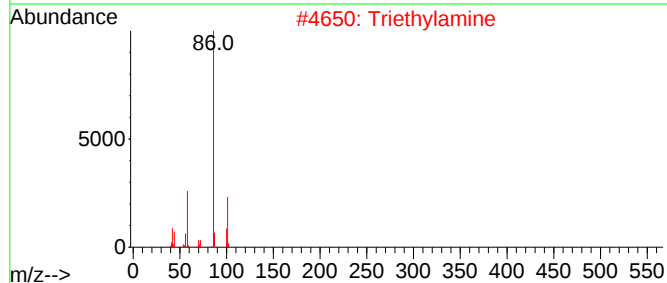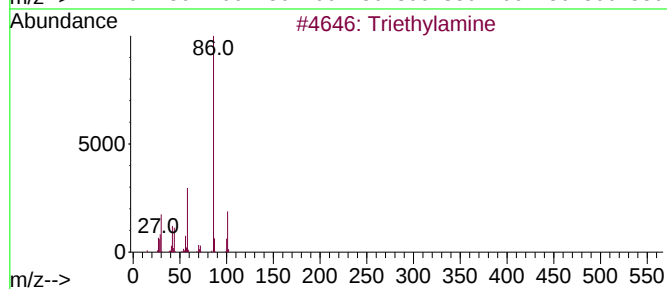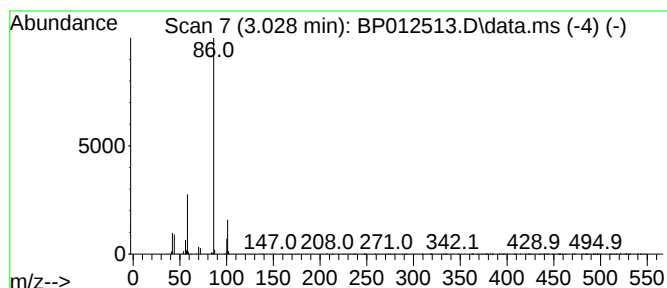

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP110222\
Data File : BP012513.D
Acq On : 04 Nov 2022 05:17
Operator : CG/JU
Sample : N5320-02
Misc :
ALS Vial : 70 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
BHAB4

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP102522.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
Triethylamine	3.028	4.4	ng/u1	398871	1	7.775	1816590	20.0