

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP110222\
 Data File : BP012514.D
 Acq On : 04 Nov 2022 05:52
 Operator : CG/JU
 Sample : N5320-03
 Misc :
 ALS Vial : 71 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 BHAB5

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP102522.M
 Title : SVOA CALIBRATION

Signal : TIC: BP012514.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.023	3	6	25	rVB	638023	1006979	9.77%	0.976%
2	3.228	37	41	46	rBV	59972	81705	0.79%	0.079%
3	3.658	111	114	130	rBV	353606	644590	6.25%	0.625%
4	3.864	145	149	154	rVB	22680	32486	0.32%	0.031%
5	3.964	162	166	174	rVB	26359	43647	0.42%	0.042%
6	5.087	352	357	369	rBV	439817	692474	6.72%	0.671%
7	5.417	406	413	414	rBV2	30410	45835	0.44%	0.044%
8	5.434	414	416	422	rVV	37418	49003	0.48%	0.047%
9	5.487	422	425	434	rVB5	14683	24161	0.23%	0.023%
10	5.781	470	475	480	rBV3	14120	24855	0.24%	0.024%
11	6.258	546	556	563	rBV	99531	168109	1.63%	0.163%
12	6.446	583	588	595	rVB2	40766	67684	0.66%	0.066%
13	6.752	634	640	645	rBV	31666	54213	0.53%	0.053%
14	6.958	668	675	685	rVV	289423	544845	5.28%	0.528%
15	7.034	685	688	694	rVB2	21952	33097	0.32%	0.032%
16	7.116	695	702	714	rBV	1110807	1887832	18.31%	1.829%
17	7.211	714	718	723	rVB2	16777	28013	0.27%	0.027%
18	7.311	728	735	749	rBV	1061585	1817443	17.62%	1.761%
19	7.416	749	753	759	rVV2	26782	40089	0.39%	0.039%
20	7.475	759	763	768	rVB	18140	25596	0.25%	0.025%
21	7.663	787	795	803	rVB9	13881	33544	0.33%	0.033%
22	7.775	803	814	827	rBV	1215261	2026775	19.65%	1.964%
23	7.881	827	832	838	rVB	39426	65540	0.64%	0.064%
24	7.969	843	847	856	rVB3	42162	69818	0.68%	0.068%
25	8.140	868	876	881	rBV2	63864	137219	1.33%	0.133%
26	8.493	929	936	948	rBV	889258	1569549	15.22%	1.521%
27	8.775	979	984	990	rVB8	12959	24580	0.24%	0.024%
28	8.875	996	1001	1006	rBV2	29038	47863	0.46%	0.046%
29	8.946	1006	1013	1033	rVV	1365571	2413957	23.41%	2.339%
30	9.093	1033	1038	1049	rVV	89364	162599	1.58%	0.158%
31	9.216	1053	1059	1066	rVV7	12846	28943	0.28%	0.028%
32	9.328	1069	1078	1084	rVV5	20826	48313	0.47%	0.047%
33	9.399	1084	1090	1097	rVV2	21029	39688	0.38%	0.038%
34	9.569	1114	1119	1122	rBV5	15002	25648	0.25%	0.025%
35	9.663	1128	1135	1150	rVV	1108326	1939648	18.81%	1.879%
36	9.822	1157	1162	1172	rVB8	25267	51806	0.50%	0.050%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP110222\
 Data File : BP012514.D
 Acq On : 04 Nov 2022 05:52
 Operator : CG/JU
 Sample : N5320-03
 Misc :
 ALS Vial : 71 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 BHAB5

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP102522.M
 Title : SVOA CALIBRATION

37	9.993	1179	1191	1200	rBV9	32133	115917	1.12%	0.112%
38	10.205	1219	1227	1238	rBV	1694689	3009702	29.19%	2.916%
39	10.369	1249	1255	1271	rVB2	105313	284897	2.76%	0.276%
40	10.516	1275	1280	1283	rBV6	12466	24382	0.24%	0.024%
41	10.575	1283	1290	1301	rVV	1945362	3260424	31.62%	3.159%
42	10.669	1301	1306	1309	rVV	85946	140075	1.36%	0.136%
43	10.728	1309	1316	1336	rVB	1603176	3096527	30.03%	3.000%
44	11.181	1388	1393	1402	rVV3	27373	53733	0.52%	0.052%
45	11.269	1402	1408	1419	rVB3	14720	41611	0.40%	0.040%
46	11.610	1459	1466	1472	rBV10	11714	28490	0.28%	0.028%
47	11.793	1490	1497	1500	rBV7	12555	24664	0.24%	0.024%
48	11.928	1511	1520	1528	rBV	223448	419250	4.07%	0.406%
49	12.169	1557	1561	1567	rVV3	29720	52589	0.51%	0.051%
50	12.393	1592	1599	1607	rBV9	18254	51336	0.50%	0.050%
51	12.969	1690	1697	1701	rVV2	41470	93631	0.91%	0.091%
52	13.022	1703	1706	1709	rVV3	18797	28285	0.27%	0.027%
53	13.063	1710	1713	1723	rVB2	16148	31575	0.31%	0.031%
54	13.281	1746	1750	1752	rVV4	18113	25303	0.25%	0.025%
55	13.322	1752	1757	1764	rVV	76246	120993	1.17%	0.117%
56	13.481	1780	1784	1788	rVB	19391	24844	0.24%	0.024%
57	13.846	1839	1846	1860	rBV	3459258	4983354	48.33%	4.828%
58	14.122	1883	1893	1907	rBV	3880452	5780926	56.06%	5.601%
59	14.222	1907	1910	1918	rVB2	25498	52420	0.51%	0.051%
60	14.428	1937	1945	1965	rVB	3270314	5010756	48.59%	4.855%
61	14.669	1980	1986	2002	rBV2	150575	418564	4.06%	0.406%
62	15.187	2070	2074	2078	rVV	20878	26944	0.26%	0.026%
63	15.275	2083	2089	2093	rBV2	79585	109992	1.07%	0.107%
64	15.334	2095	2099	2104	rVB6	15222	23345	0.23%	0.023%
65	15.428	2108	2115	2129	rBV	5322688	7996086	77.54%	7.747%
66	15.563	2132	2138	2148	rVV	1479681	2199297	21.33%	2.131%
67	15.663	2151	2155	2157	rVV2	61250	98727	0.96%	0.096%
68	15.698	2157	2161	2171	rVB	231522	353868	3.43%	0.343%
69	15.951	2198	2204	2211	rBV4	72157	154852	1.50%	0.150%
70	16.139	2232	2236	2245	rBV3	194924	347750	3.37%	0.337%
71	16.492	2289	2296	2302	rBV4	86569	170513	1.65%	0.165%
72	16.863	2355	2359	2363	rBV6	12673	22567	0.22%	0.022%
73	16.939	2367	2372	2376	rBV	96075	127886	1.24%	0.124%
74	17.157	2404	2409	2410	rBV	361117	443829	4.30%	0.430%
75	17.192	2410	2415	2425	rVV	4167733	6107311	59.23%	5.917%
76	17.292	2425	2432	2444	rVV	5866357	8783059	85.17%	8.510%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP110222\
 Data File : BP012514.D
 Acq On : 04 Nov 2022 05:52
 Operator : CG/JU
 Sample : N5320-03
 Misc :
 ALS Vial : 71 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 BHAB5

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP102522.M
 Title : SVOA CALIBRATION

77	17.557	2474	2477	2491	rVB9	26562	64927	0.63%	0.063%
78	17.681	2494	2498	2502	rBV	69287	90739	0.88%	0.088%
79	17.828	2519	2523	2526	rBV	54602	79352	0.77%	0.077%
80	17.857	2526	2528	2531	rVB2	37091	43277	0.42%	0.042%
81	18.081	2562	2566	2575	rBV	125898	205784	2.00%	0.199%
82	18.157	2576	2579	2585	rVB2	49251	62280	0.60%	0.060%
83	18.233	2588	2592	2601	rVB	107396	144120	1.40%	0.140%
84	18.328	2605	2608	2610	rVV	88902	109787	1.06%	0.106%
85	18.375	2610	2616	2623	rVB2	189837	397470	3.85%	0.385%
86	18.751	2677	2680	2684	rBV6	22090	33767	0.33%	0.033%
87	18.898	2702	2705	2710	rBV2	52506	74146	0.72%	0.072%
88	19.110	2737	2741	2746	rBV2	103329	142514	1.38%	0.138%
89	19.175	2749	2752	2756	rBV	77195	109572	1.06%	0.106%
90	19.257	2763	2766	2772	rVB5	66280	74883	0.73%	0.073%
91	19.316	2773	2776	2784	rBV3	92071	142332	1.38%	0.138%
92	19.533	2807	2813	2819	rBV	7524863	10311833	100.00%	9.991%
93	19.580	2819	2821	2831	rVB	205621	289830	2.81%	0.281%
94	20.386	2956	2958	2962	rVB2	65588	71046	0.69%	0.069%
95	20.528	2979	2982	2987	rBV3	111321	128624	1.25%	0.125%
96	20.992	3058	3061	3067	rBV3	168596	253609	2.46%	0.246%
97	21.286	3106	3111	3119	rBV	4704896	6026714	58.44%	5.839%
98	22.510	3316	3319	3326	rVB2	307554	486428	4.72%	0.471%
99	23.516	3483	3490	3500	rVB2	4113121	8526255	82.68%	8.261%
100	23.669	3509	3516	3527	rVB2	2540508	5201761	50.44%	5.040%




Sum of corrected areas: 103209470

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP110222\
Data File : BP012514.D
Acq On : 04 Nov 2022 05:52
Operator : CG/JU
Sample : N5320-03
Misc :
ALS Vial : 71 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
BHAB5

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP102522.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

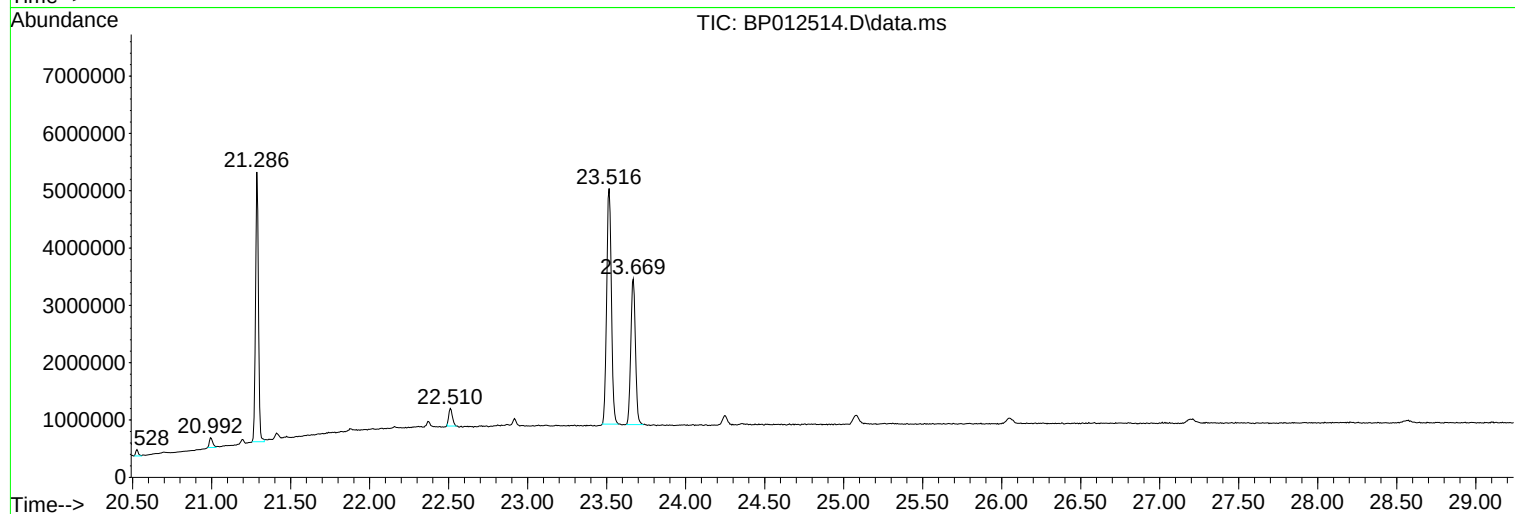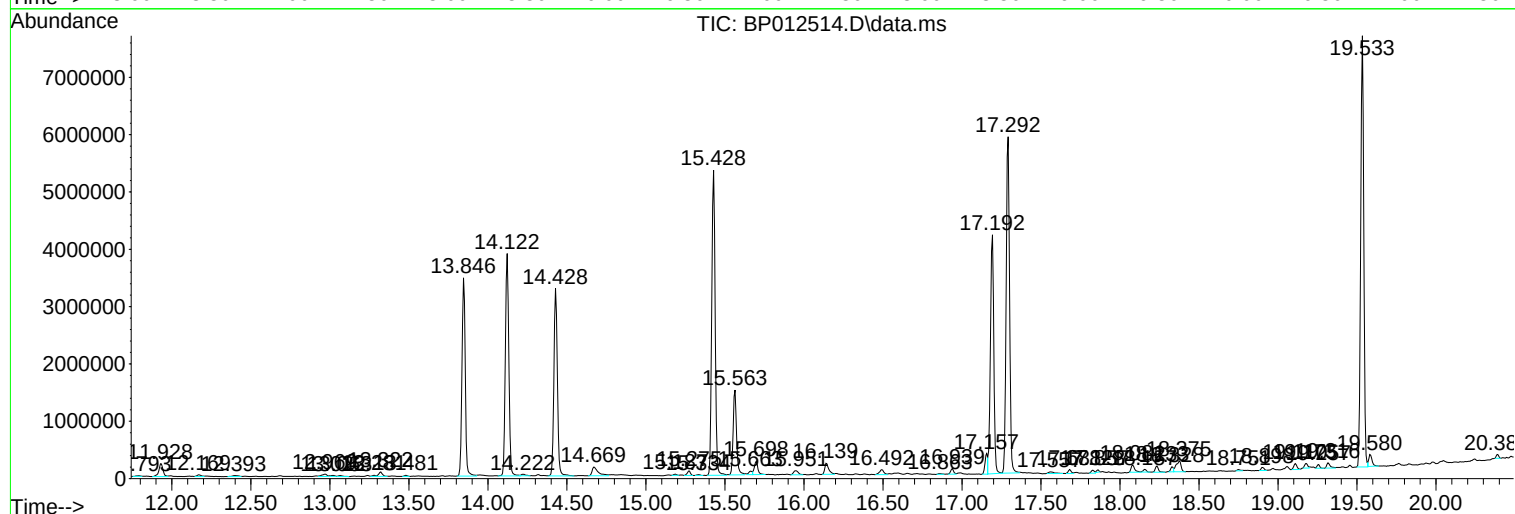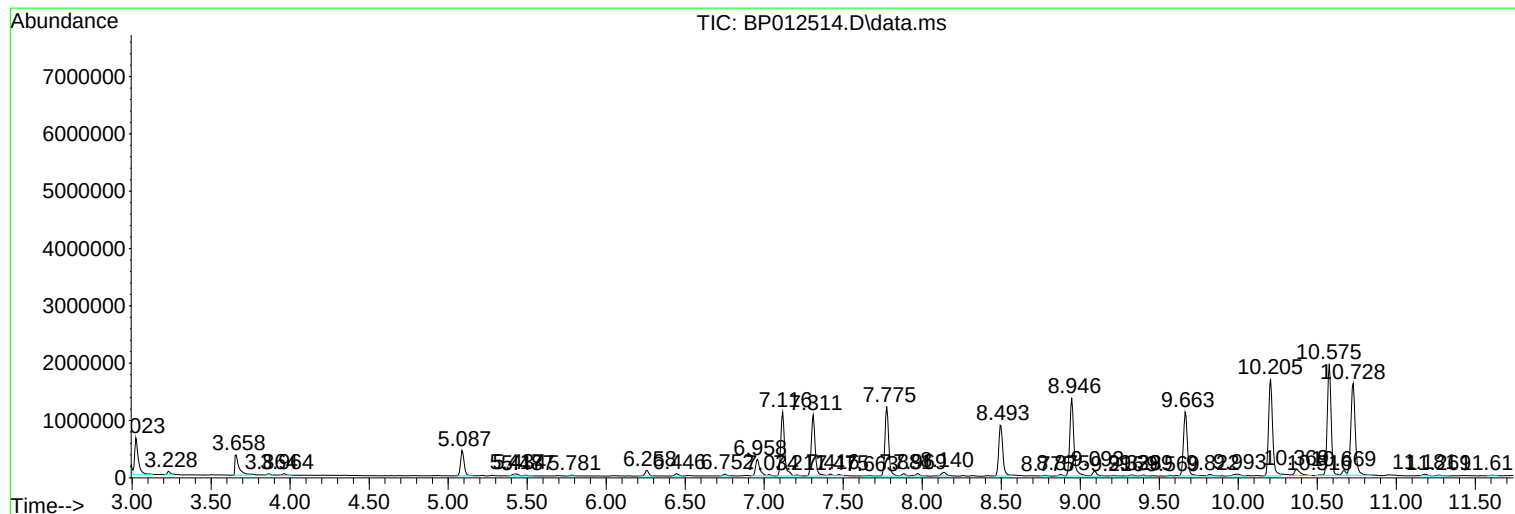

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP110222\
Data File : BP012514.D
Acq On : 04 Nov 2022 05:52
Operator : CG/JU
Sample : N5320-03
Misc :
ALS Vial : 71 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
BHAB5










Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP102522.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 Triethylamine Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
3.023	9.94 ng/ul	1006980	1,4-Dichlorobenzene-d4	7.775

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			Triethylamine	101	C6H15N	000121-44-8	91
2			Triethylamine	101	C6H15N	000121-44-8	91
3			Triethylamine	101	C6H15N	000121-44-8	91
4			Tetraethylammonium chloride	165	C8H20ClN	000056-34-8	83
5			1,2-Ethanediamine, N,N-diethyl-	116	C6H16N2	000100-36-7	72

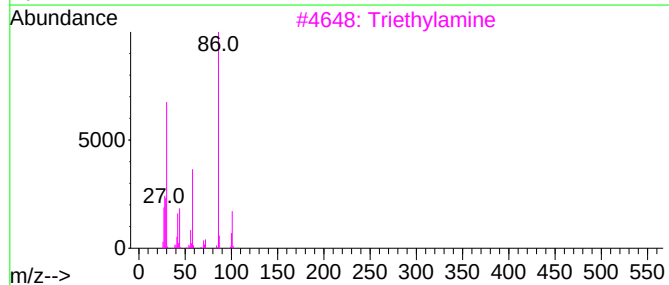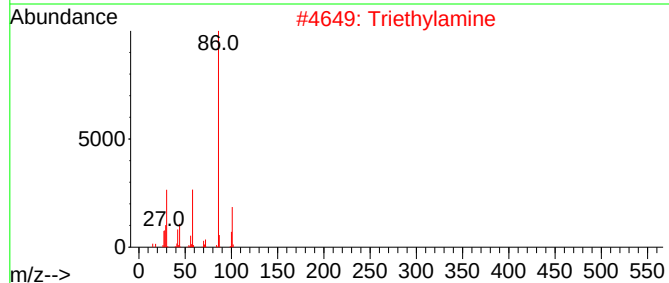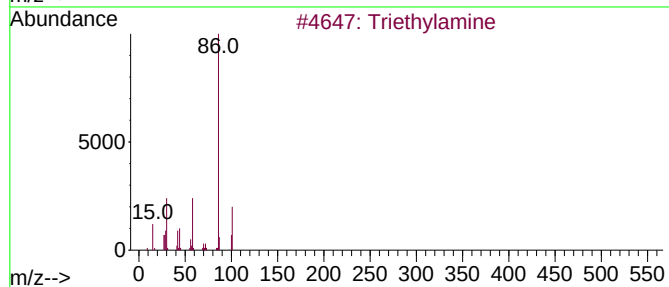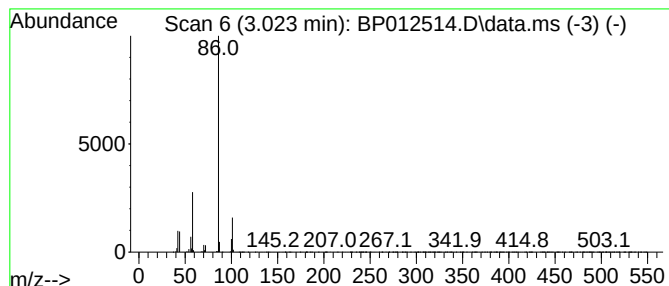

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP110222\
Data File : BP012514.D
Acq On : 04 Nov 2022 05:52
Operator : CG/JU
Sample : N5320-03
Misc :
ALS Vial : 71 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
BHAB5










Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP102522.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 3 Phenol, p-tert-butyl- Concentration Rank 3

R.T.	EstConc	Area	Relative to ISTD	R.T.
11.928	2.57 ng/ul	419250	Naphthalene-d8	10.575

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			Phenol, p-tert-butyl-	150	C10H14O	000098-54-4	97
2			Phenol, p-tert-butyl-	150	C10H14O	000098-54-4	94
3			Phenol, m-tert-butyl-	150	C10H14O	000585-34-2	91
4			Phenol, m-tert-butyl-	150	C10H14O	000585-34-2	91
5			Phenol, m-tert-butyl-	150	C10H14O	000585-34-2	91

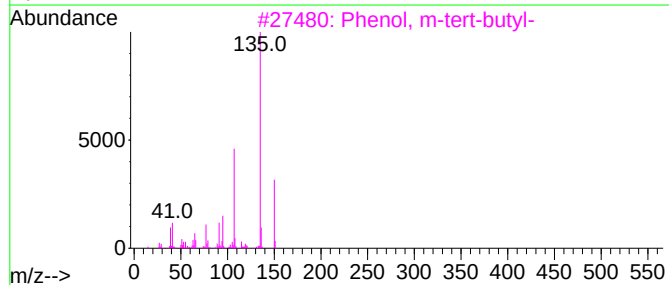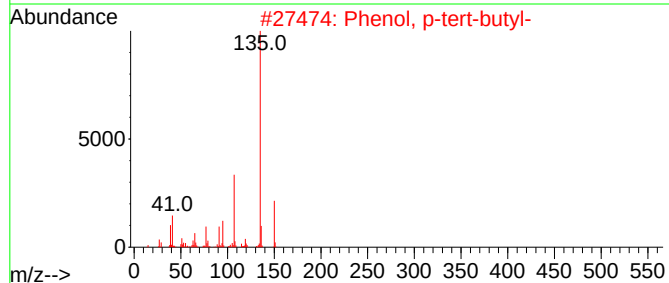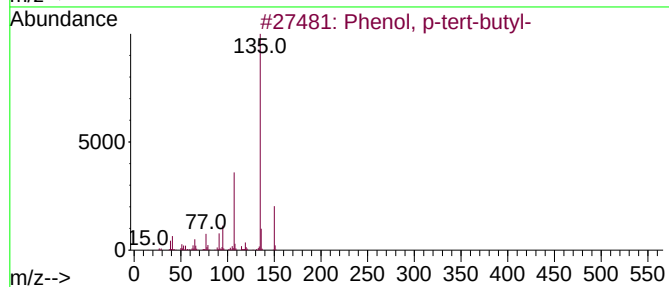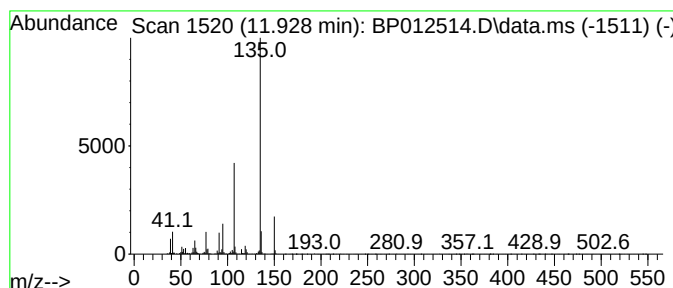

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP110222\
Data File : BP012514.D
Acq On : 04 Nov 2022 05:52
Operator : CG/JU
Sample : N5320-03
Misc :
ALS Vial : 71 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
BHAB5

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP102522.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST0.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
Triethylamine	3.023	9.9	ng/ul	1006980	1	7.775	2026780	20.0
Phenol, p-tert-...	11.928	2.6	ng/ul	419250	2	10.575	3260420	20.0